

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096982.D
 Acq On : 18 Jul 2018 6:29
 Operator : SJ/JU
 Sample : J3967-06DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jul 18 07:58:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 07:15:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	1990	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	10323	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	6306	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	18311	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	25137	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	26708	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.74	152	1226	0.07	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	4057	0.07	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.43	266	13626	6.583	ng/ul	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096982.D
Acq On : 18 Jul 2018 6:29
Operator : SJ/JU
Sample : J3967-06DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jul 18 07:58:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 07:15:45 2018
Response via : Initial Calibration

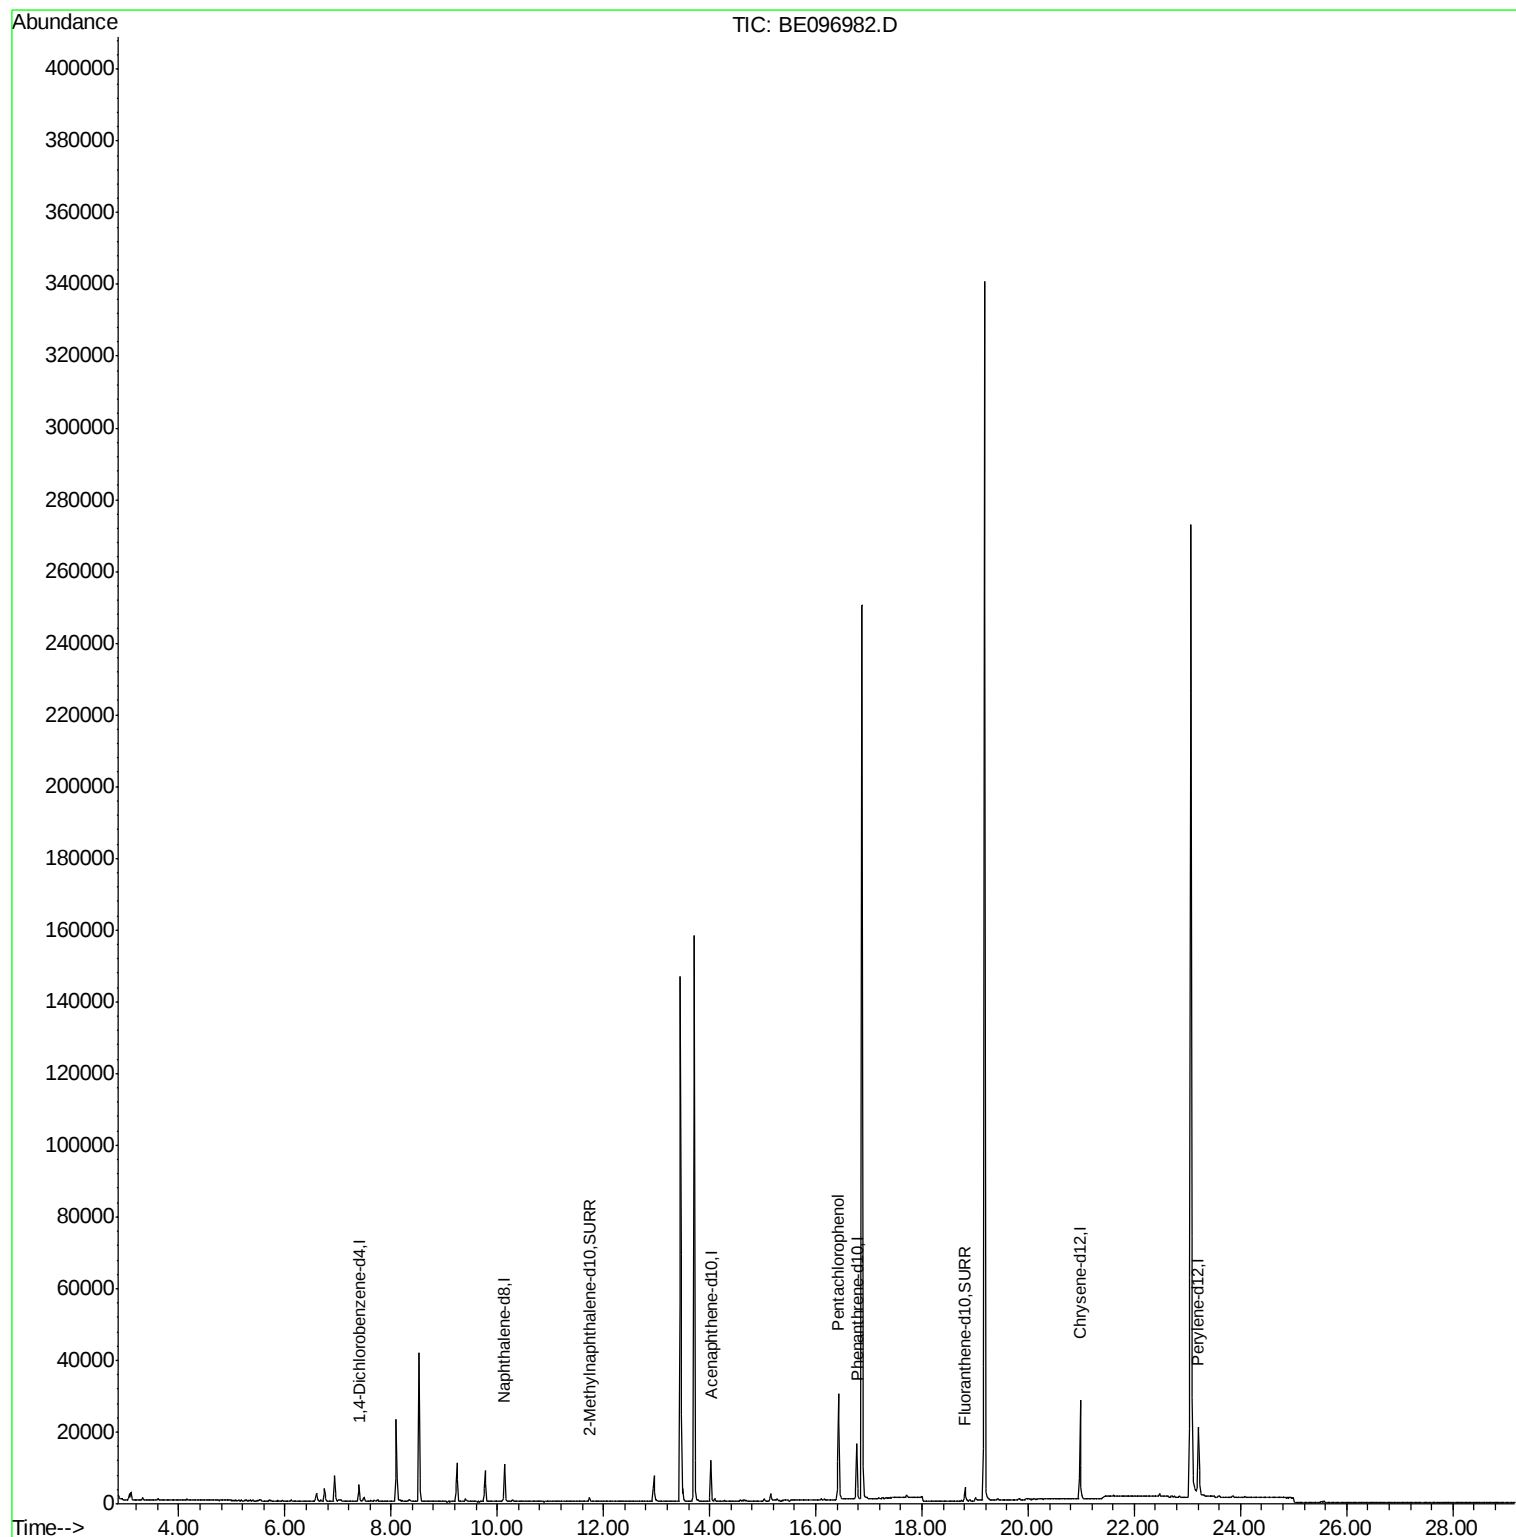

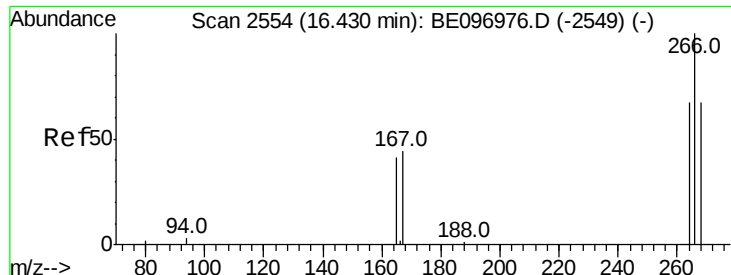

#11

Pentachlorophenol

Concen: 6.583 ng/ul

RT: 16.43 min Scan# 2553

Delta R.T. 0.00 min

Lab File: BE096982.D

Acq: 18 Jul 2018 6:29

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 266 Resp: 13626

Ion Ratio Lower Upper

266 100

264 62.8 47.9 71.9

268 63.6 49.8 74.8

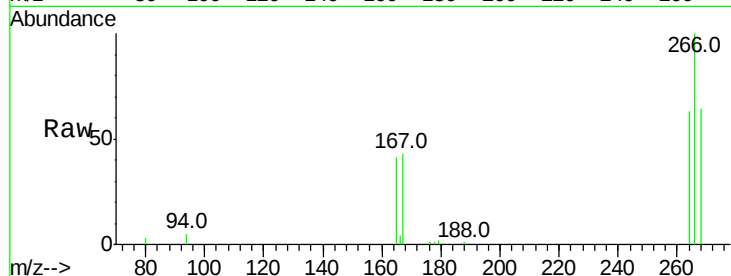

Abundance

Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

