

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:13:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

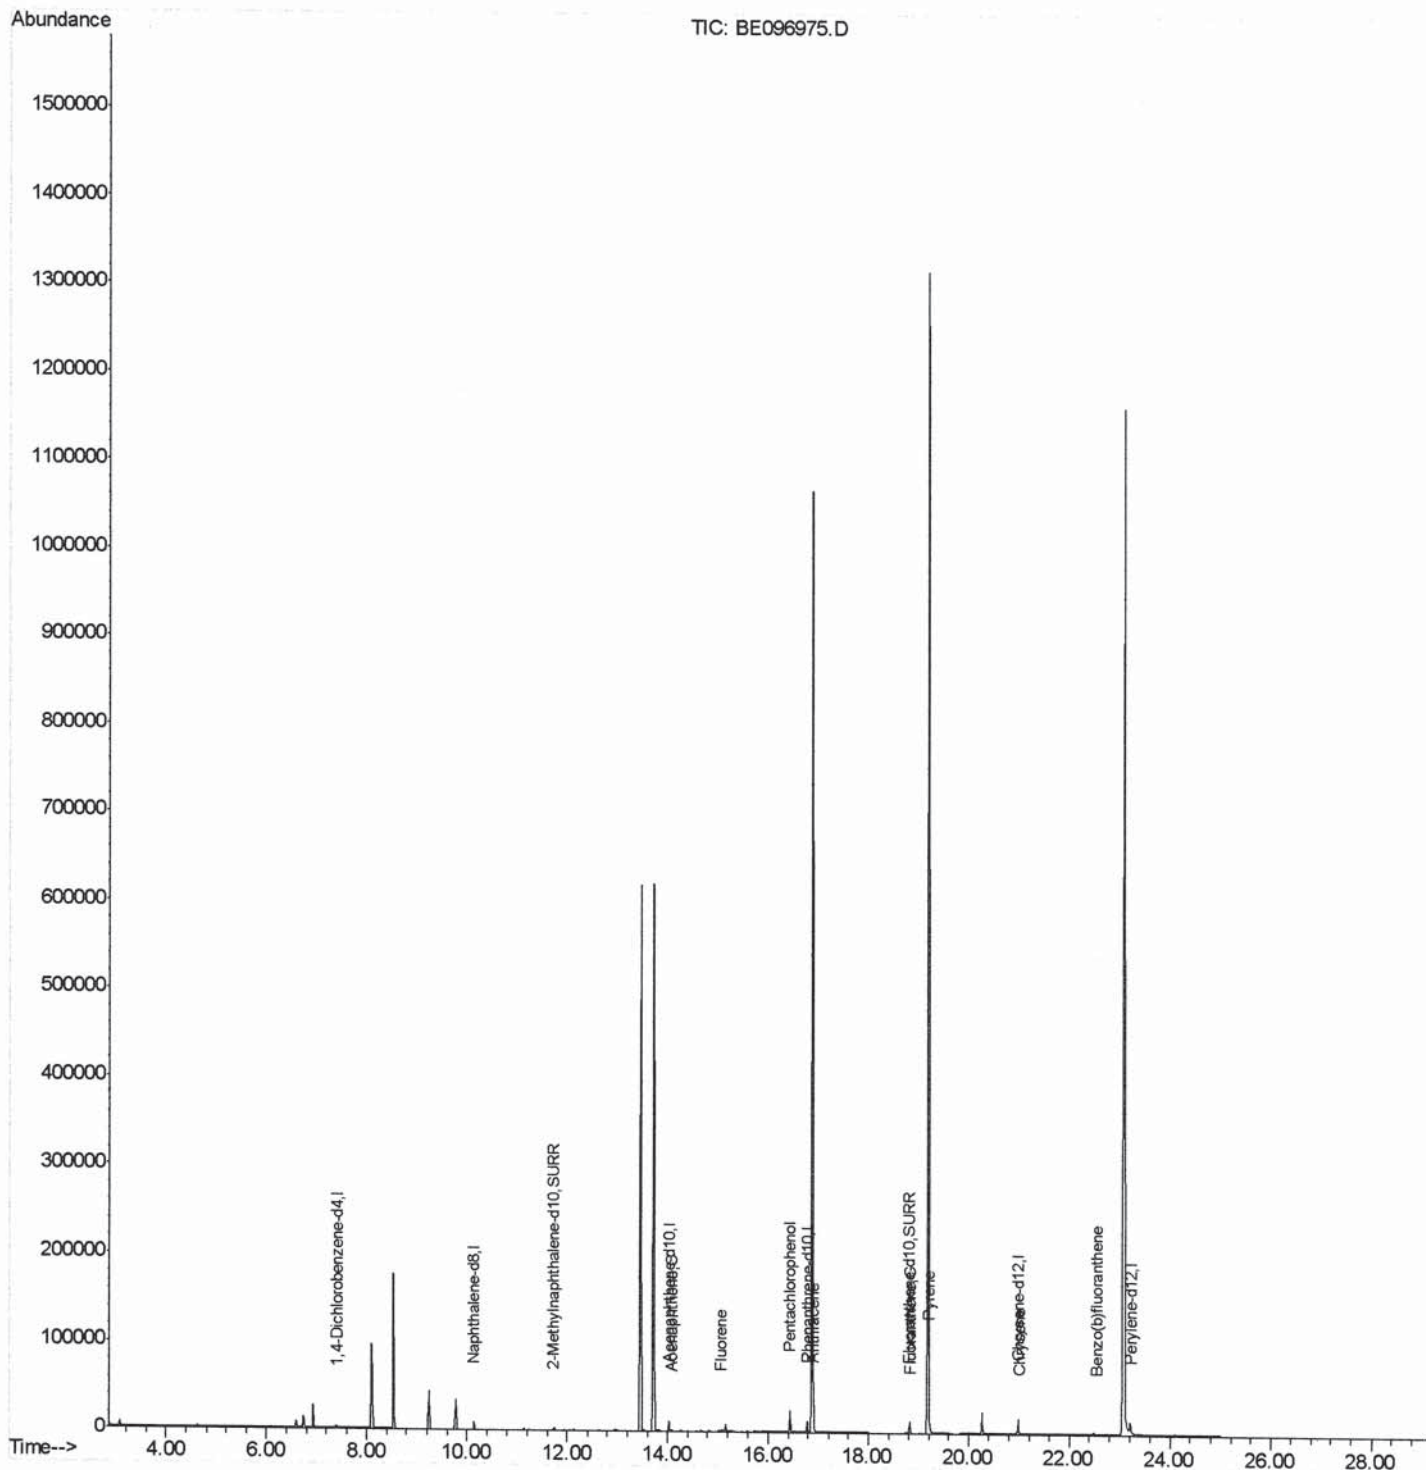

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

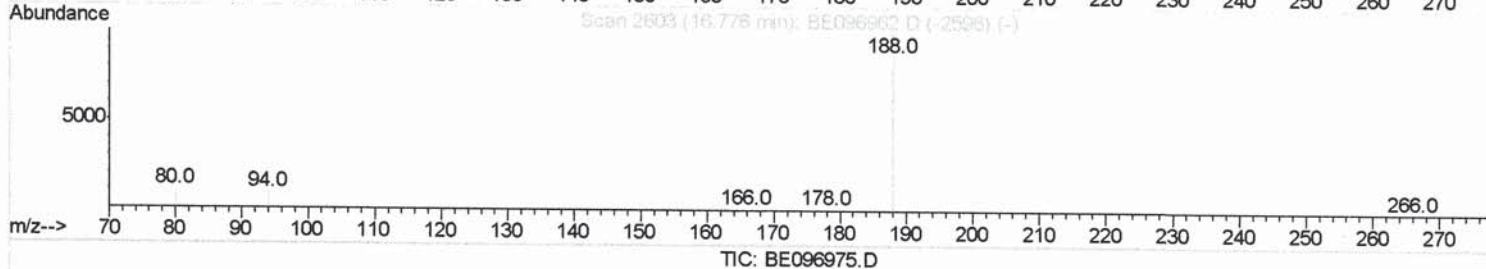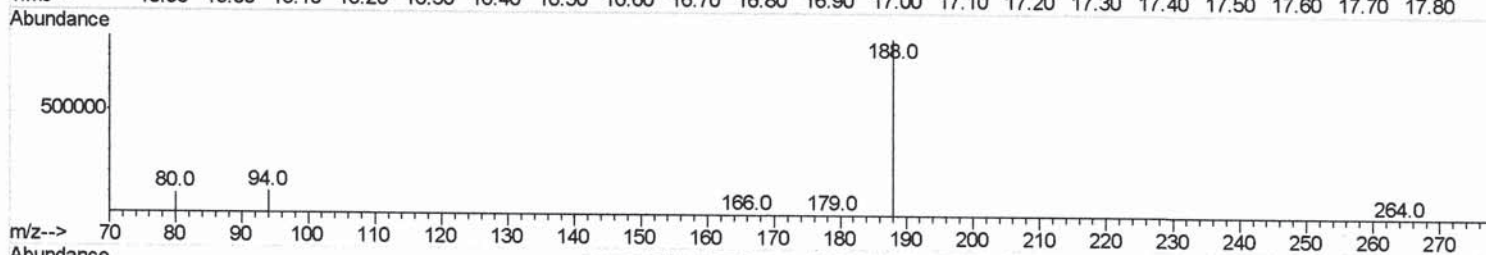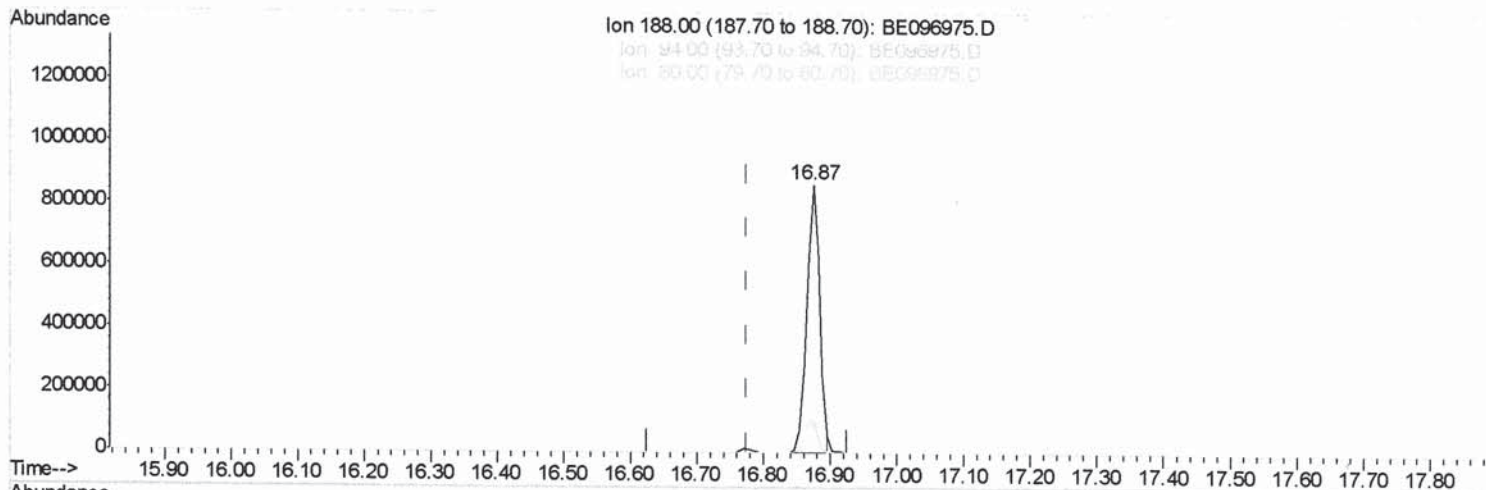

(10) Phenanthrene-d10 (I)

16.874min (+0.098) 0.40ng/ul

response 1169558

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.30
80.00	11.80	11.18
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

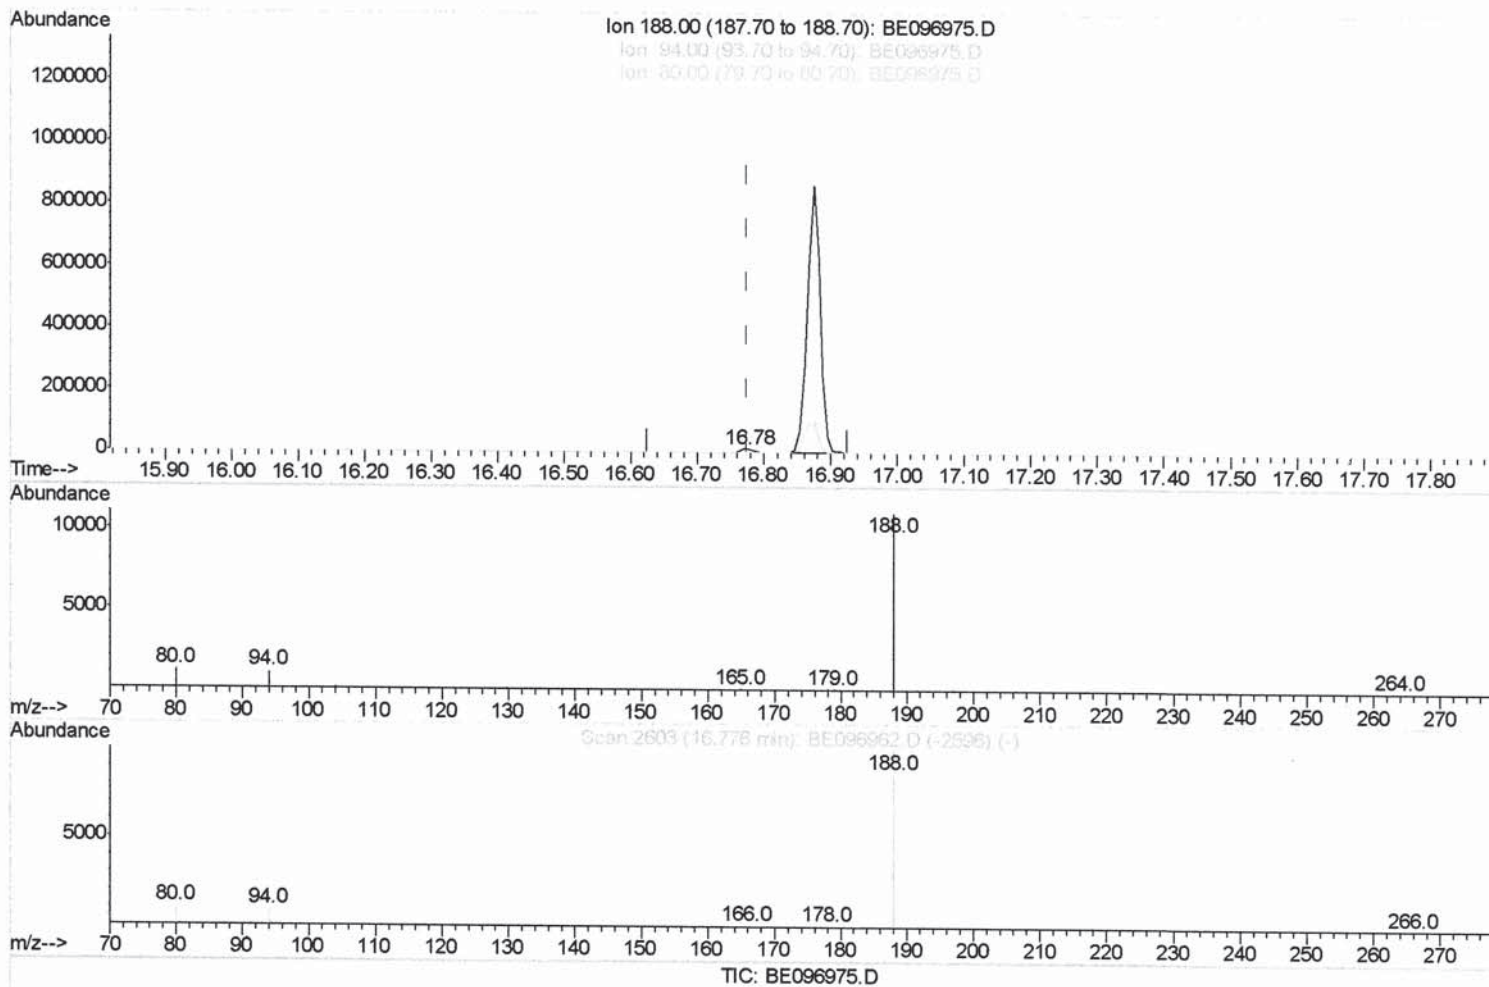

(10) Phenanthrene-d10 (I)

16.775min (-0.000) 0.40ng/ul m

response 15830

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.51
80.00	11.80	10.45
0.00	0.00	0.00

SJ 7/19/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

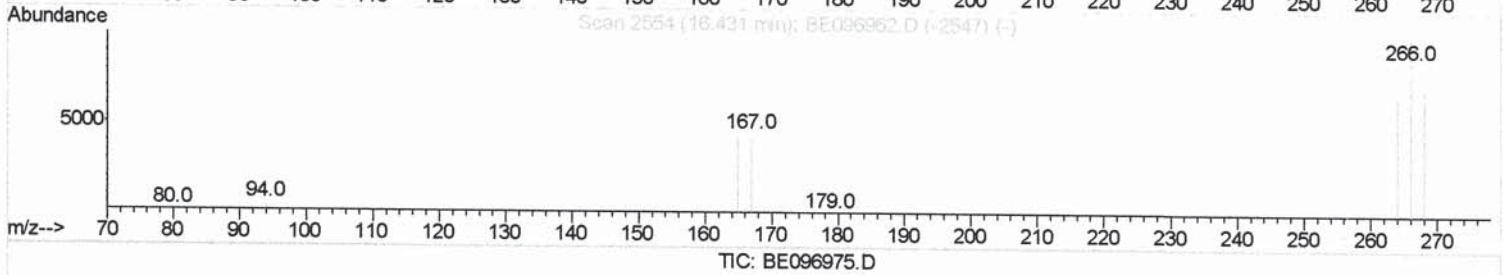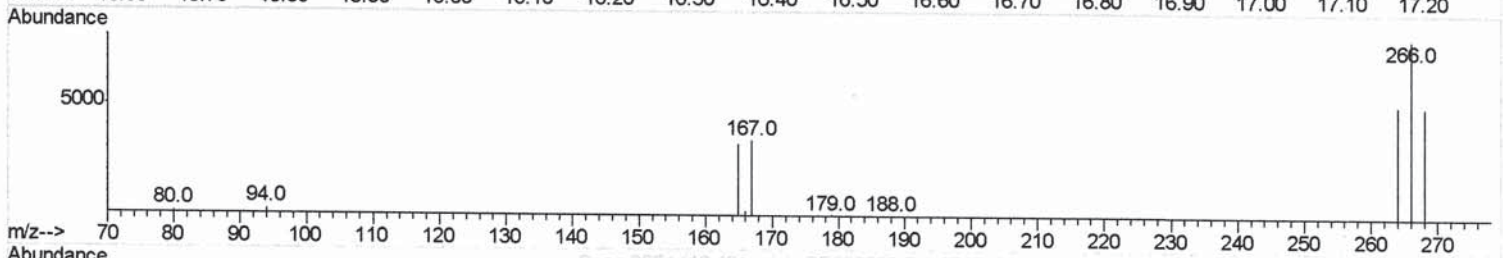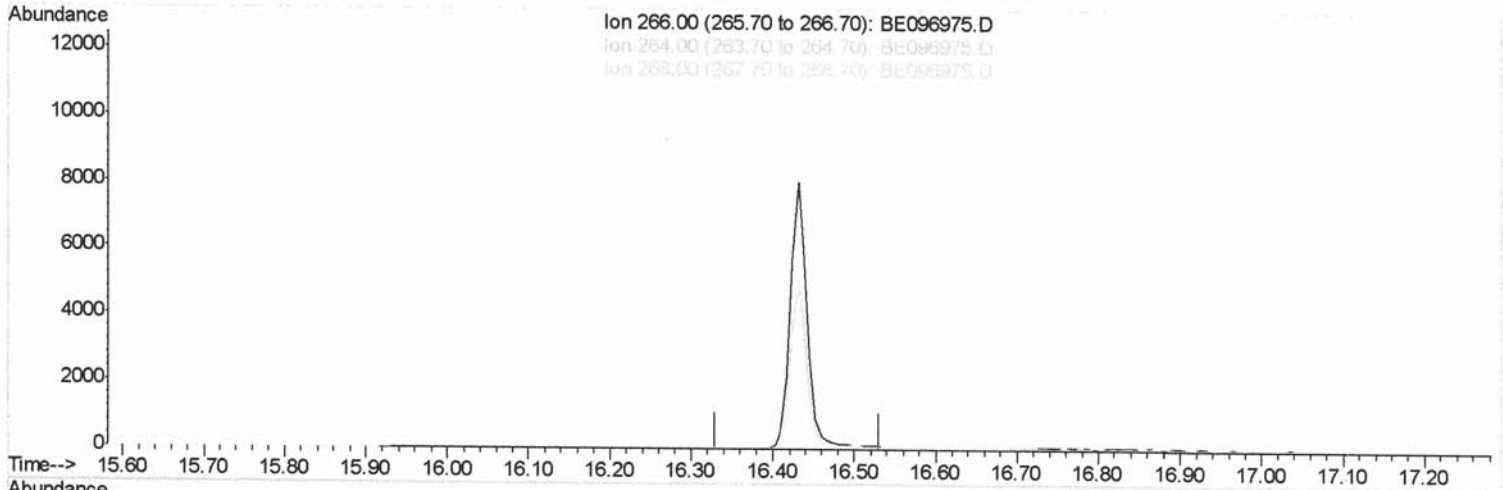

(11) Pentachlorophenol

16.431min (-16.431) 0.00ng/ul

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	59.90	0.00#
268.00	62.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

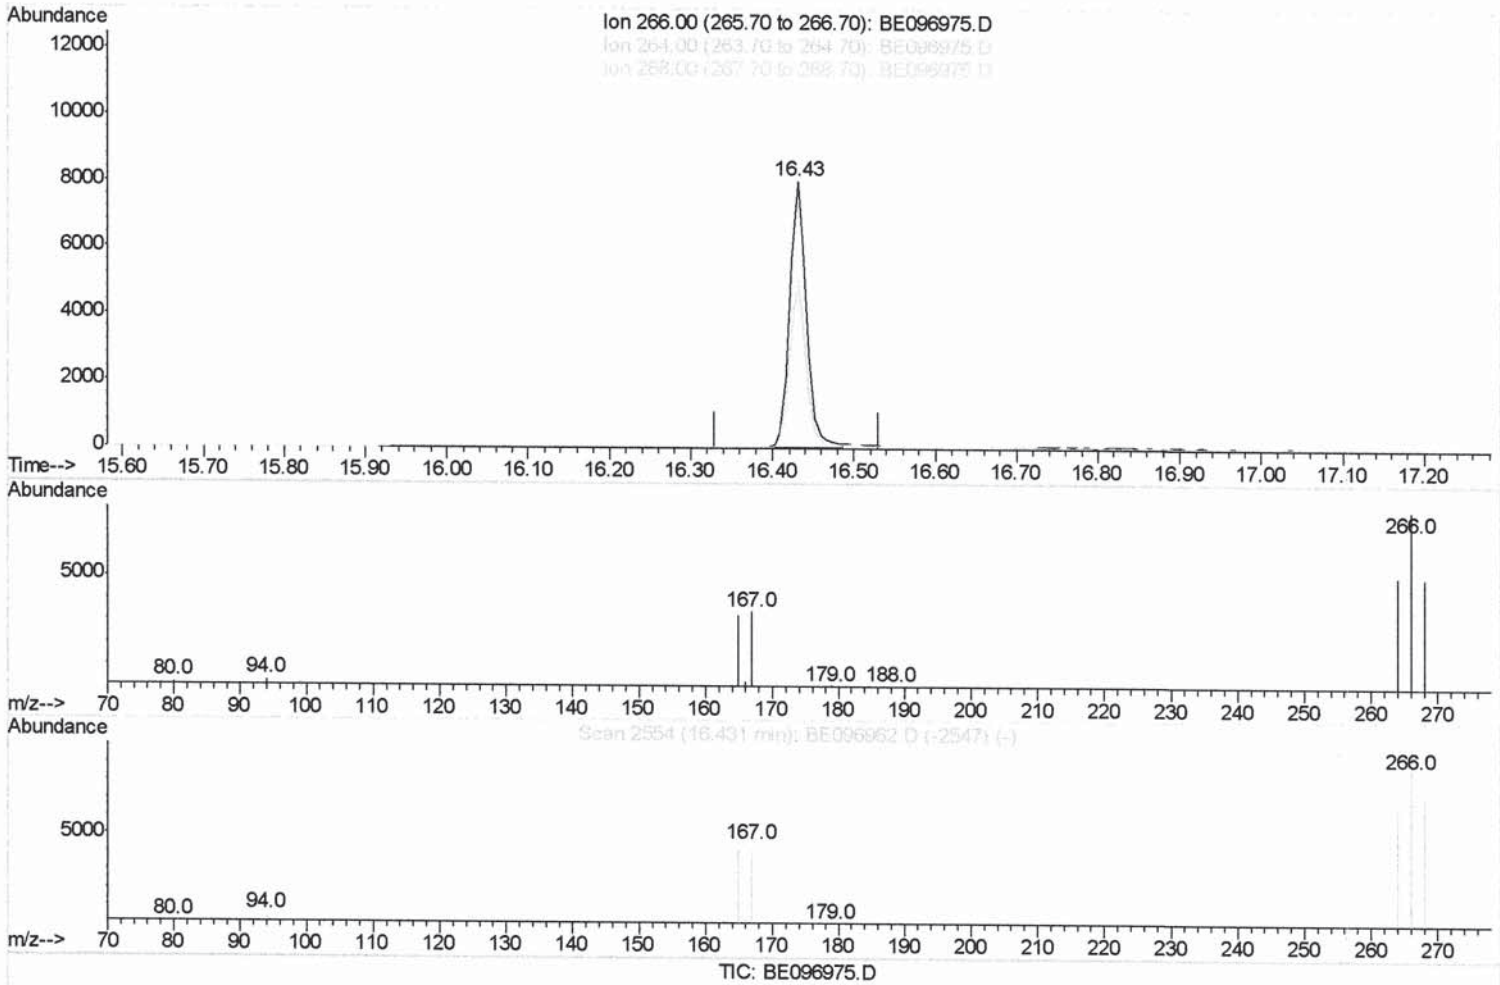

(11) Pentachlorophenol

16.431min (-0.000) 6.33ng/ul m

5/17/19/18

response 11322

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	0.00#
268.00	62.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

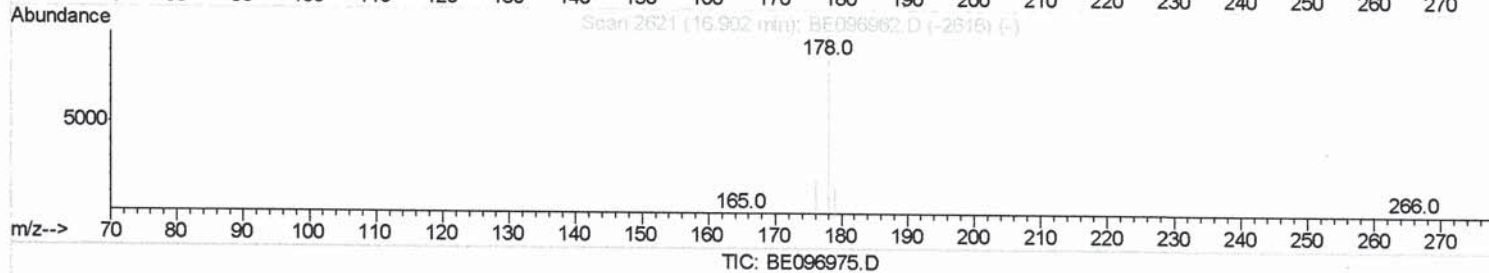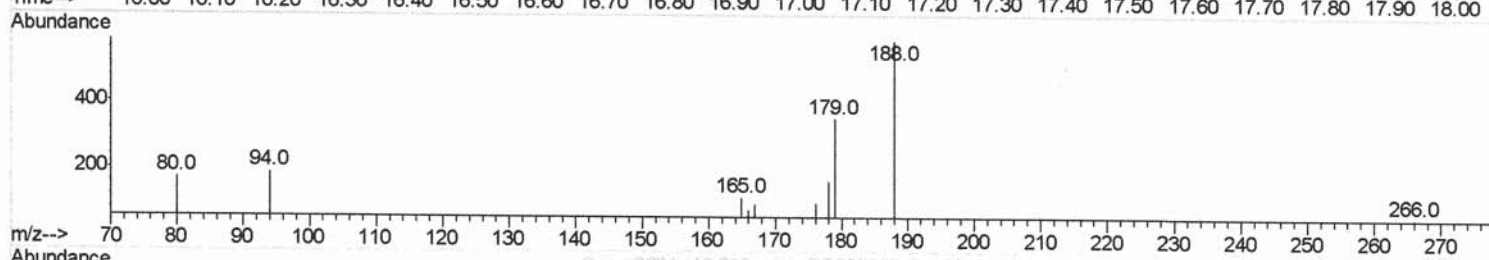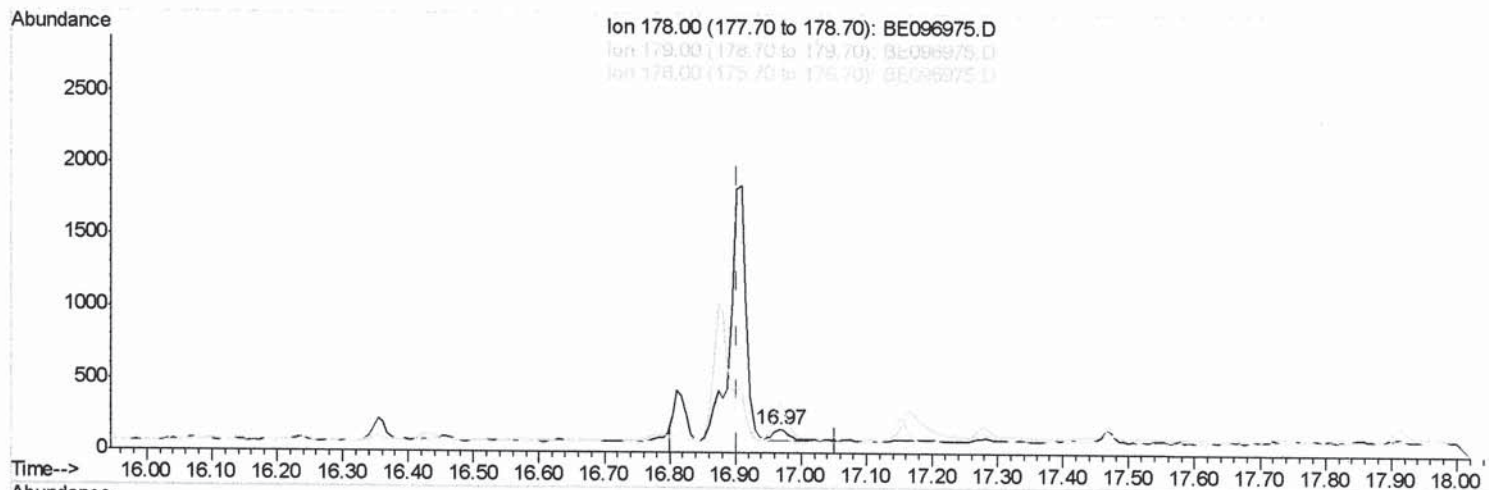

(13) Anthracene

16.965min (+0.063) 0.00ng/ul

response 150

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	214.02#
176.00	18.40	59.15#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

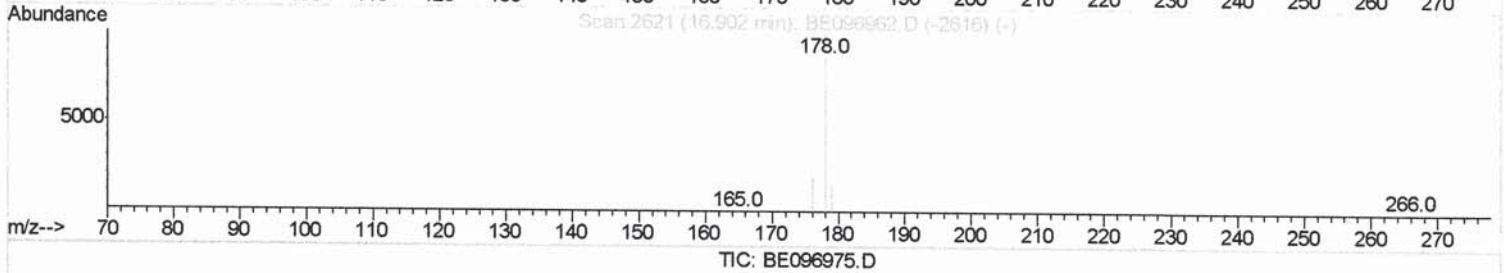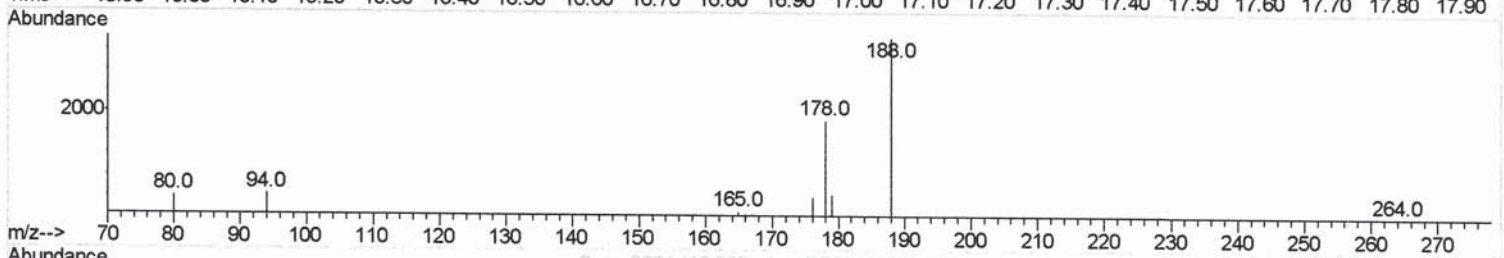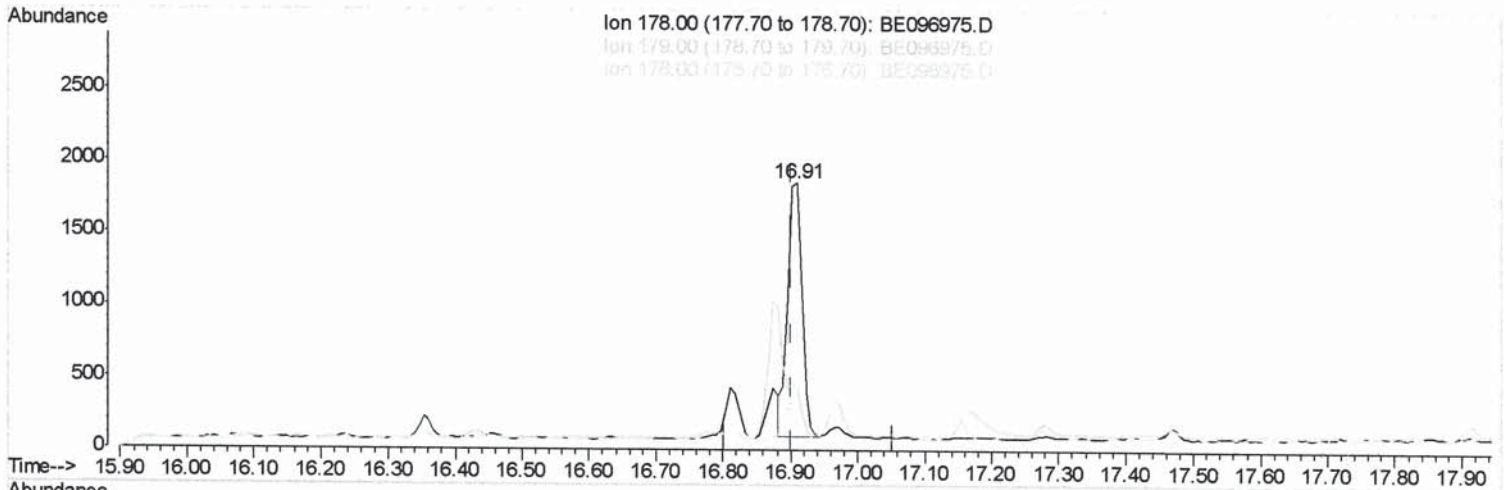

(13) Anthracene

16.909min (+0.007) 0.07ng/ul m

SJ 7/19/18

response 2588

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	23.60
176.00	18.40	21.34
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

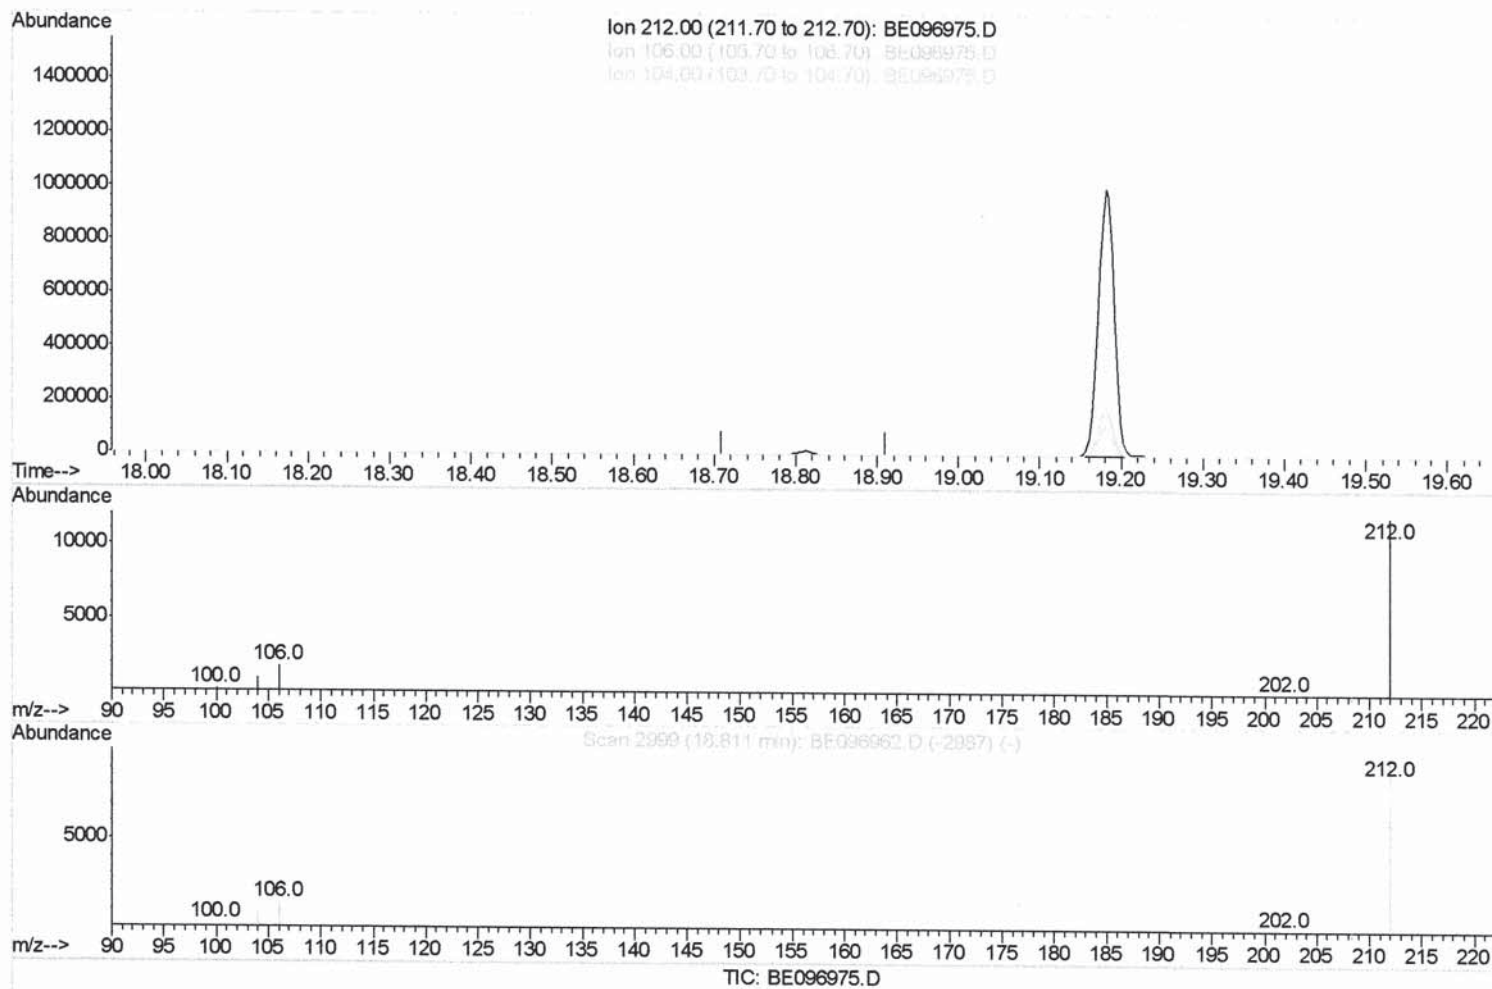

(14) Fluoranthene-d10 (SURR)

18.811min (-18.811) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

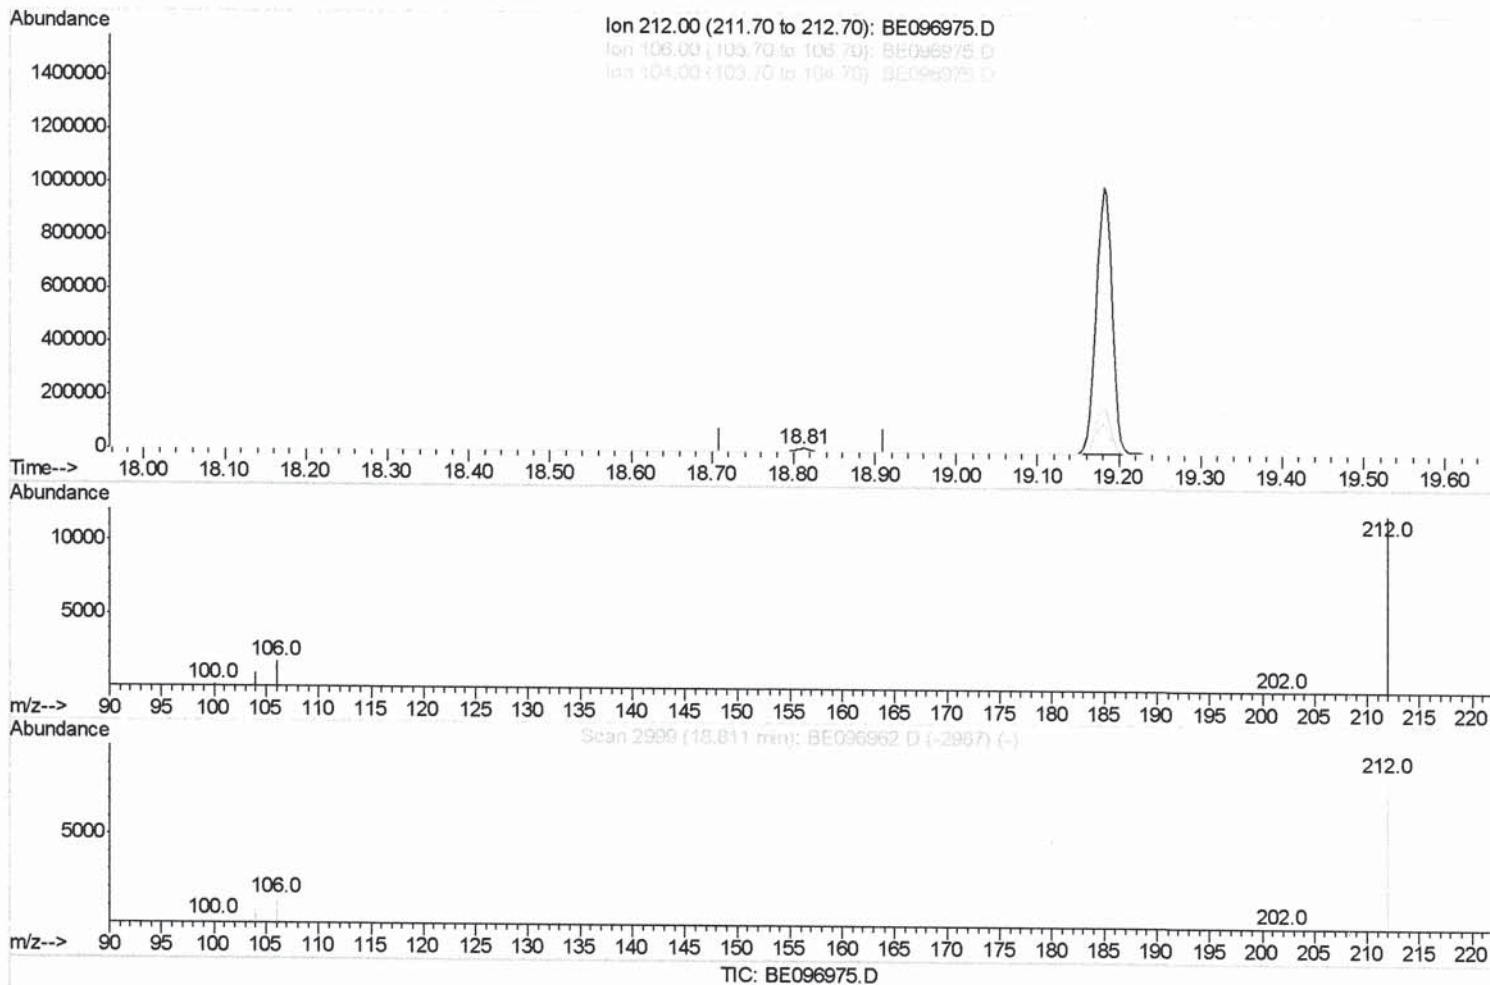

(14) Fluoranthene-d10 (SURR)

18.810min (-0.001) 0.33ng/ul m

response 15987

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

SJ 7/19/18

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

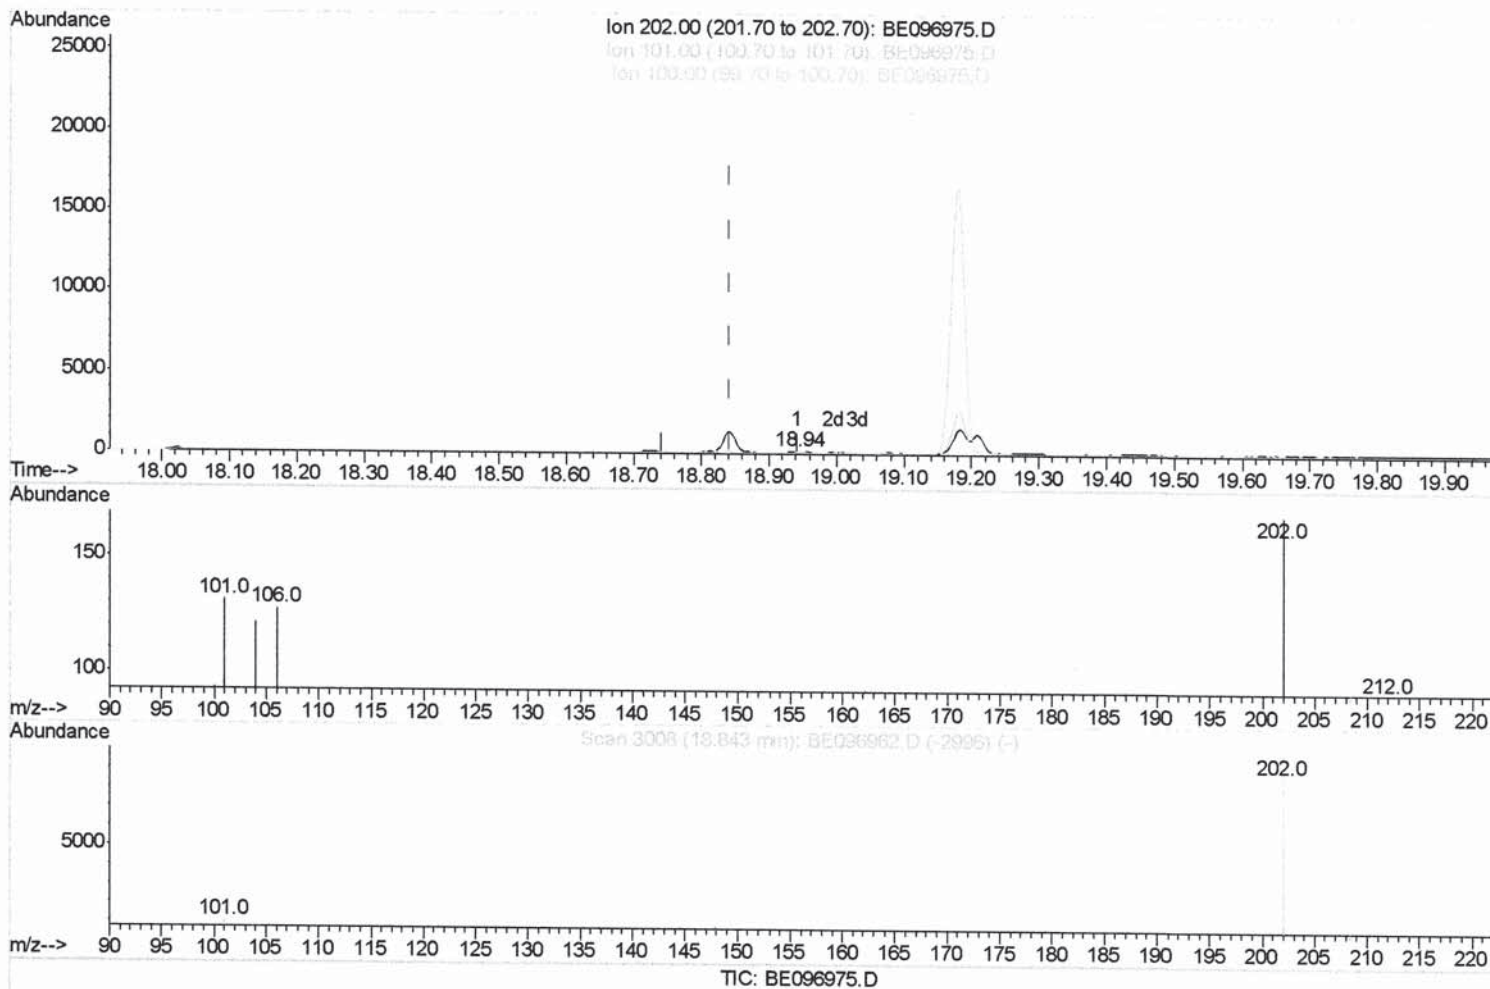

(15) Fluoranthene (C)

18.942min (+0.099) 0.00ng/ul

response 92

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	77.51#
100.00	19.50	55.03#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

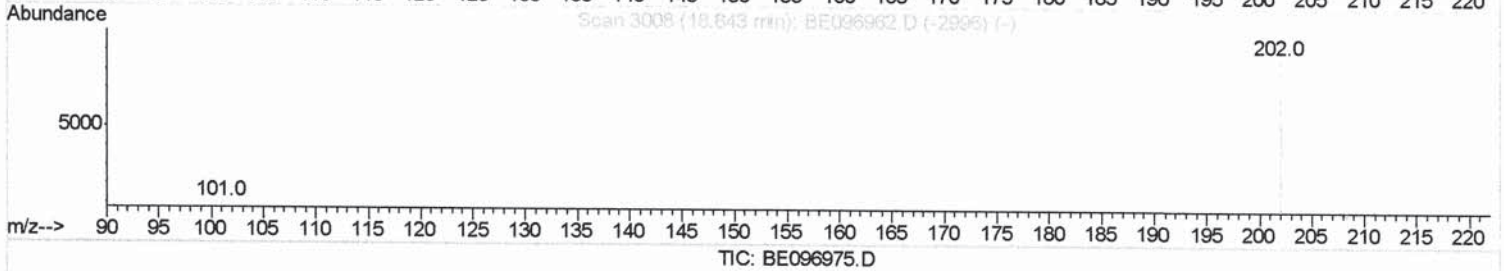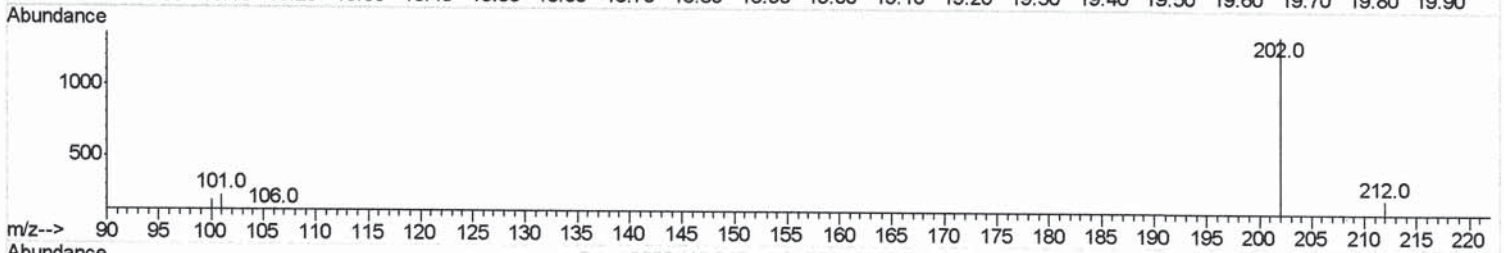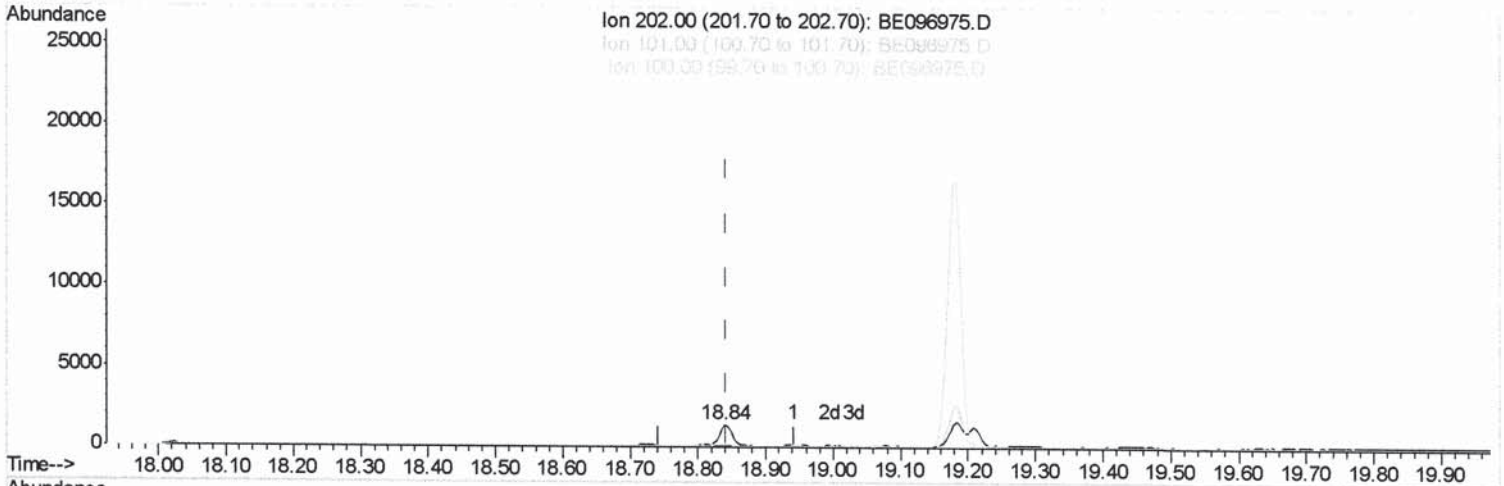

(15) Fluoranthene (C)

18.839min (-0.004) 0.03ng/ul m

SJ 7/19/18

response 1702

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	17.07
100.00	19.50	14.35
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

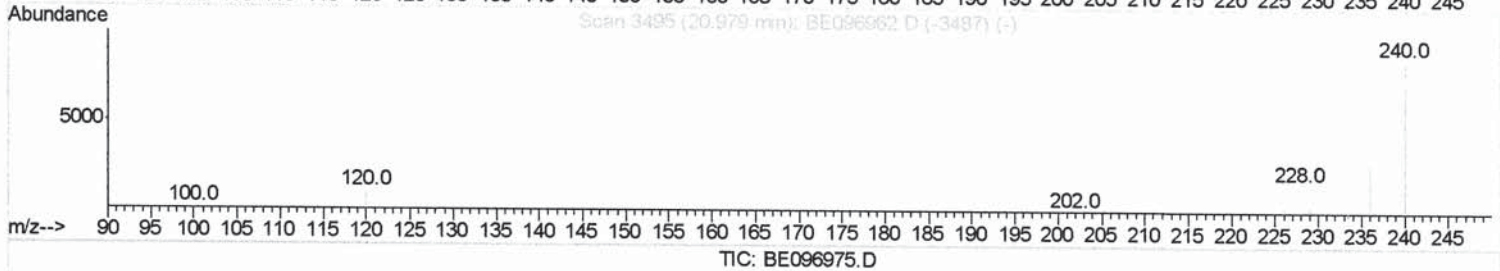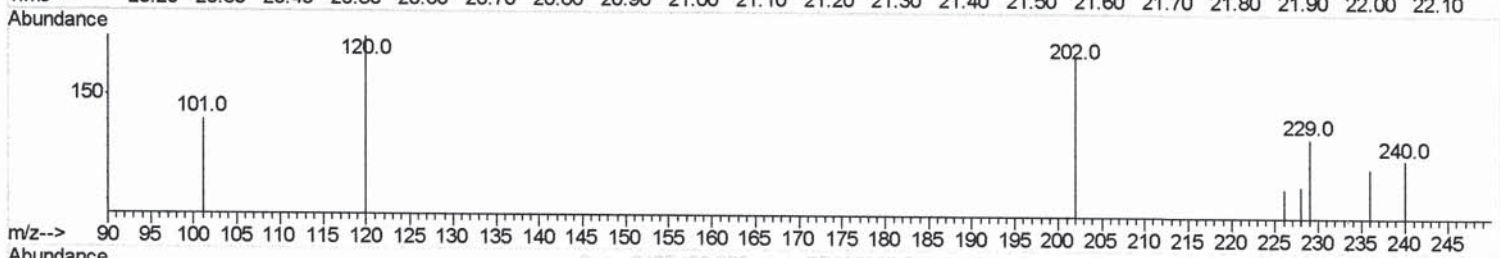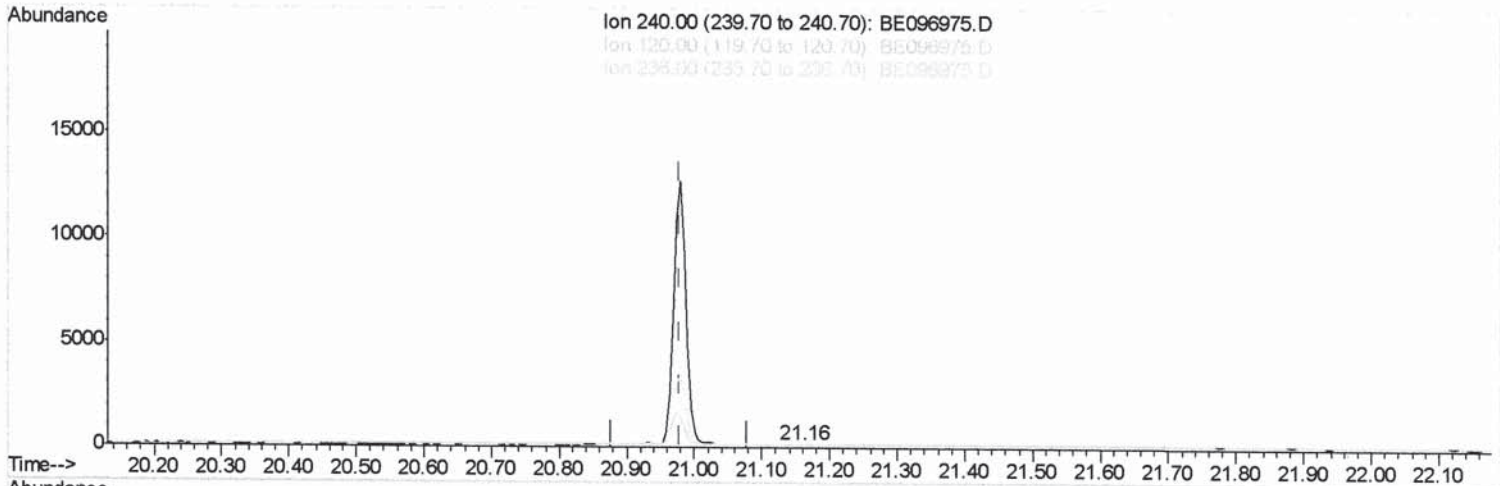

(16) Chrysene-d12 (I)
 21.159min (+0.180) 0.40ng/ul
 response 21

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	135.43#
236.00	34.90	97.64#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:06:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

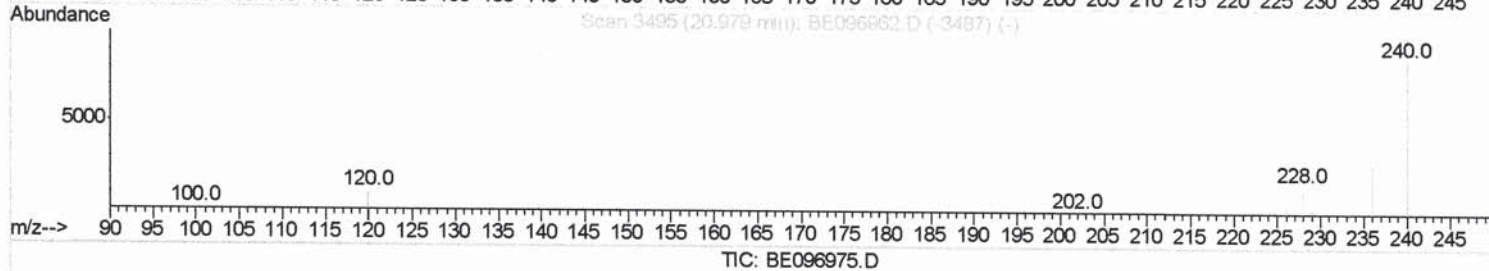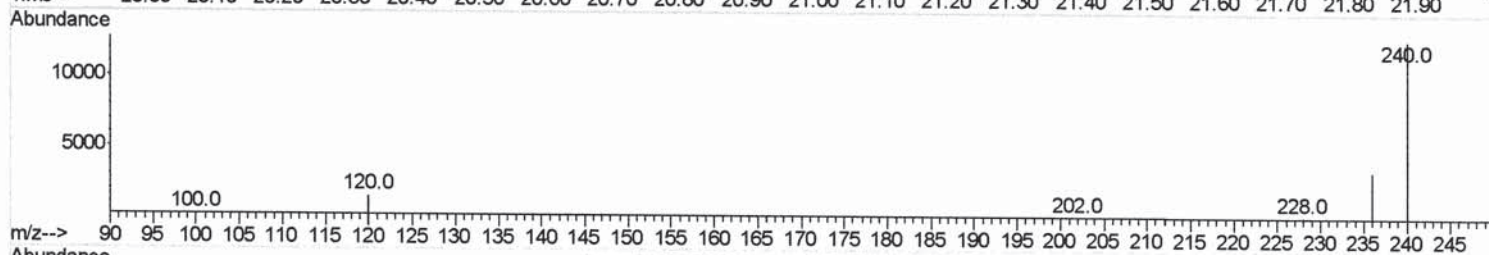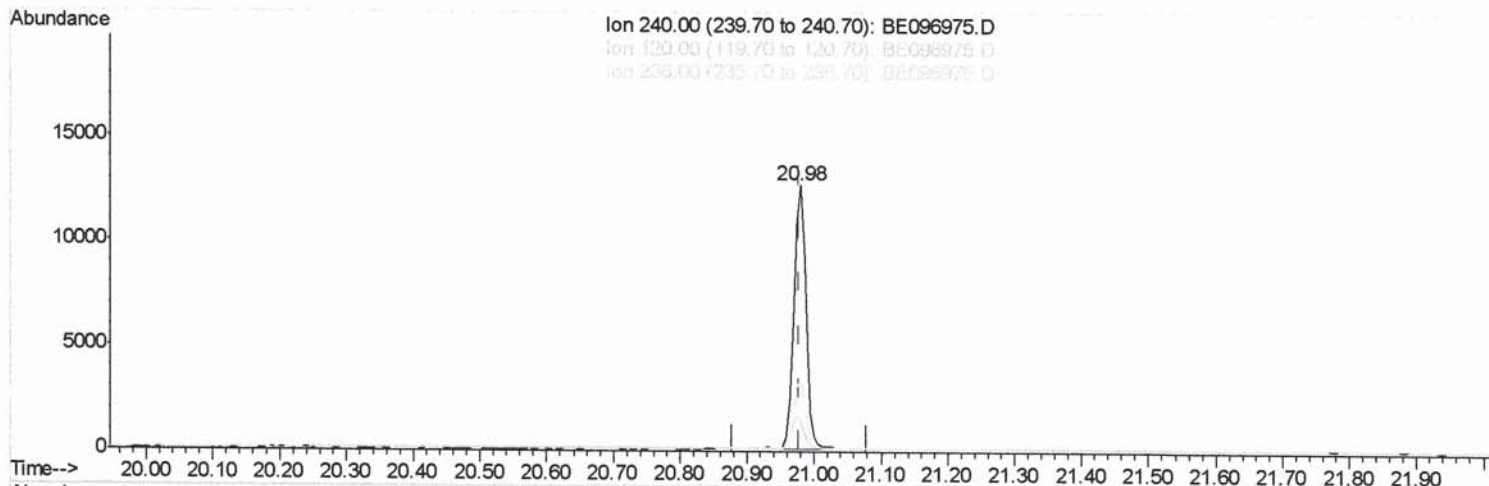

(16) Chrysene-d12 (I)

20.979min (-0.000) 0.40ng/ul m

SJ 7/19/18

response 15826

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.55#
236.00	34.90	27.14#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:08:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

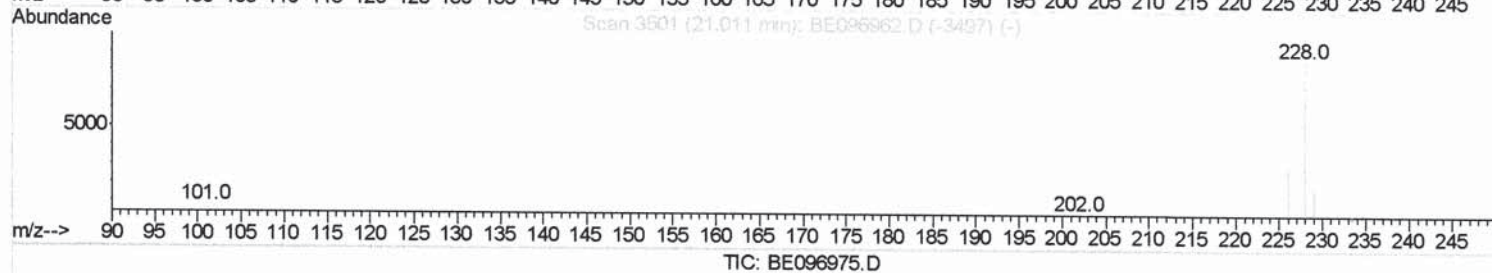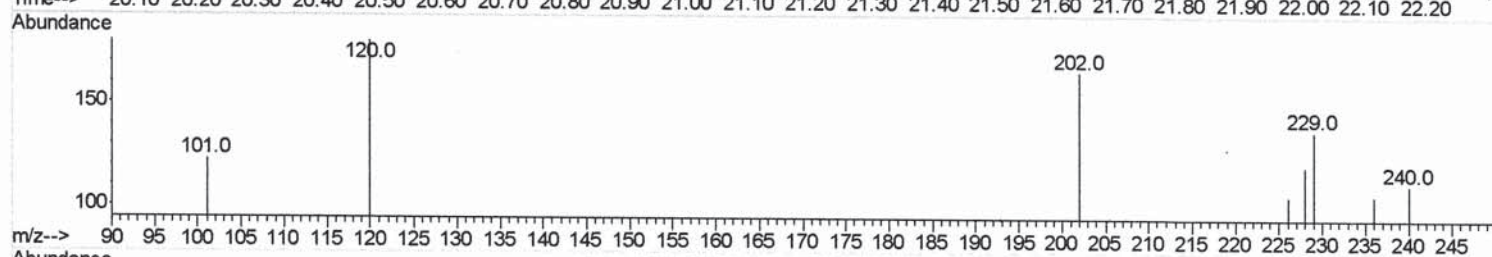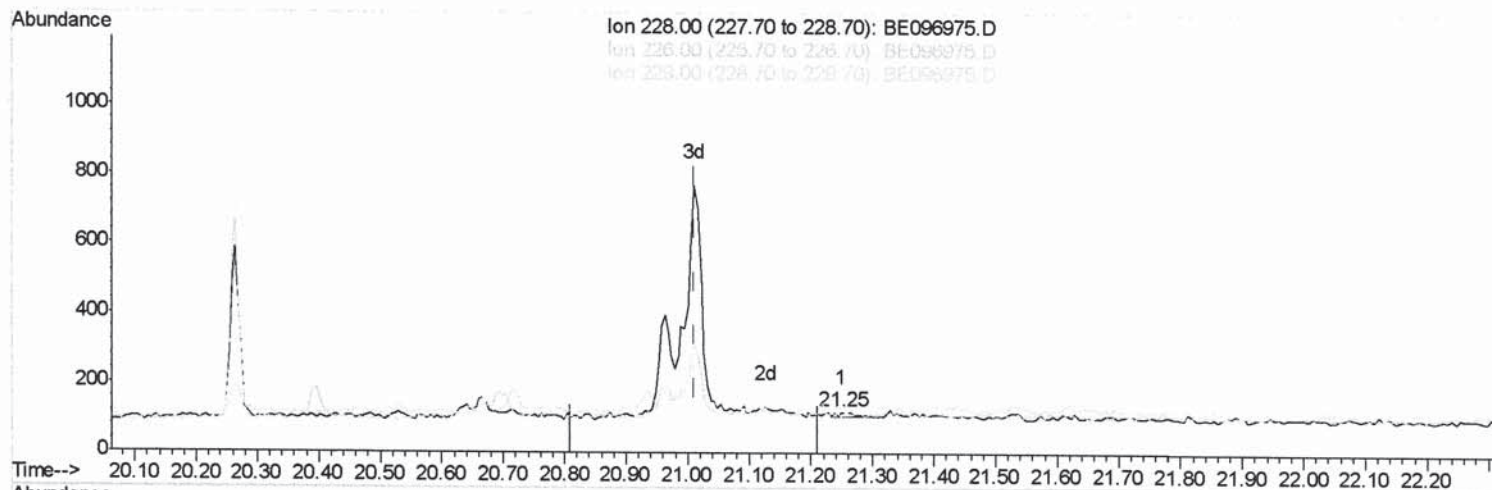

(19) Chrysene

21.249min (+0.238) 0.00ng/ul

response 29

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	87.50#
229.00	22.10	114.17#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:08:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

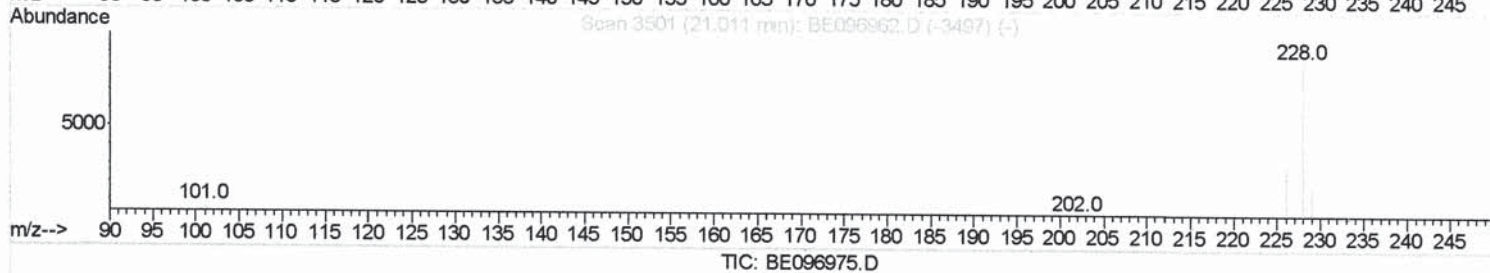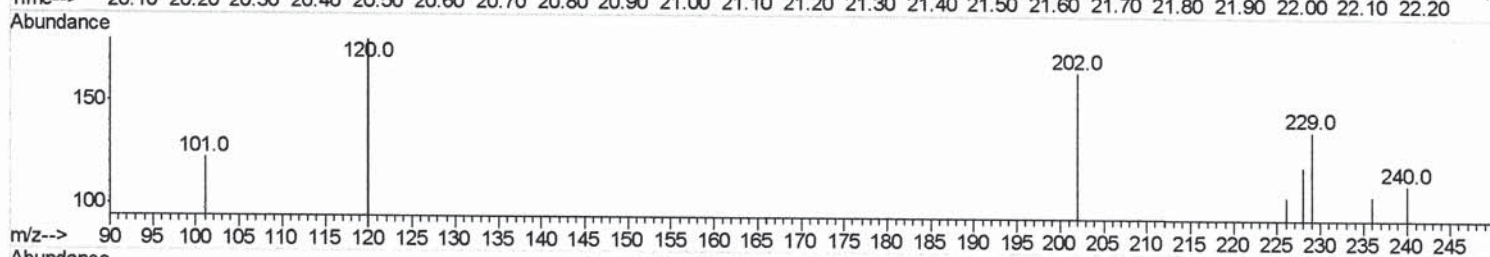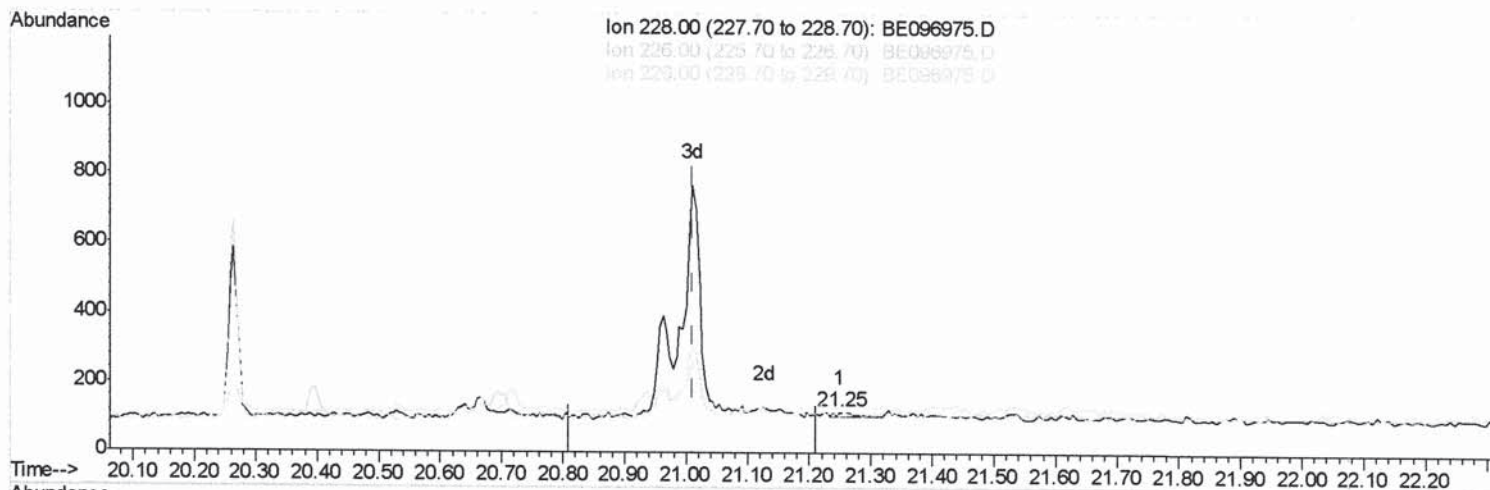

(19) Chrysene

21.249min (+0.238) 0.00ng/ul

response 29

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	87.50#
229.00	22.10	114.17#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096975.D
Acq On : 18 Jul 2018 2:03
Operator : SJ/JU
Sample : J3967-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DB1F8

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:08:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

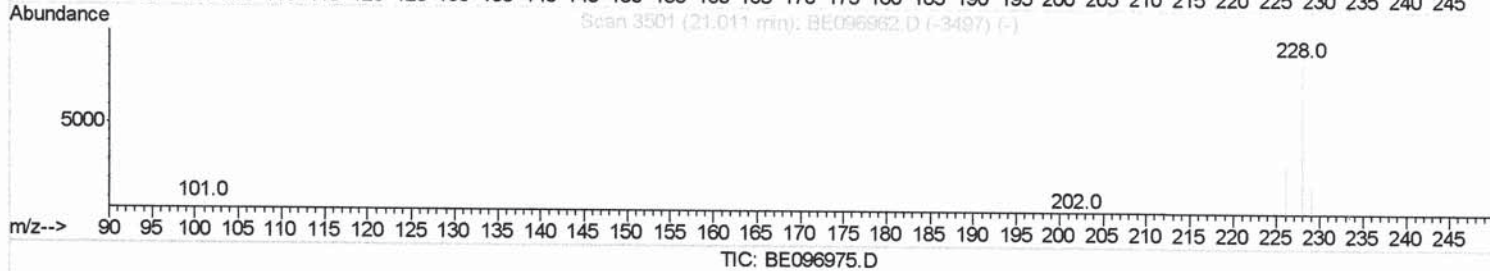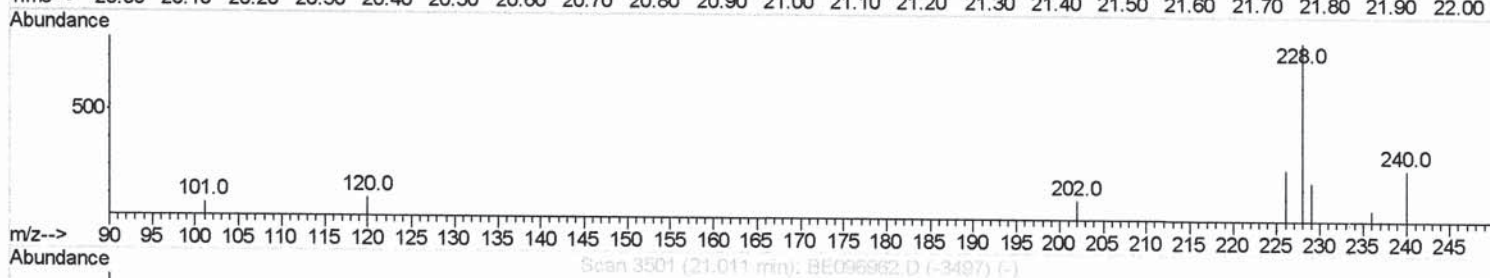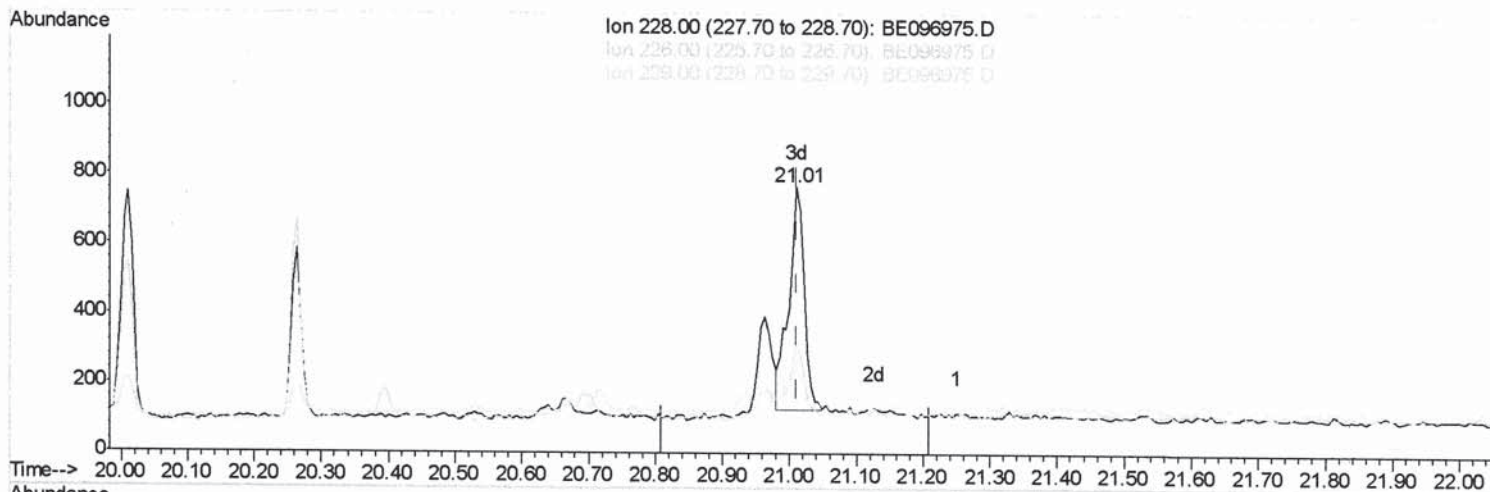

(19) Chrysene

21.011min (-0.000) 0.02ng/ul m

557/19/18

response 1027

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	39.79#
229.00	22.10	34.20#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:11:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

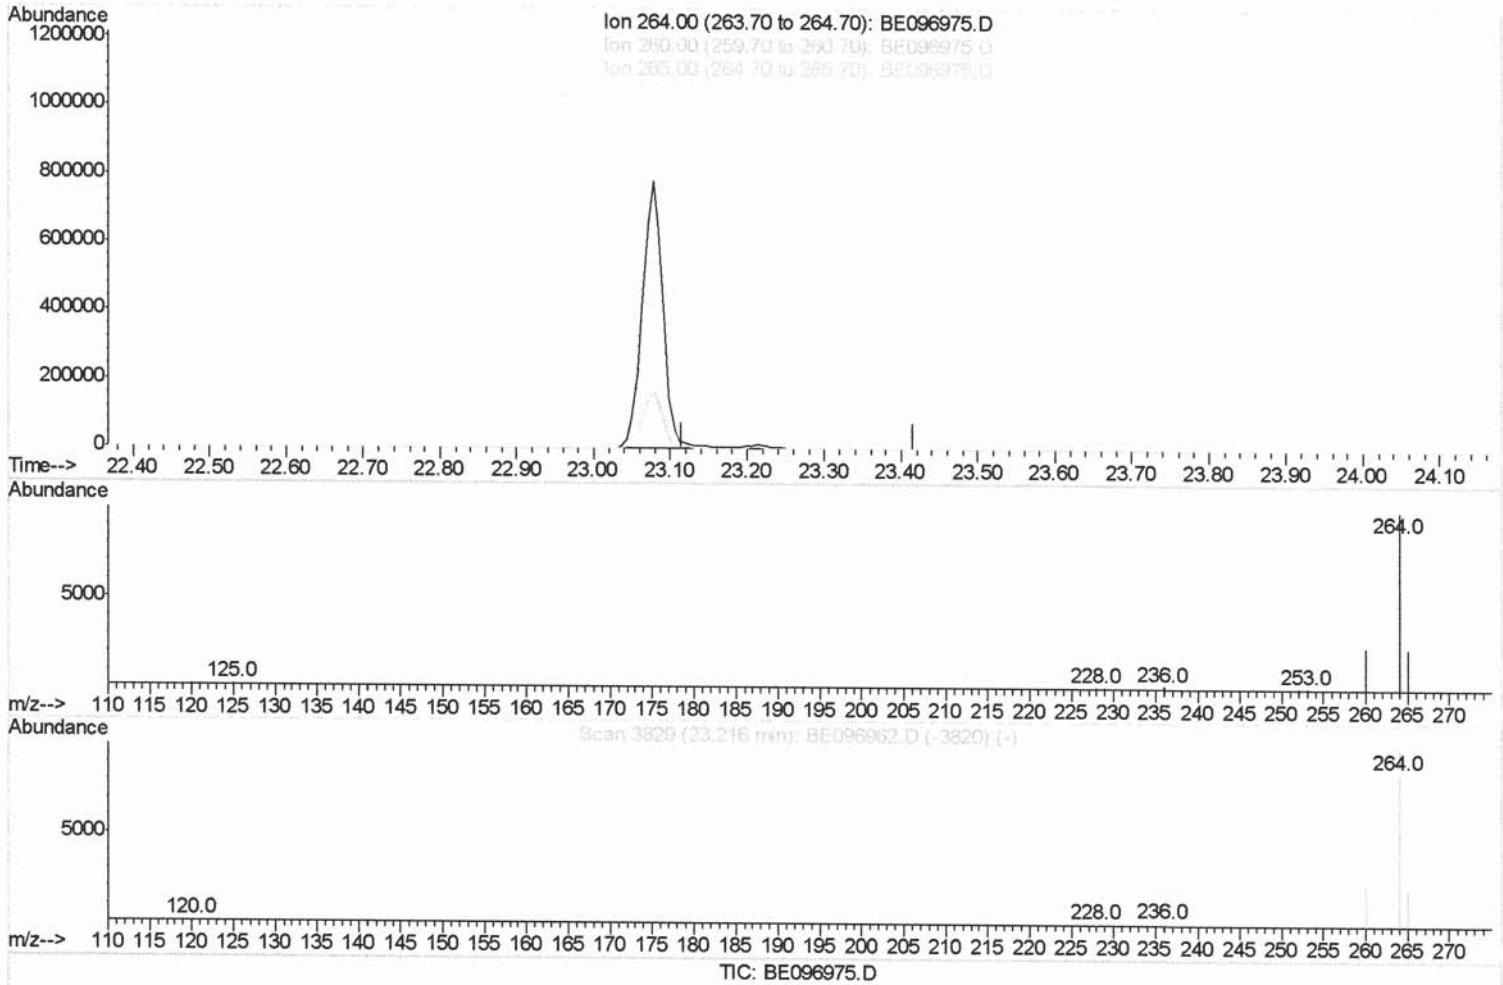

(20) Perylene-d12 (I)
 23.216min (-23.216) 0.00ng/ul
 response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	30.10	0.00#
265.00	103.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:11:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

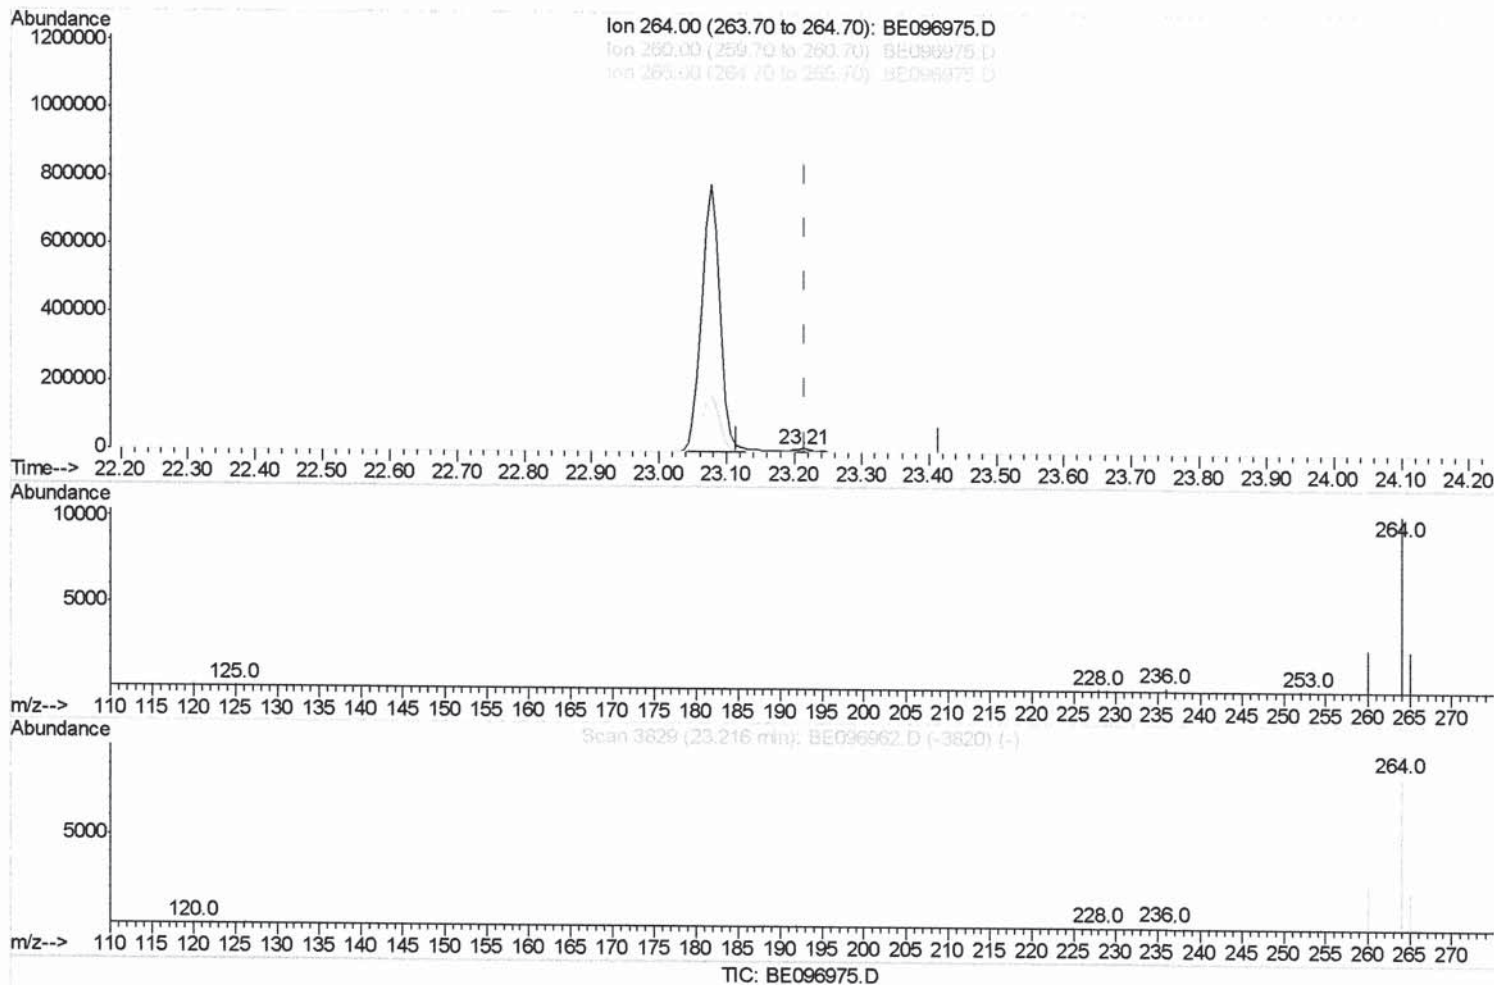

(20) Perylene-d12 (I)

23.211min (-0.005) 0.40ng/ul m

SJ 7/19/18

response 13335

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.49
265.00	103.50	23.70#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:12:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

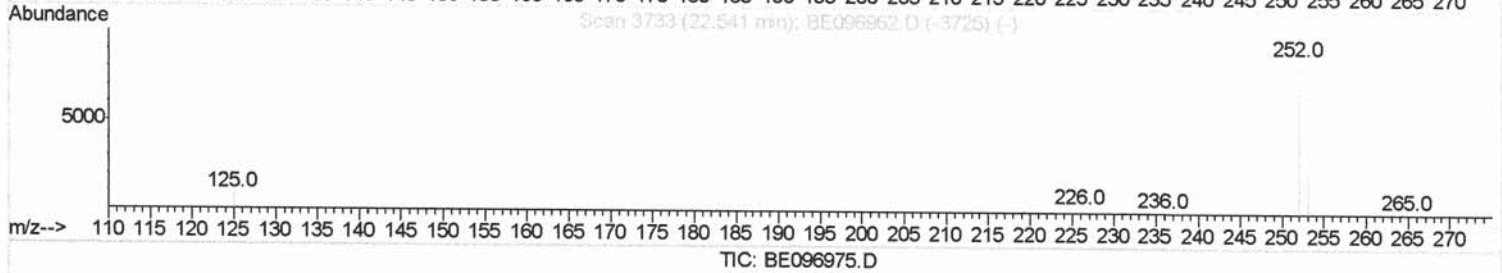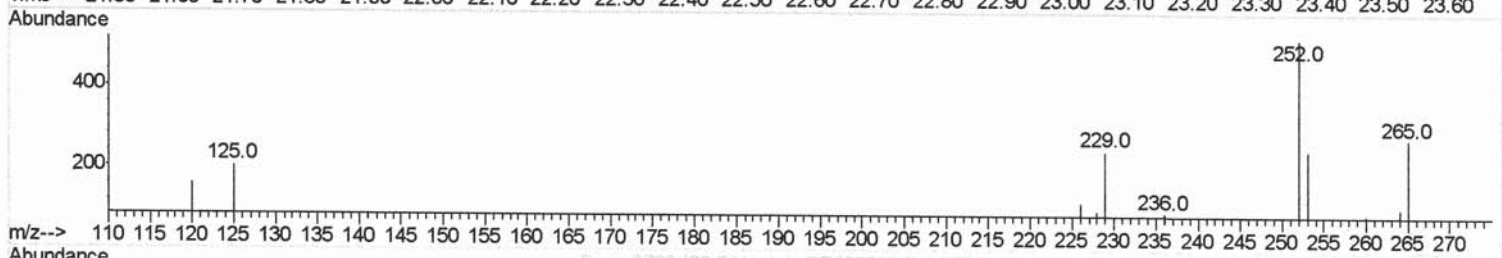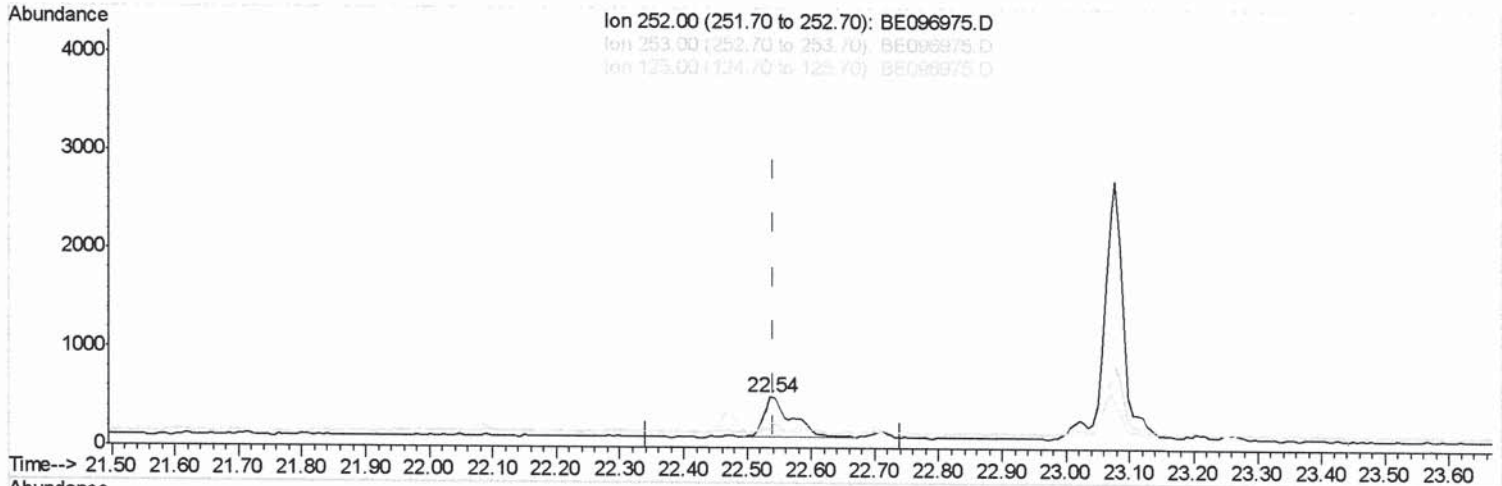

(21) Benzo(b)fluoranthene
 22.536min (-0.005) 0.03ng/ul
 response 1244

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	47.59
125.00	17.50	38.92#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:12:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

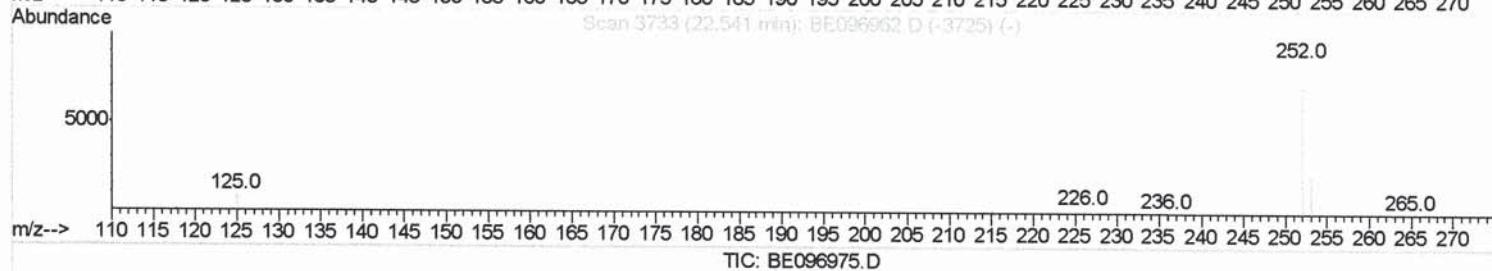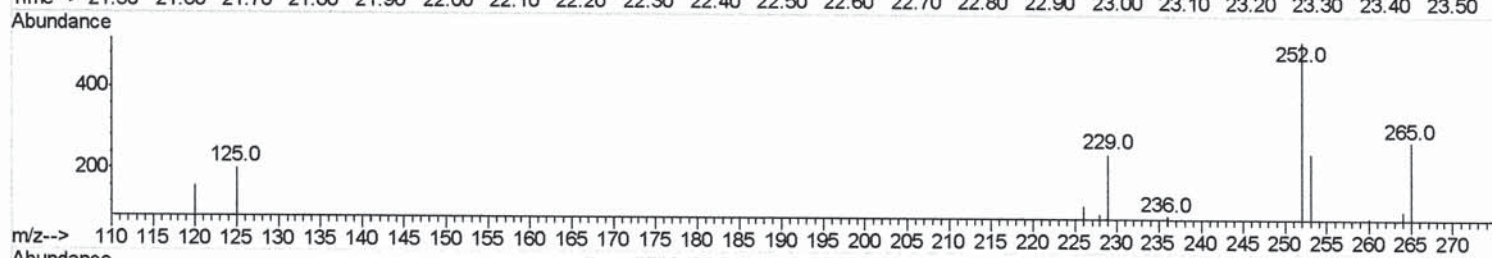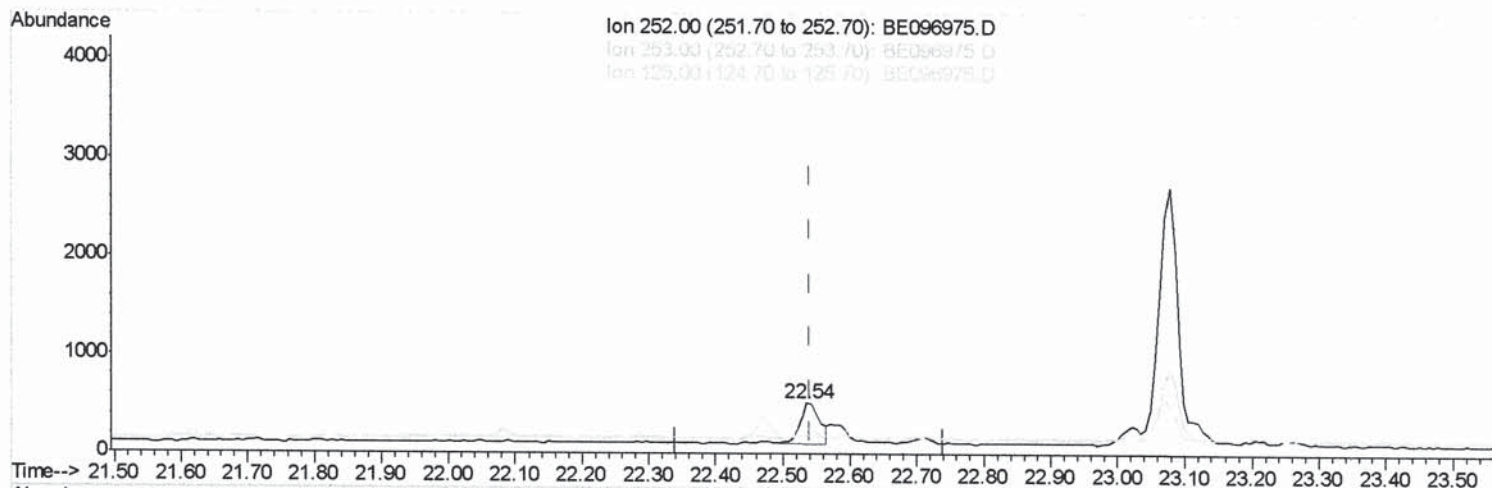

(21) Benzo(b)fluoranthene

22.536min (-0.005) 0.02ng/ul m

response 849

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	47.59
125.00	17.50	38.92#
0.00	0.00	0.00

5/17/19/18

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096975.D
 Acq On : 18 Jul 2018 2:03
 Operator : SJ/JU
 Sample : J3967-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F8

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:50 AM

Quant Time: Jul 18 07:13:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1795	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	9514	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	6094	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	15830m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	15826m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	13335m	0.40	ng/ul	0.00

} SJ 7/19/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.73	152	4880	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	15987m	0.33	ng/ul	0.00

SJ 7/19/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Acenaphthene	14.08	153	760	0.037	ng/ul#	93
9) Fluorene	15.08	166	2035	0.093	ng/ul	94
11) Pentachlorophenol	16.43	266	11322m	6.327	ng/ul	
13) Anthracene	16.91	178	2588m	0.071	ng/ul	
15) Fluoranthene	18.84	202	1702m	0.031	ng/ul	
17) Pyrene	19.21	202	1270	0.028	ng/ul#	94
19) Chrysene	21.01	228	1027m	0.022	ng/ul	
21) Benzo(b)fluoranthene	22.54	252	849m	0.022	ng/ul	

} SJ 7/19/18
 > SJ 7/19/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed