

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096973.D
 Acq On : 18 Jul 2018 00:49
 Operator : SJ/JU
 Sample : J3967-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1E5

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:44 AM

Quant Time: Jul 18 05:02:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1829	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	9353	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	5814	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	14813m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	15711m	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	13941m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	4702	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	15517m	0.35	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.43	266	177m	0.106	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096973.D
Acq On : 18 Jul 2018 00:49
Operator : SJ/JU
Sample : J3967-13
Misc :
ALS Vial : 22 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
DB1E5

Manual Integrations
APPROVED

Sohil
7/18/2018 10:49:44 AM

Quant Time: Jul 18 05:02:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

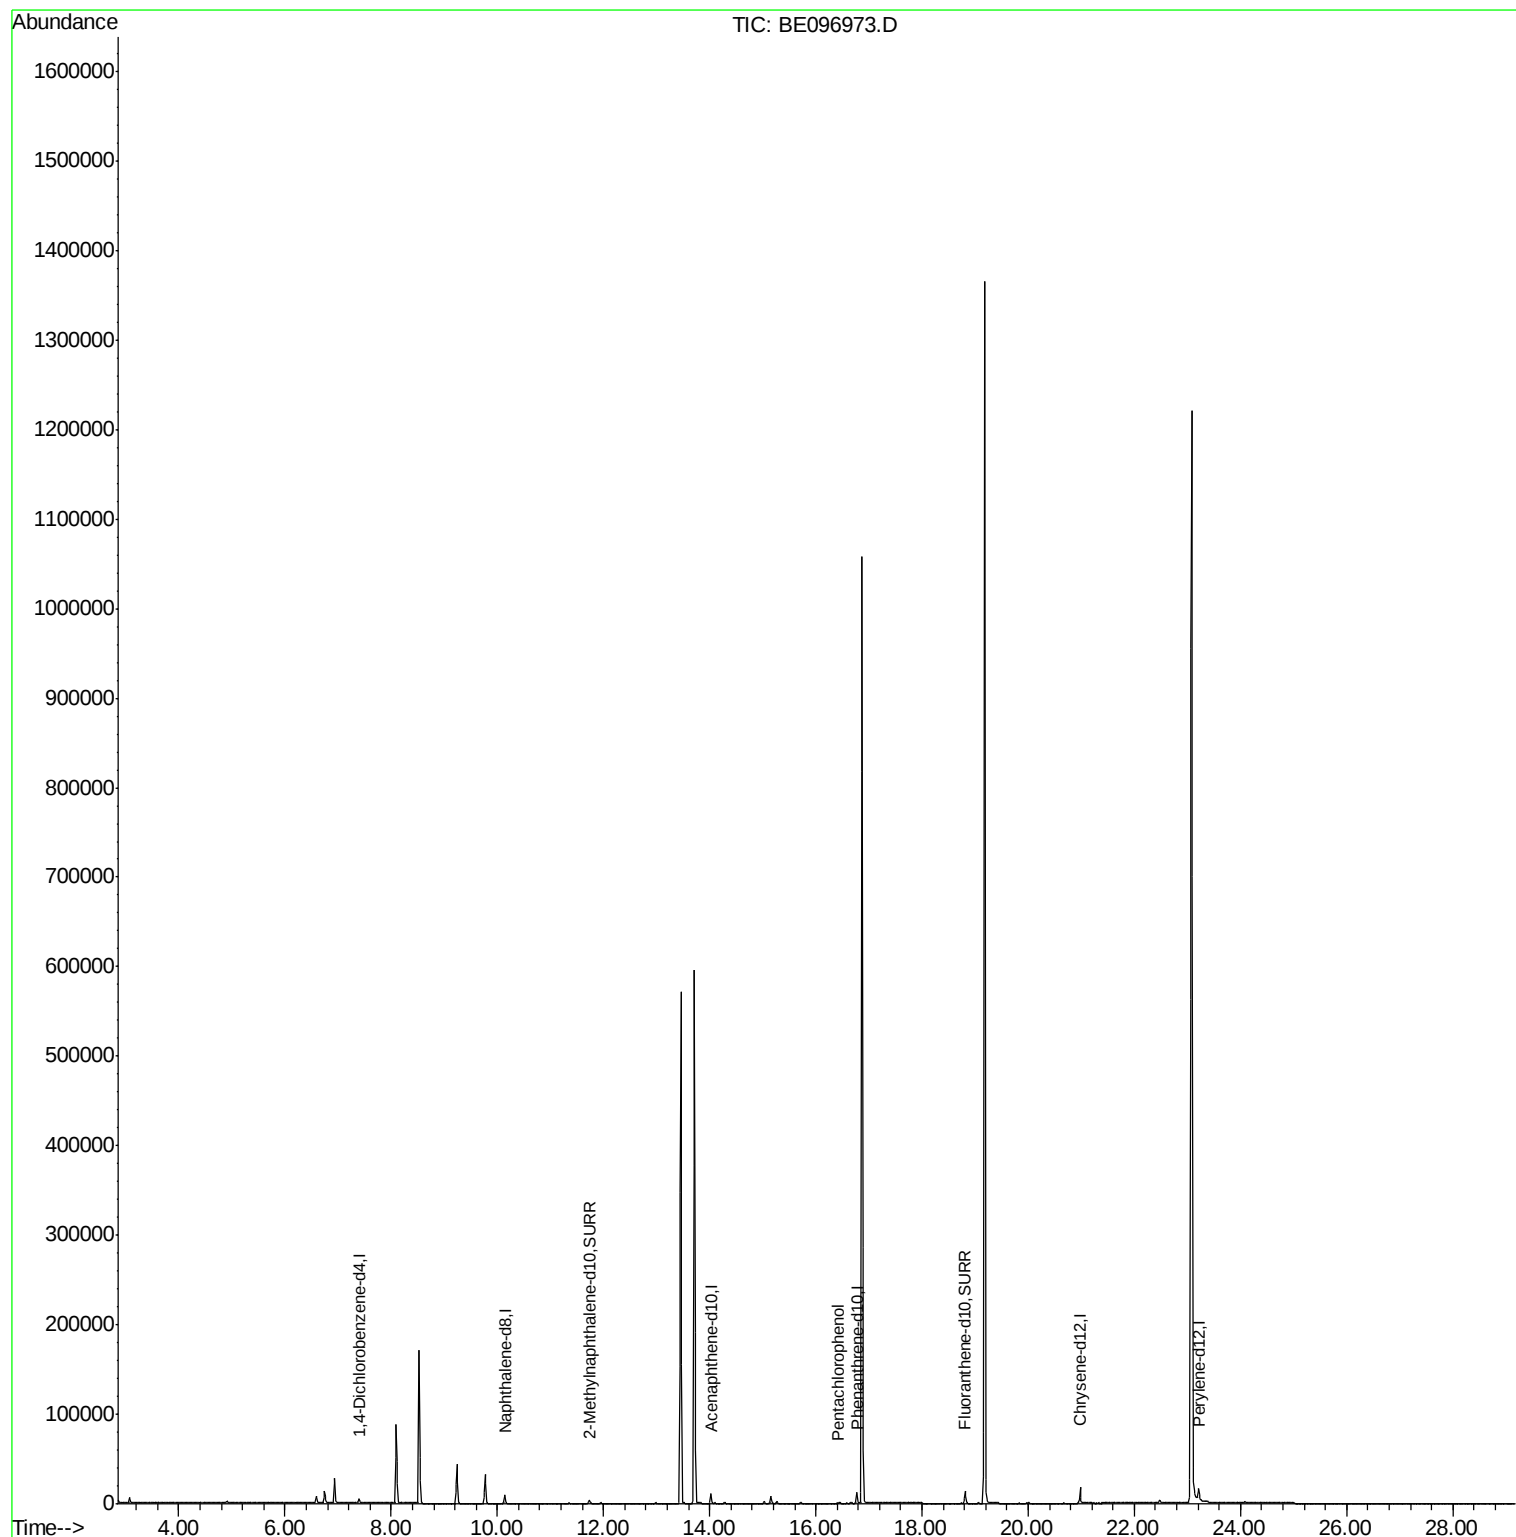

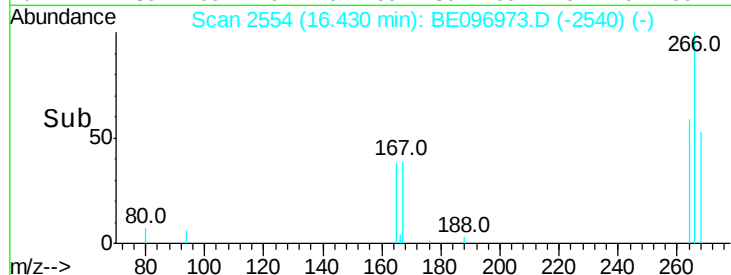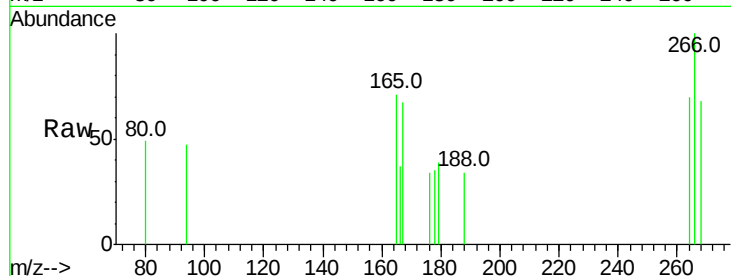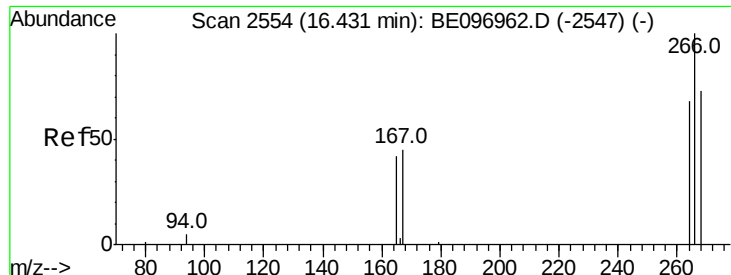

#11
 Pentachlorophenol
 Concen: 0.106 ng/ul m
 RT: 16.43 min Scan# 2554
 Delta R.T. -0.00 min
 Lab File: BE096973.D
 Acq: 18 Jul 2018 00:49

Instrument :
 BNA_E
 ClientSampleId :
 DB1E5

Tot Ion	Ratio	Lower	Upper
266	100		
264	0.0	47.9	71.9#
268	0.0	49.8	74.8#

Manual Integrations
 APPROVED

Sohil
 7/18/2018 10:49:44 AM

