


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071719\
Data File : BE100448.D
Acq On : 17 Jul 2019 13:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 16 14:03:26 2019

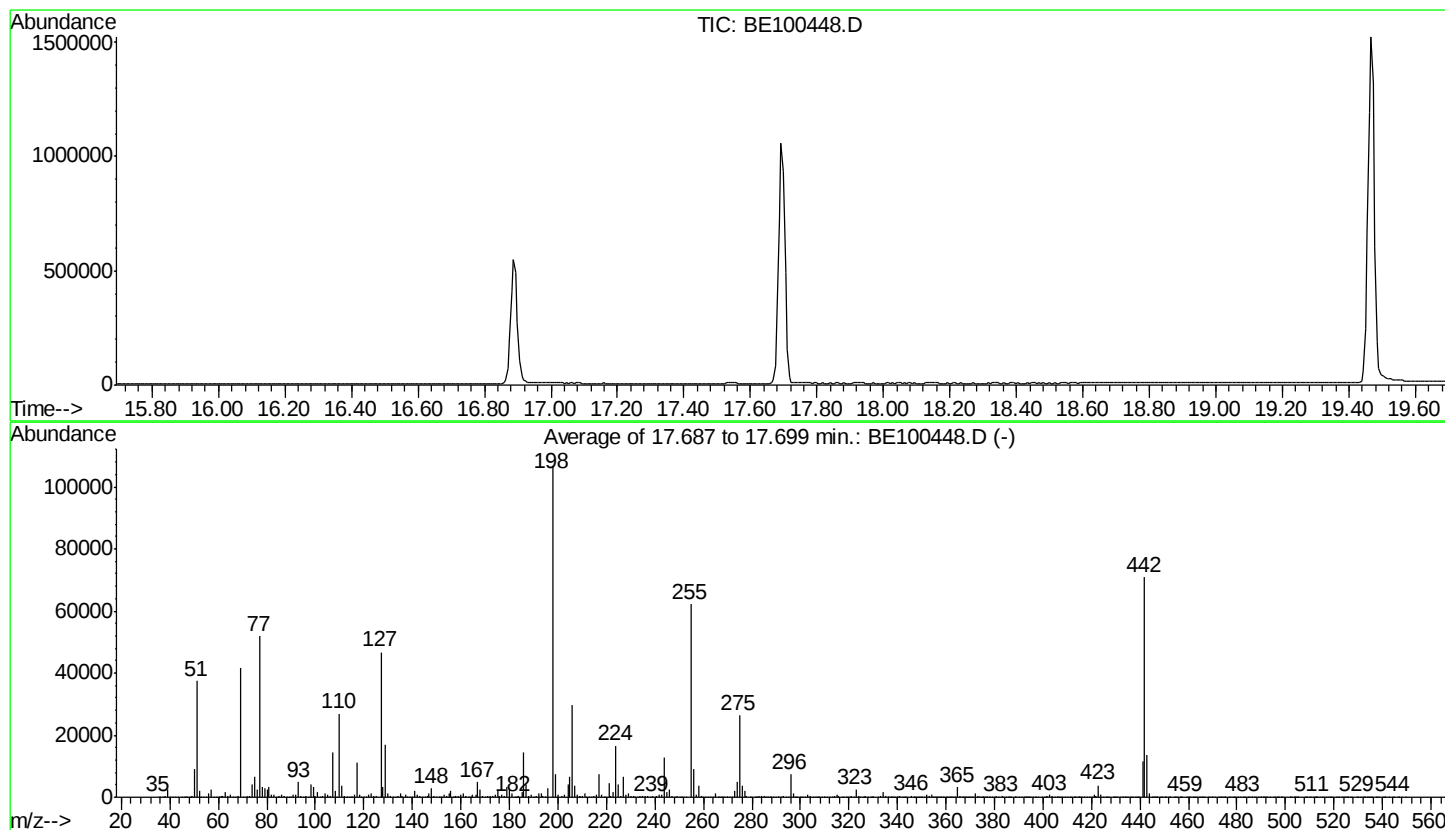

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	37393	PASS
68	69	0.00	2	1.2	495	PASS
69	198	0.00	100	39.1	41818	PASS
70	69	0.00	2	0.4	159	PASS
127	198	10	80	43.7	46645	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106833	PASS
199	198	5	9	6.8	7312	PASS
275	198	10	60	24.6	26285	PASS
365	198	1	100	2.9	3139	PASS
441	198	0.01	100	11.0	11719	PASS
442	198	50	100	66.4	70911	PASS
443	442	15	24	19.4	13744	PASS