

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE071818\
 Data File : BE096992.D
 Acq On : 18 Jul 2018 14:11
 Operator : SJ/JU
 Sample : J3967-22
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1F4

Manual Integrations
 APPROVED

Sohil
 7/19/2018 11:36:46 AM

Quant Time: Jul 18 16:28:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 15:28:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	1436	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	7694	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	5313	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	13975m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	15244m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	12046m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.74	152	4476	0.37	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	17812m	0.42	ng/ul	0.00
Target Compounds						
9) Fluorene	15.08	166	513	0.027	ng/ul#	88
11) Pentachlorophenol	16.43	266	486m	0.308	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE071818\
Data File : BE096992.D
Acq On : 18 Jul 2018 14:11
Operator : SJ/JU
Sample : J3967-22
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
DB1F4

Manual Integrations
APPROVED

Sohil
7/19/2018 11:36:46 AM

Quant Time: Jul 18 16:28:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 15:28:33 2018
Response via : Initial Calibration

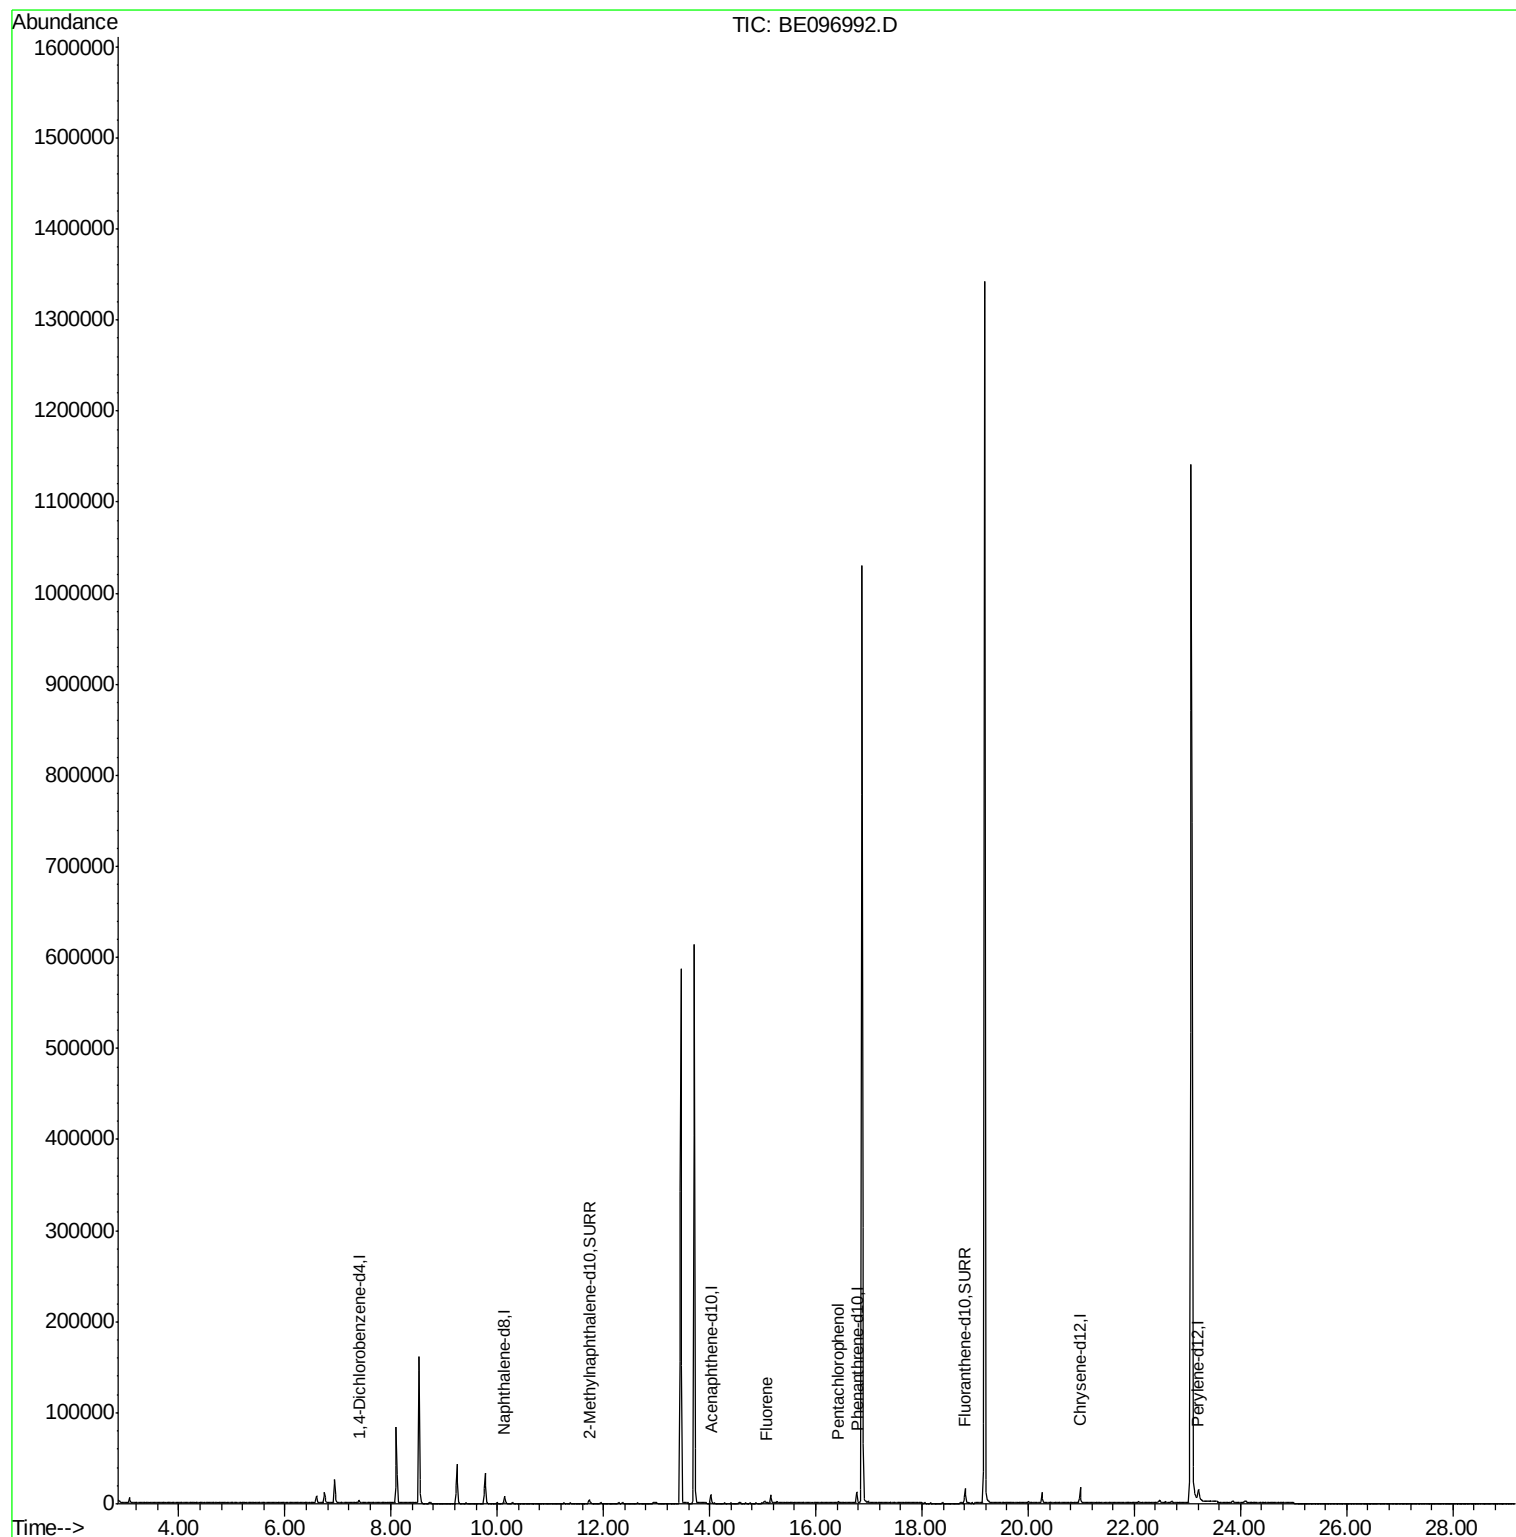

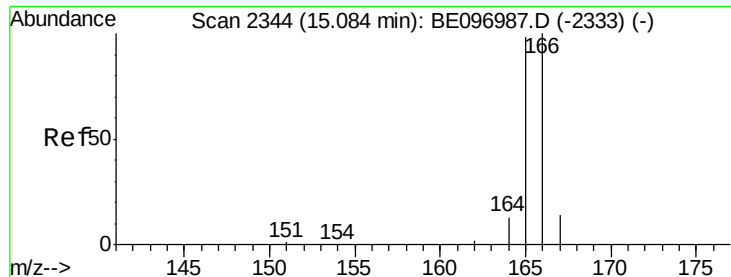

#9

Fluorene

Concen: 0.027 ng/ul

RT: 15.08 min Scan# 2341

Delta R.T. -0.00 min

Lab File: BE096992.D

Acq: 18 Jul 2018 14:11

Instrument :

BNA_E

ClientSampleId :

DB1F4





Tgt Ion:166 Resp: 513

Ion	Ratio	Lower	Upper
166	100		
165	99.3	73.4	110.2
167	32.2	14.6	22.0#

Manual Integrations
APPROVED

Sohil

7/19/2018 11:36:46 AM

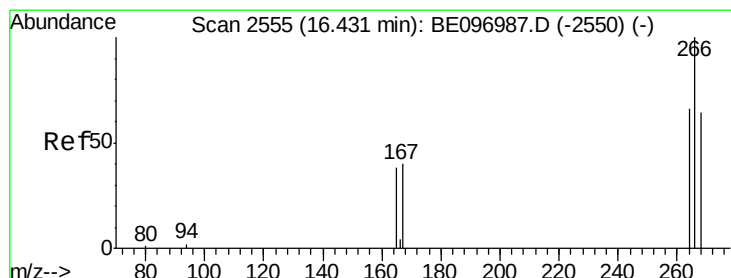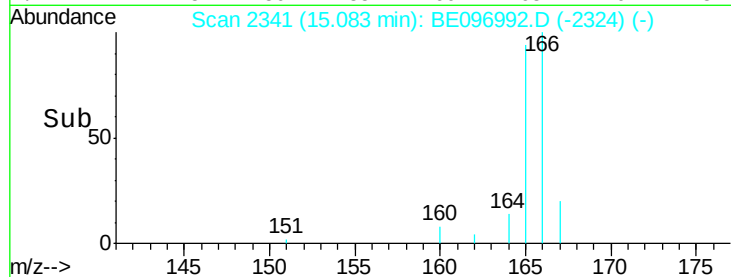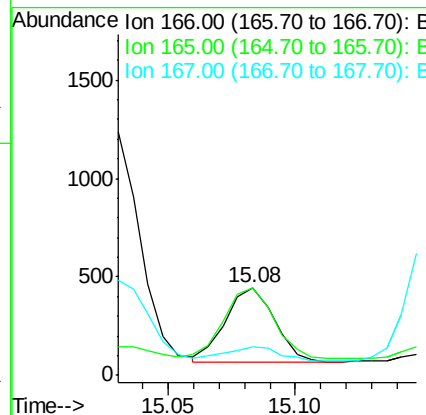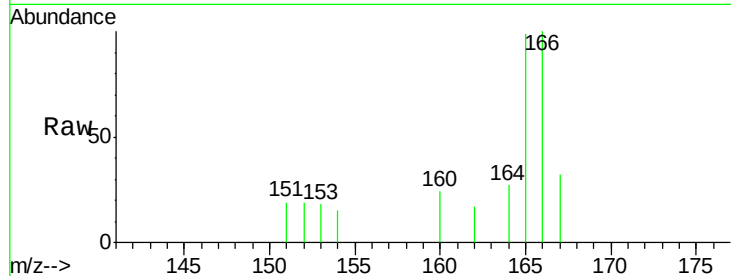

#11

Pentachlorophenol

Concen: 0.308 ng/ul m

RT: 16.43 min Scan# 2552

Delta R.T. 0.00 min

Lab File: BE096992.D

Acq: 18 Jul 2018 14:11

Tgt Ion:266 Resp: 486

Ion	Ratio	Lower	Upper
266	100		
264	0.0	47.9	71.9#
268	0.0	49.8	74.8#

