

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE071818\
 Data File : BE096994.D
 Acq On : 18 Jul 2018 15:26
 Operator : SJ/JU
 Sample : J3967-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DB1E3

Manual Integrations
 APPROVED

Sohil
 7/19/2018 11:36:51 AM

Quant Time: Jul 18 16:38:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 15:28:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	2037	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	11393	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	7997	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	20287m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	22522m	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	19189m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.74	152	6323	0.35	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	21203m	0.34	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Pentachlorophenol	16.43	266	72493m	31.612	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE071818\
Data File : BE096994.D
Acq On : 18 Jul 2018 15:26
Operator : SJ/JU
Sample : J3967-06
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
DB1E3

Manual Integrations
APPROVED

Sohil
7/19/2018 11:36:51 AM

Quant Time: Jul 18 16:38:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 15:28:33 2018
Response via : Initial Calibration

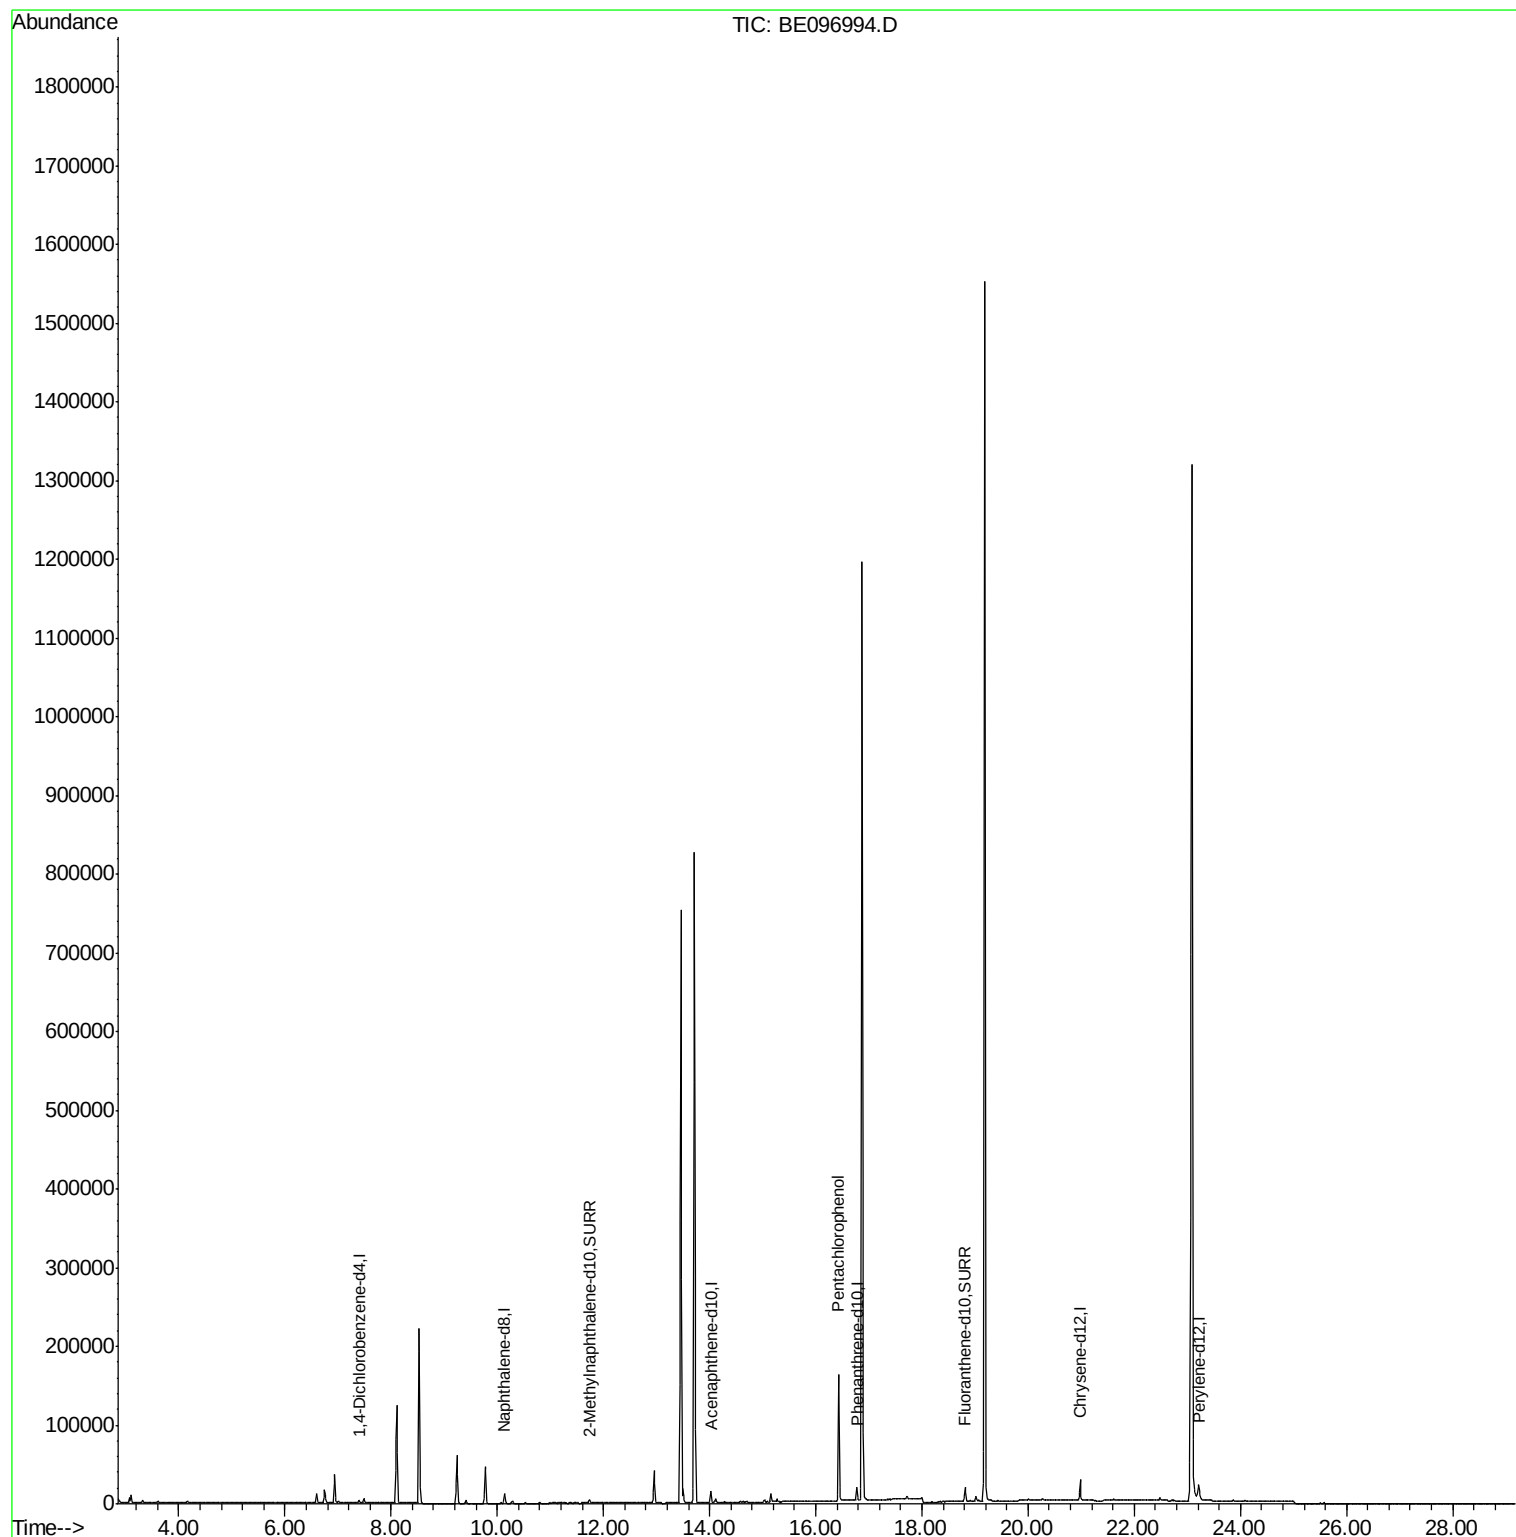

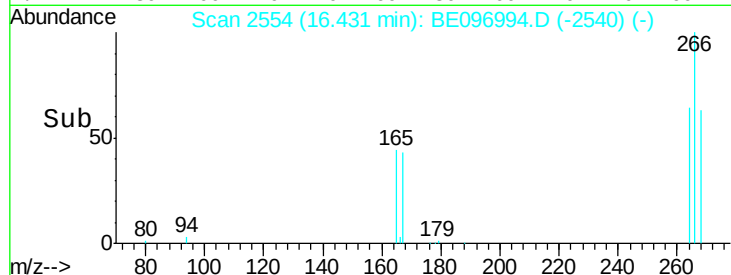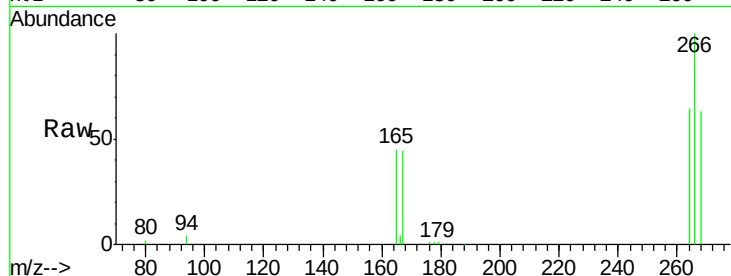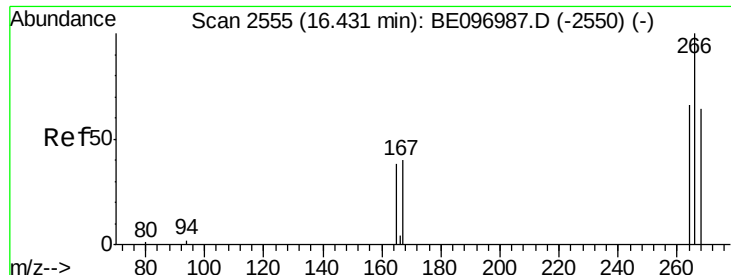

#11
 Pentachlorophenol
 Concen: 31.612 ng/ul m
 RT: 16.43 min Scan# 2554
 Delta R.T. 0.00 min
 Lab File: BE096994.D
 Acq: 18 Jul 2018 15:26

Instrument :
 BNA_E
 ClientSampleId :
 DB1E3

Tgt Ion	Ratio	Resp Lower	Resp Upper
266	100		
264	0.0	47.9	71.9#
268	0.0	49.8	74.8#

Manual Integrations
 APPROVED

Sohil
 7/19/2018 11:36:51 AM

