


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE071918\
 Data File : BE096999.D
 Acq On : 19 Jul 2018 9:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 11:34:20 2018

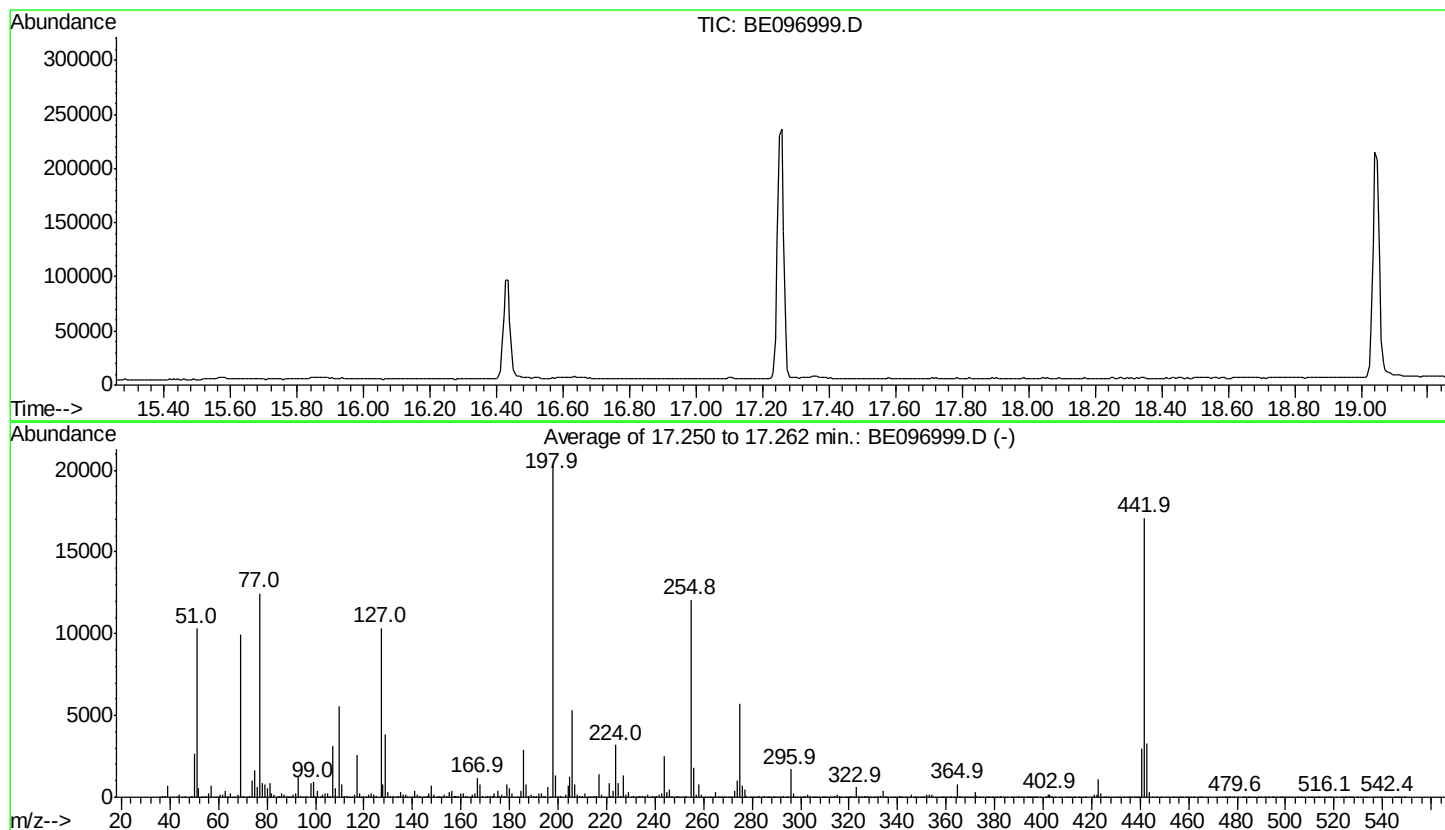

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	10322	PASS
68	69	0.00	2	1.4	140	PASS
69	198	0.00	100	49.1	9960	PASS
70	69	0.00	2	0.6	60	PASS
127	198	10	80	51.1	10370	PASS
197	198	0.00	2	0.1	26	PASS
198	198	100	100	100.0	20283	PASS
199	198	5	9	6.7	1351	PASS
275	198	10	60	28.2	5723	PASS
365	198	1	100	3.9	785	PASS
441	443	0.01	100	89.4	2957	PASS
442	198	50	100	84.3	17095	PASS
443	442	15	24	19.4	3309	PASS