


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071919\  
 Data File : BE100461.D  
 Acq On : 19 Jul 2019 8:47  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE071919.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jul 19 13:59:01 2019

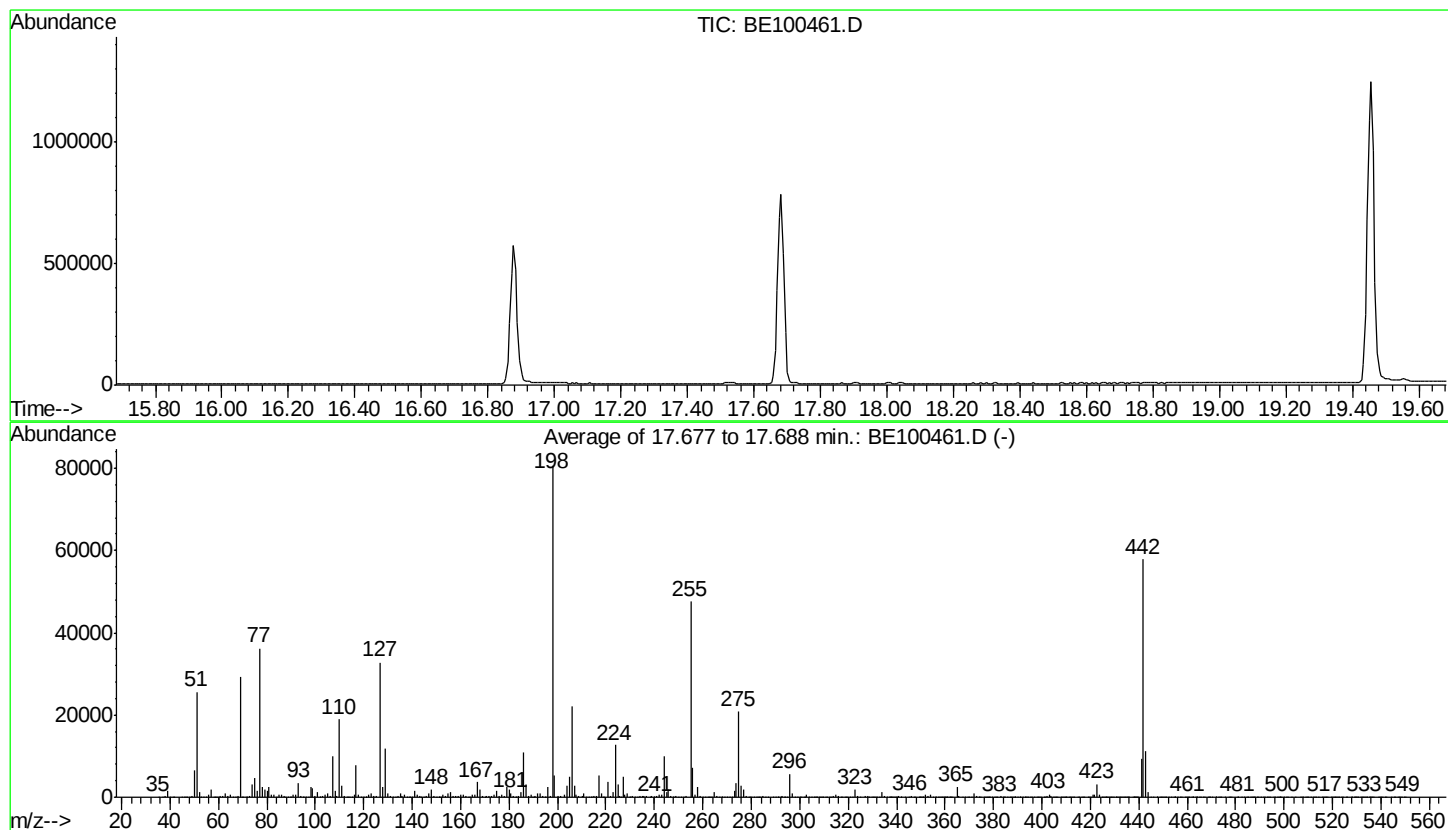

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.7      | 25584   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.6       | 187     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.2      | 29181   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 98      | PASS             |
| 127         | 198          | 10           | 80           | 40.7      | 32838   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 180     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 80642   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 5244    | PASS             |
| 275         | 198          | 10           | 60           | 25.7      | 20713   | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 2582    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.6      | 9388    | PASS             |
| 442         | 198          | 50           | 100          | 71.8      | 57872   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 11262   | PASS             |