


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE072018\
 Data File : BE097015.D
 Acq On : 20 Jul 2018 5:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 11:34:20 2018

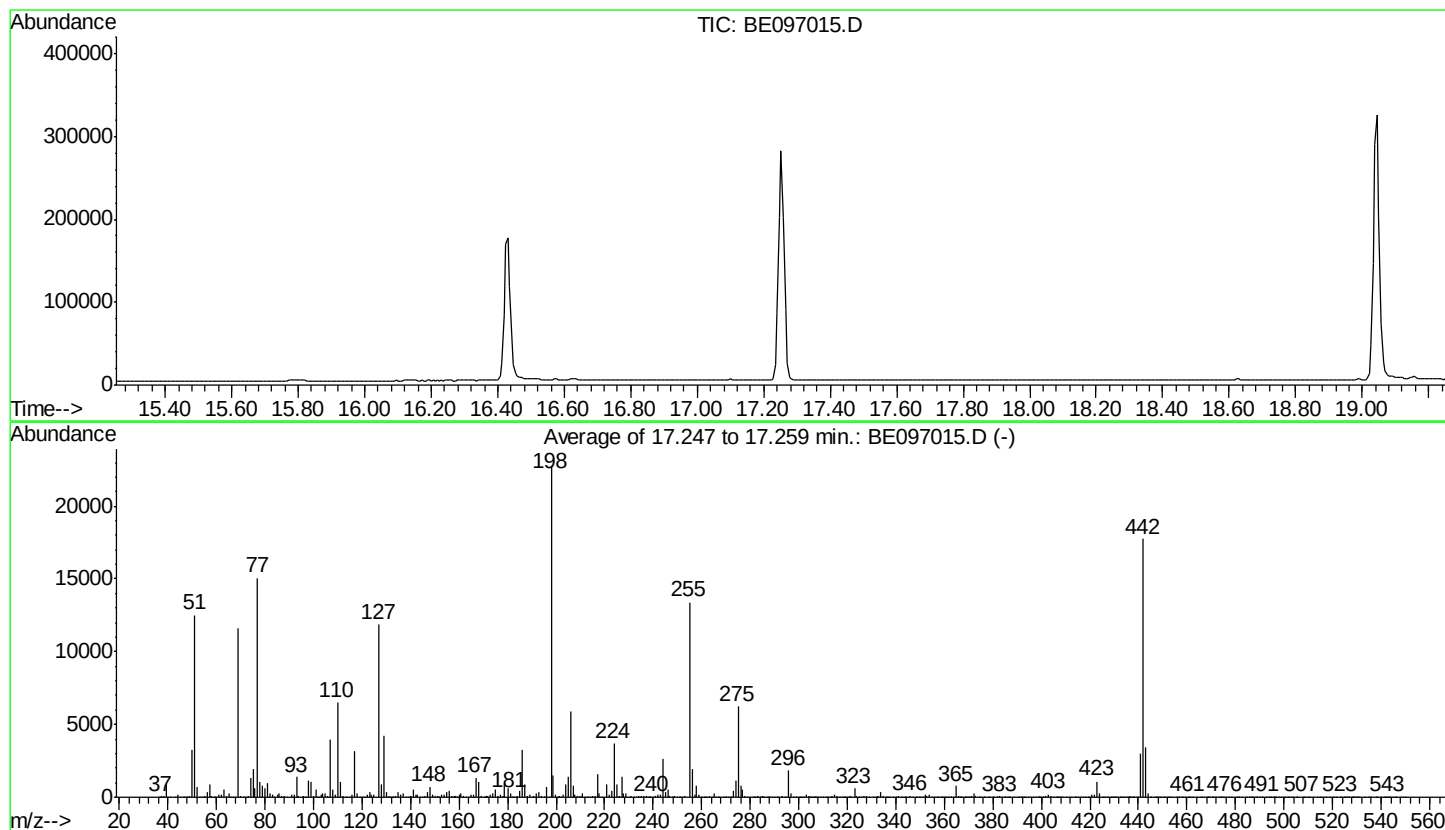

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	12495	PASS
68	69	0.00	2	0.4	41	PASS
69	198	0.00	100	51.0	11622	PASS
70	69	0.00	2	0.5	53	PASS
127	198	10	80	52.0	11854	PASS
197	198	0.00	2	0.2	42	PASS
198	198	100	100	100.0	22786	PASS
199	198	5	9	6.5	1470	PASS
275	198	10	60	27.3	6211	PASS
365	198	1	100	3.4	779	PASS
441	443	0.01	100	86.6	2975	PASS
442	198	50	100	77.9	17757	PASS
443	442	15	24	19.4	3437	PASS