


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072318\
 Data File : BE097029.D
 Acq On : 23 Jul 2018 9:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 11:34:20 2018

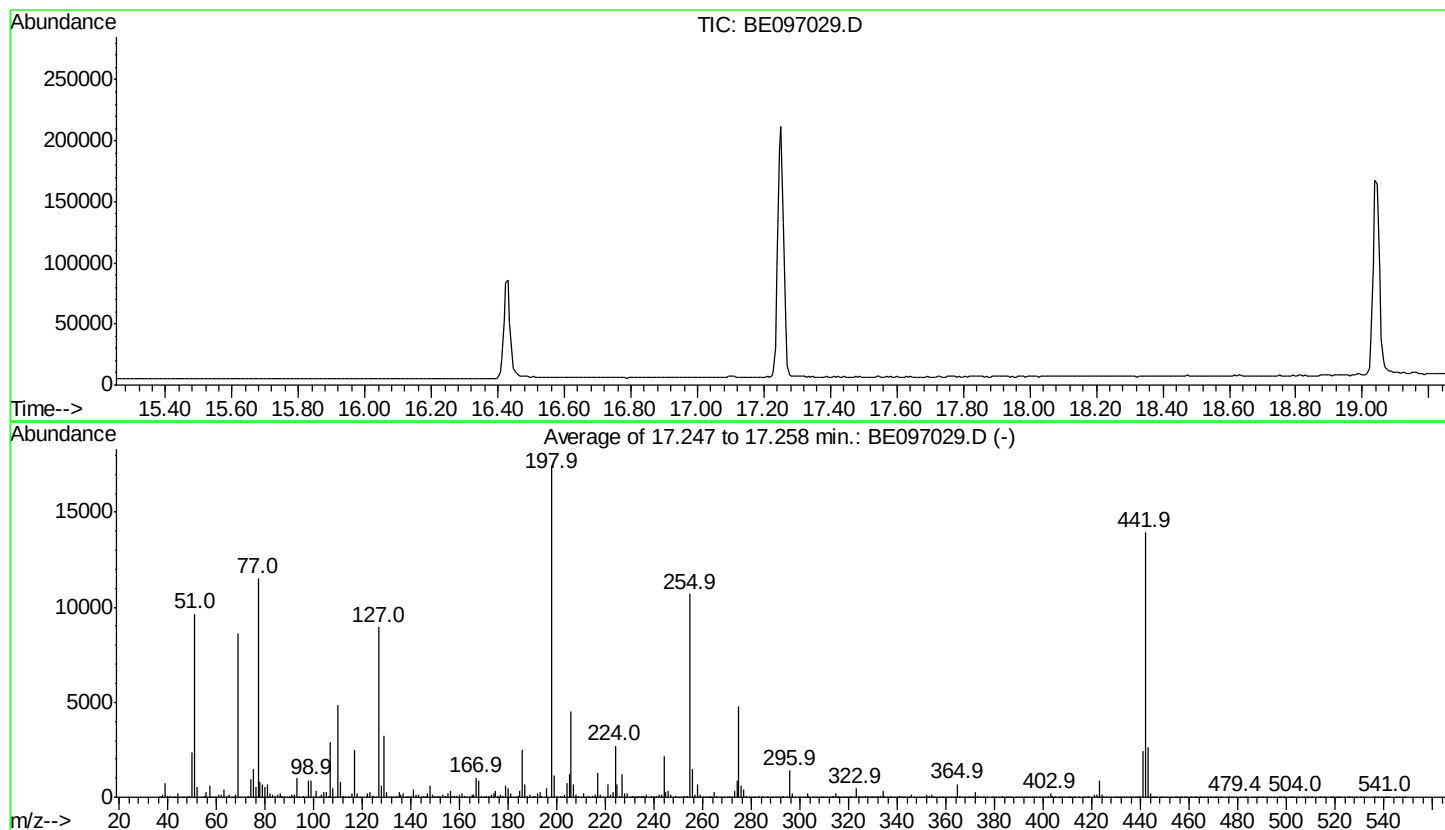

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	9671	PASS
68	69	0.00	2	1.9	163	PASS
69	198	0.00	100	49.4	8626	PASS
70	69	0.00	2	0.1	5	PASS
127	198	10	80	51.2	8938	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17455	PASS
199	198	5	9	6.7	1177	PASS
275	198	10	60	27.3	4762	PASS
365	198	1	100	3.9	683	PASS
441	443	0.01	100	91.7	2424	PASS
442	198	50	100	79.9	13942	PASS
443	442	15	24	19.0	2643	PASS