


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072318\
 Data File : BE097047.D
 Acq On : 23 Jul 2018 22:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 11:34:20 2018

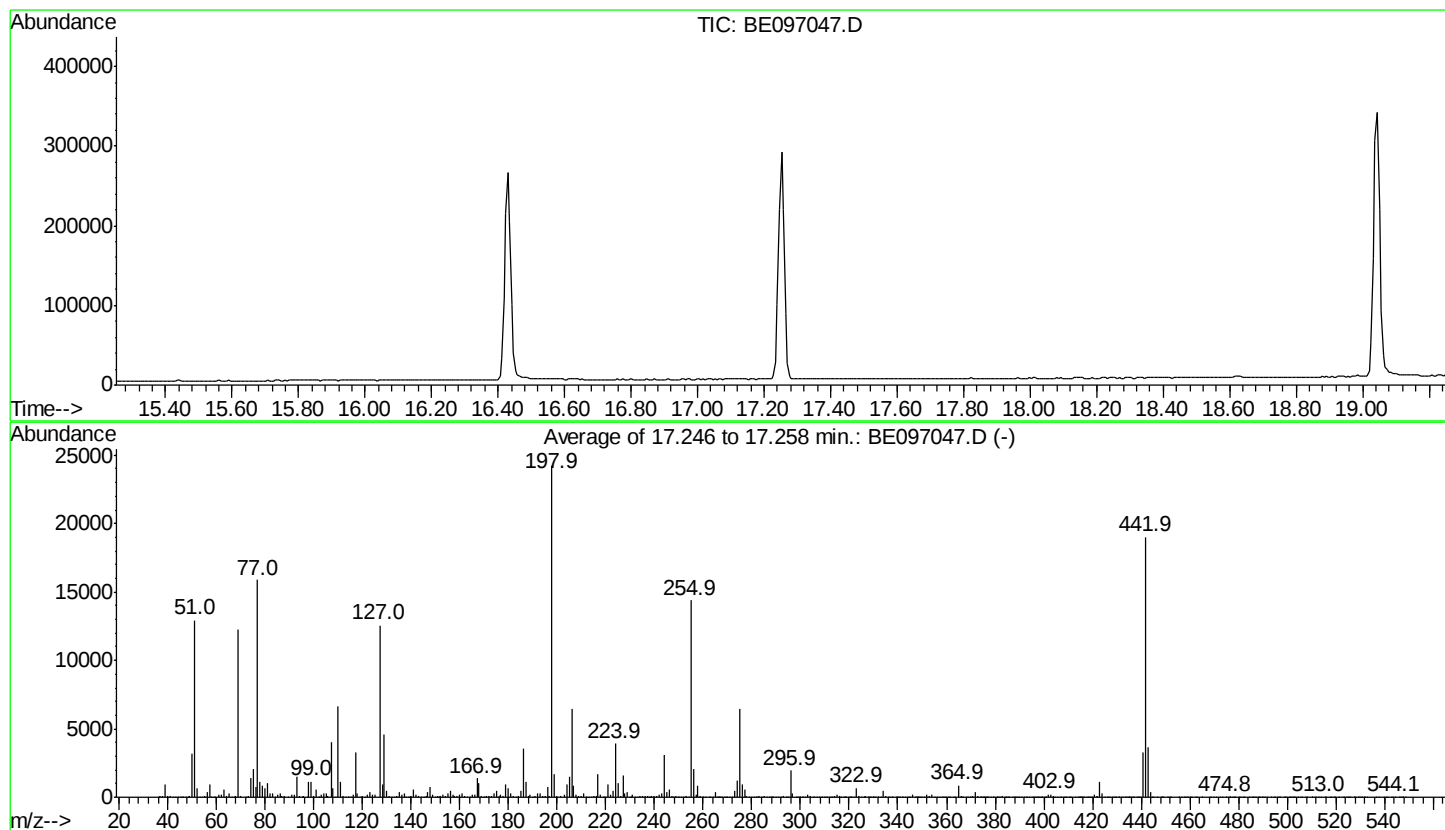

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.4	12941	PASS
68	69	0.00	2	0.6	74	PASS
69	198	0.00	100	50.4	12214	PASS
70	69	0.00	2	0.7	90	PASS
127	198	10	80	51.8	12542	PASS
197	198	0.00	2	0.4	104	PASS
198	198	100	100	100.0	24230	PASS
199	198	5	9	6.8	1659	PASS
275	198	10	60	26.8	6484	PASS
365	198	1	100	3.6	875	PASS
441	443	0.01	100	88.5	3241	PASS
442	198	50	100	78.4	18996	PASS
443	442	15	24	19.3	3661	PASS