
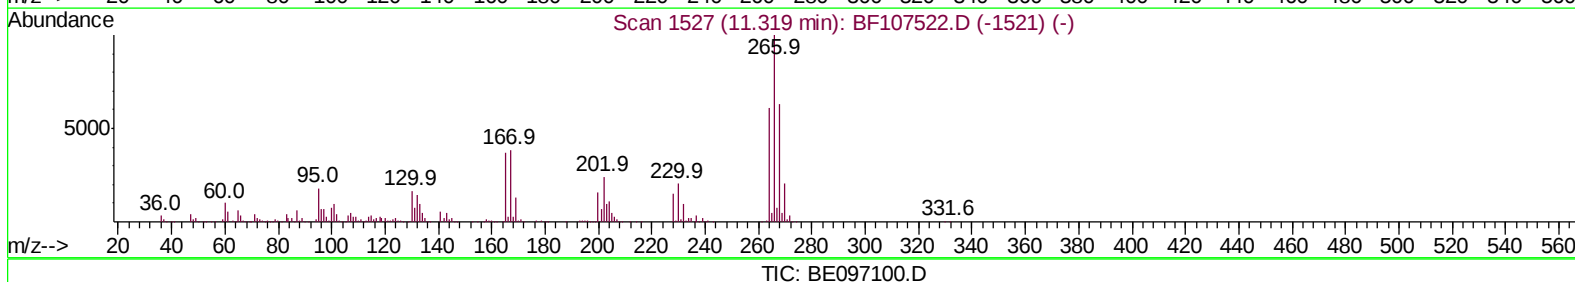
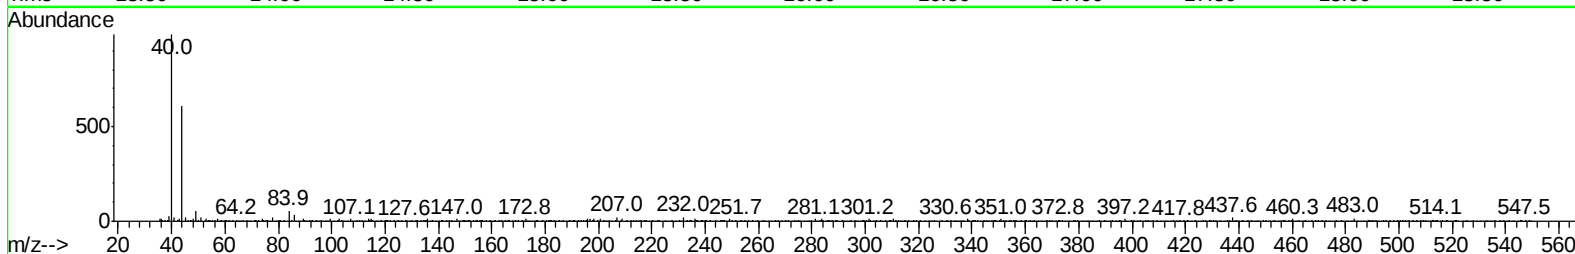


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072618\
 Data File : BE097100.D
 Acq On : 26 Jul 2018 12:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 09:11:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration

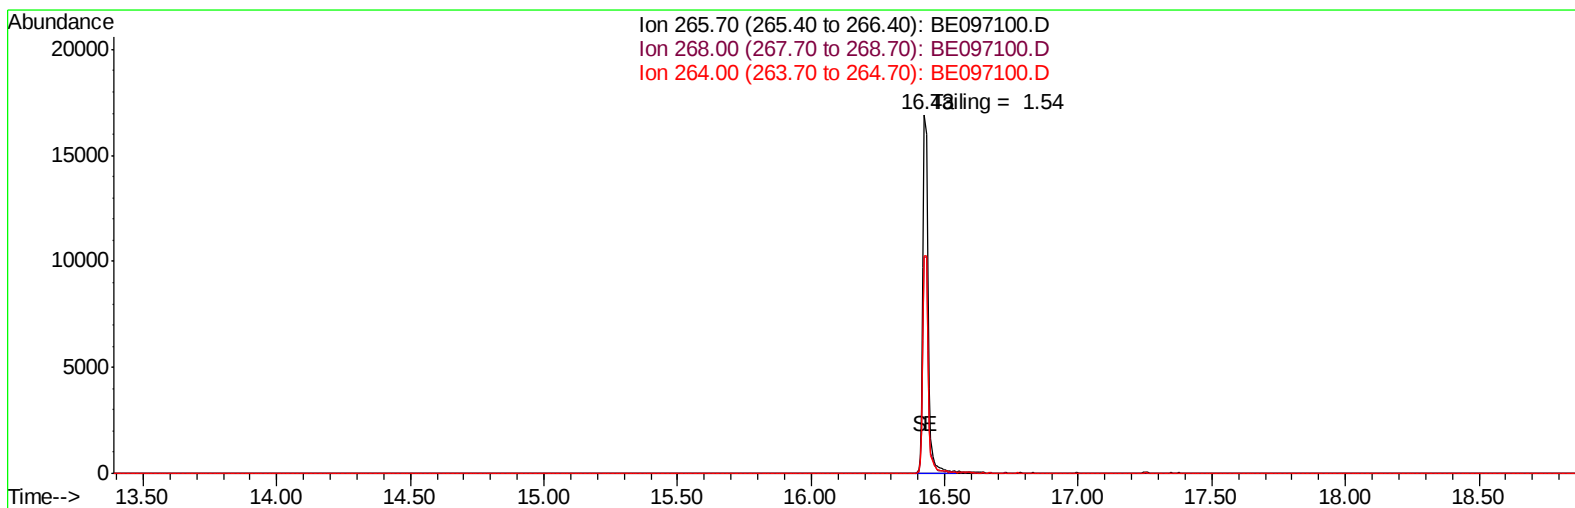

TIC: BE097100.D

(69) Pentachlorophenol (C)




11.360min (+0.042) 29.43ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.67
264.00	61.90	100.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE072618\
 Data File : BE097100.D
 Acq On : 26 Jul 2018 12:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 09:11:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration

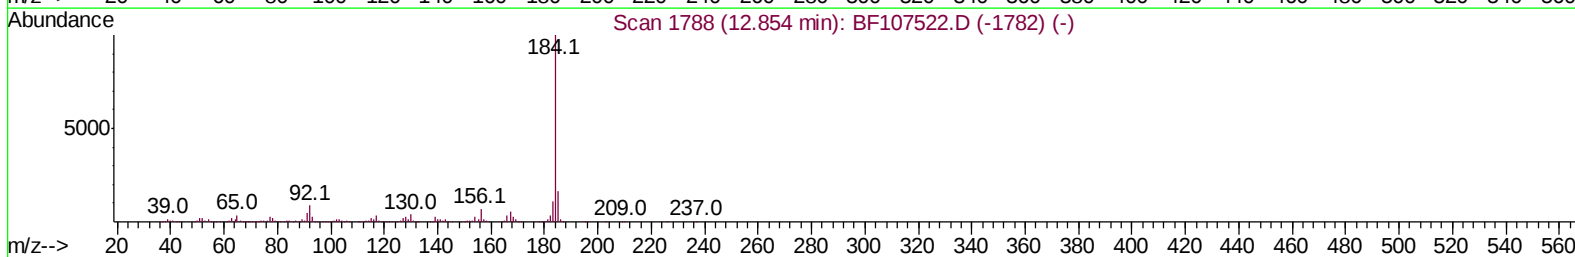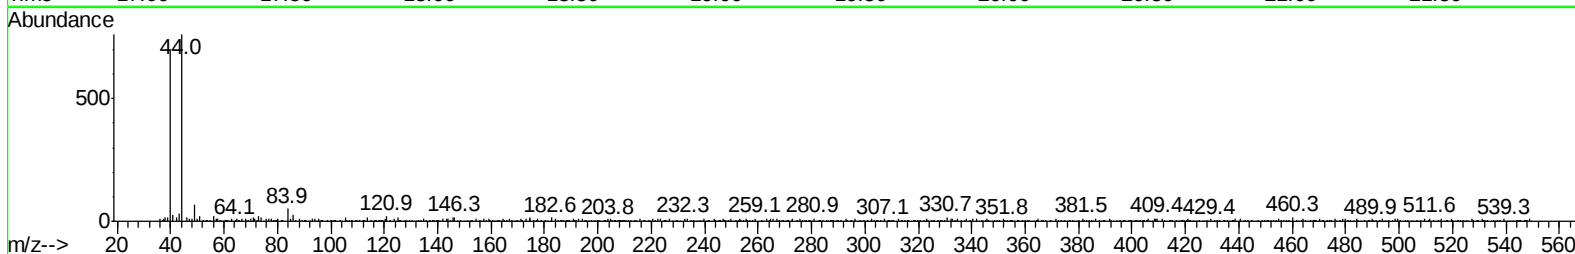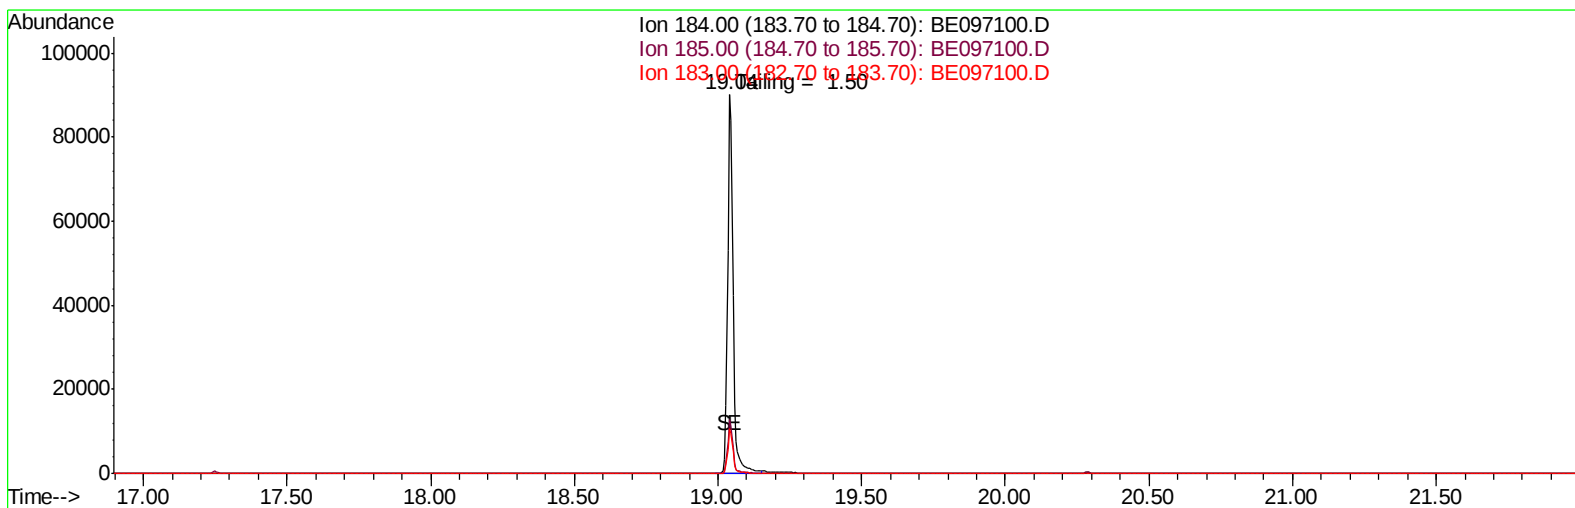

TIC: BE097100.D

(76) Benzidine

12.900min (+0.046) 50.16ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	66.67#
183.00	11.60	0.00#
0.00	0.00	0.00