


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE073118\
 Data File : BE097112.D
 Acq On : 31 Jul 2018 8:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 10:49:28 2018

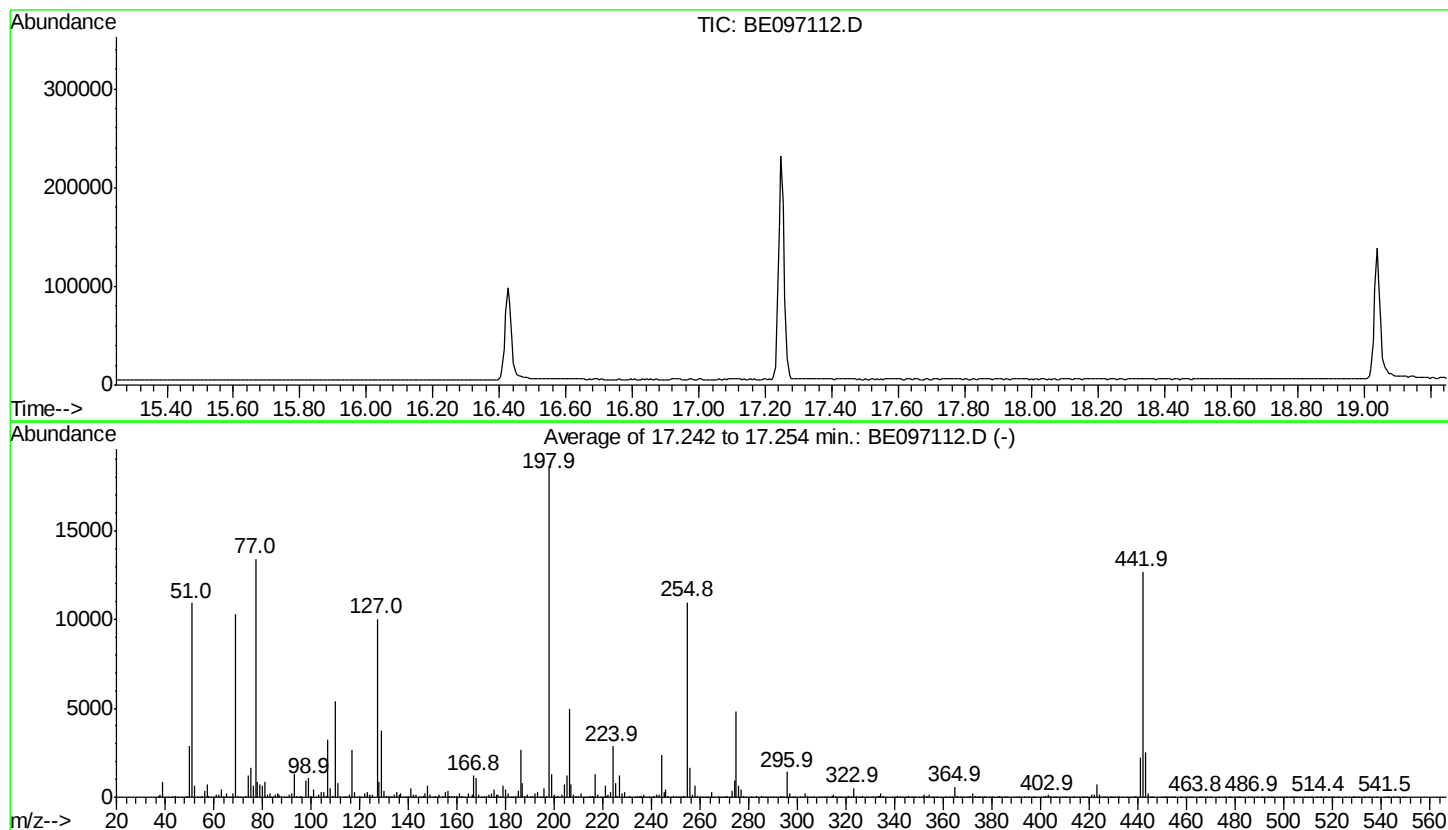

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.7	10947	PASS
68	69	0.00	2	2.0	205	PASS
69	198	0.00	100	55.3	10319	PASS
70	69	0.00	2	0.6	59	PASS
127	198	10	80	53.8	10029	PASS
197	198	0.00	2	0.2	40	PASS
198	198	100	100	100.0	18658	PASS
199	198	5	9	7.1	1316	PASS
275	198	10	60	26.0	4853	PASS
365	198	1	100	3.1	577	PASS
441	198	0.01	100	12.0	2243	PASS
442	198	50	100	68.1	12703	PASS
443	442	15	24	19.8	2516	PASS