

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080118\
 Data File : BE097141.D
 Acq On : 1 Aug 2018 22:32
 Operator : SJ/JU
 Sample : J4149-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1H9

Quant Time: Aug 02 01:50:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 01 16:16:30 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1428	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	7113	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4315	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	11567	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	13749	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	15735	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	902	0.08	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	2960	0.07	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	16.43	266	157	0.095	ng/ul	95
15) Fluoranthene	18.84	202	906	0.023	ng/ul	88
17) Pyrene	19.20	202	1023	0.028	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080118\
Data File : BE097141.D
Acq On : 1 Aug 2018 22:32
Operator : SJ/JU
Sample : J4149-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1H9

Quant Time: Aug 02 01:50:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 01 16:16:30 2018
Response via : Initial Calibration

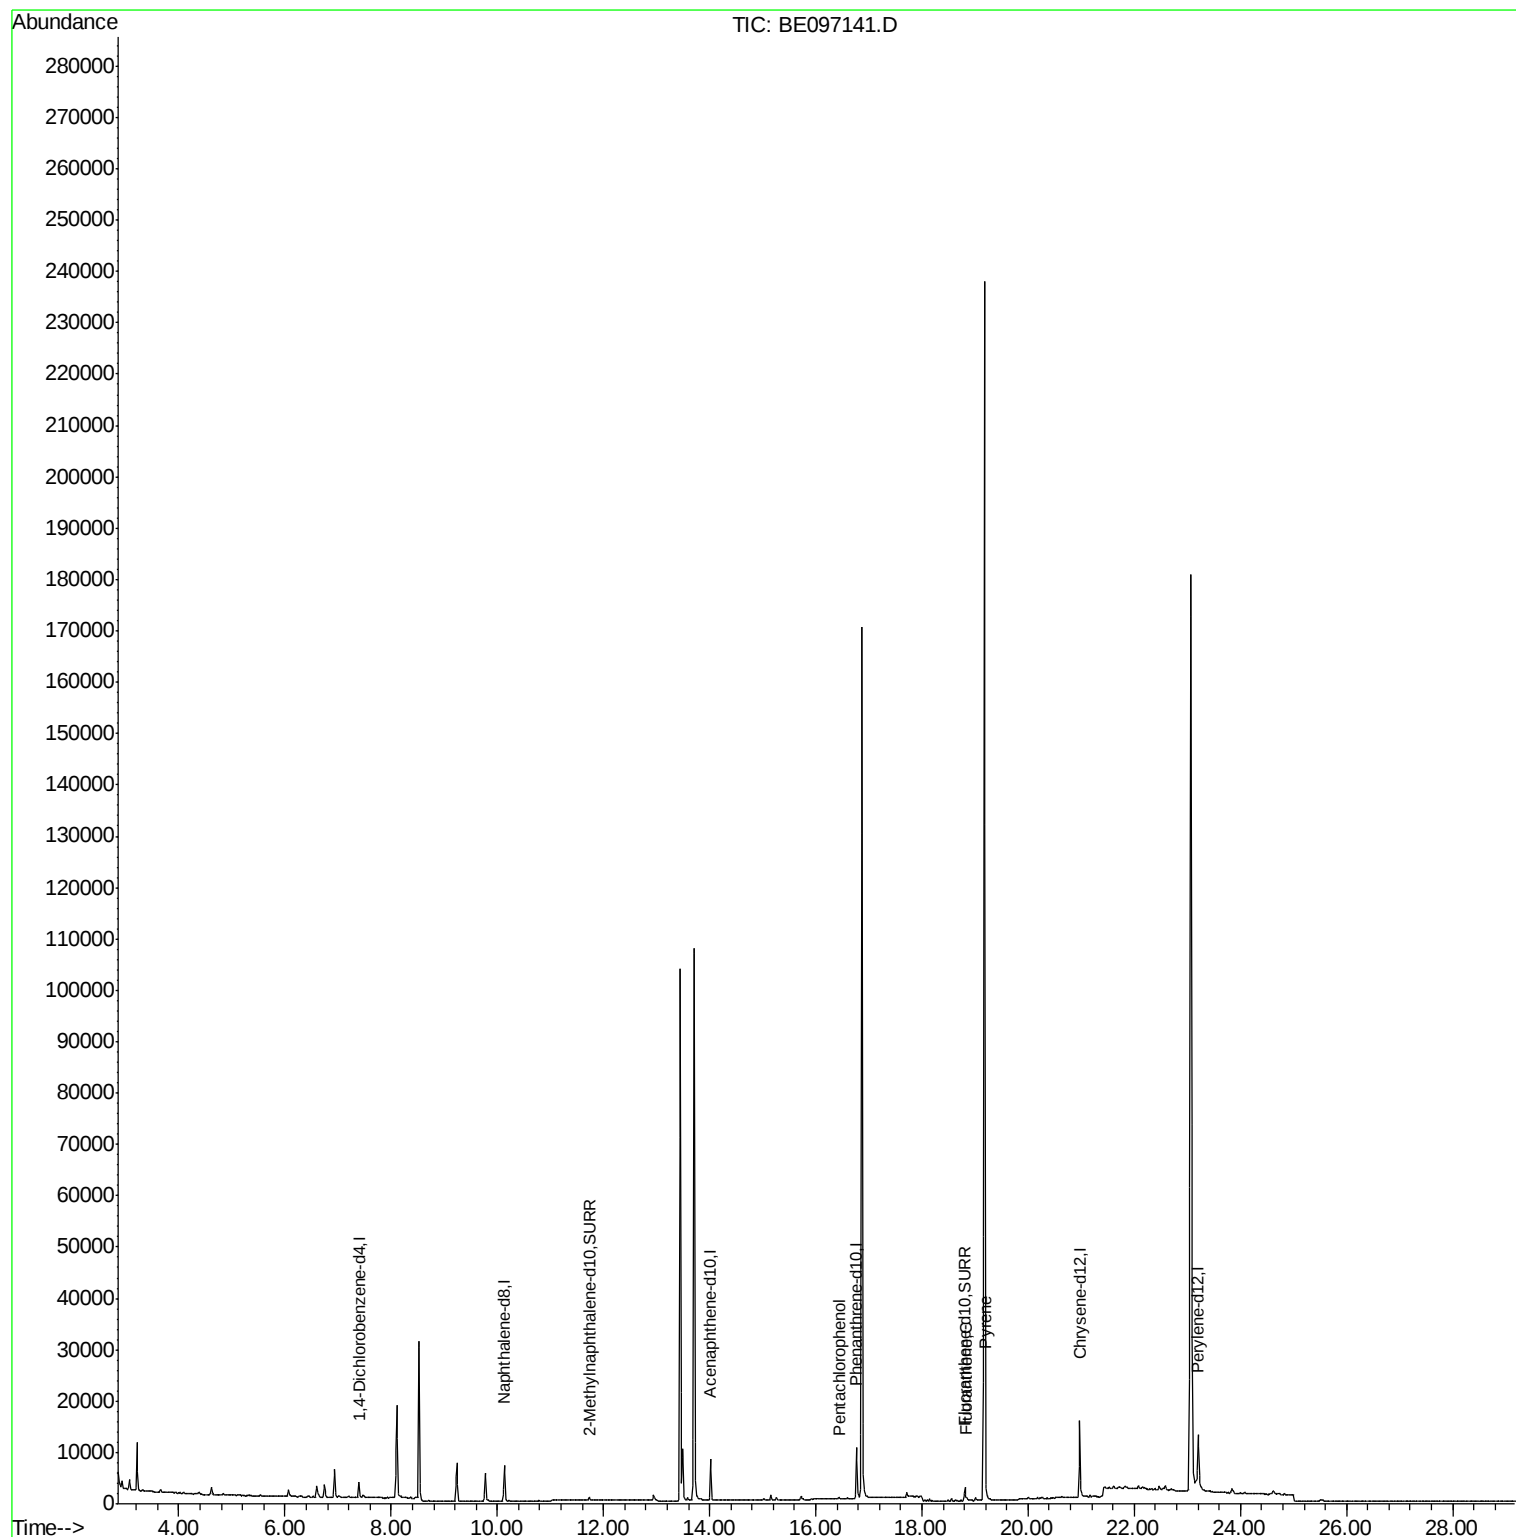


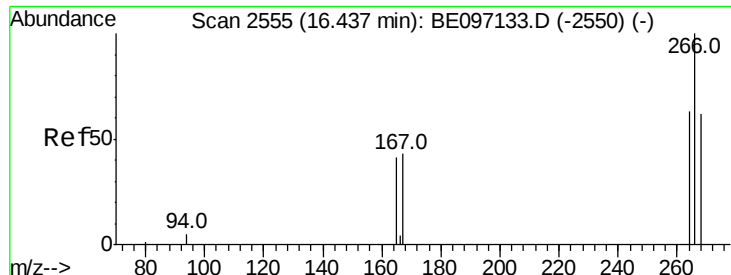




#11
 Pentachlorophenol
 Concen: 0.095 ng/ul
 RT: 16.43 min Scan# 2554
 Delta R.T. -0.01 min
 Lab File: BE097141.D
 Acq: 1 Aug 2018 22:32

Instrument :
 BNA_E
 ClientSampleId :
 JJ1H9

Tot Ion:266 Resp: 157
 Ion Ratio Lower Upper
 266 100
 264 56.7 47.9 71.9
 268 58.6 49.8 74.8

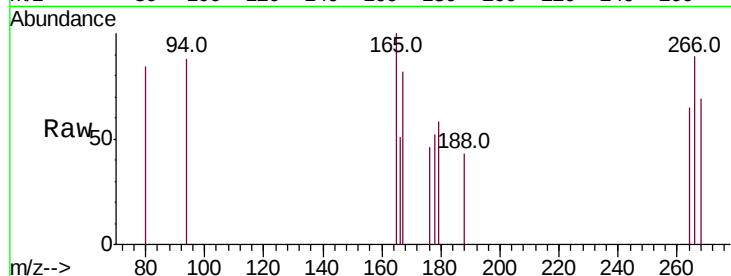


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

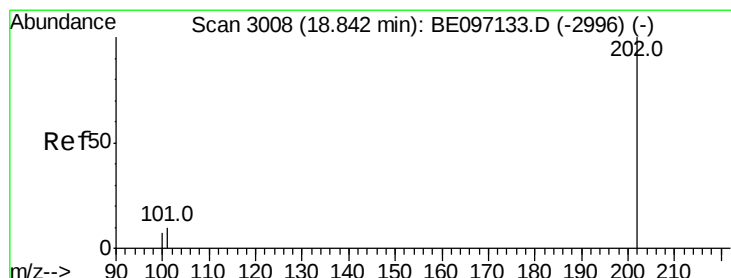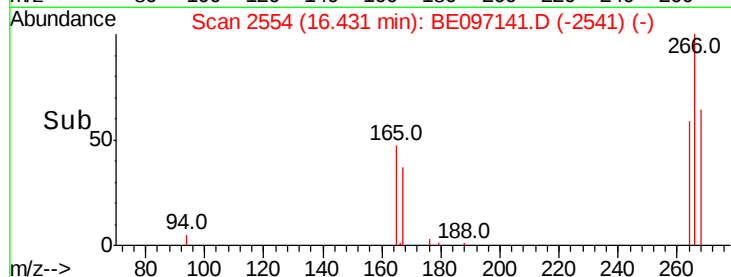
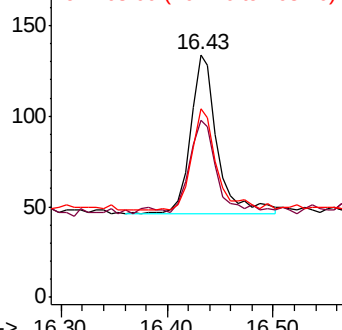



#15
 Fluoranthene
 Concen: 0.023 ng/ul
 RT: 18.84 min Scan# 3008
 Delta R.T. 0.00 min
 Lab File: BE097141.D
 Acq: 1 Aug 2018 22:32

Tgt Ion:202 Resp: 906
 Ion Ratio Lower Upper
 202 100
 101 22.1 0.0 30.3
 100 18.7 0.0 39.5

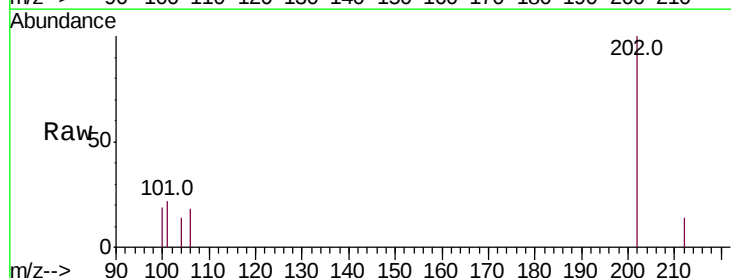

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BE

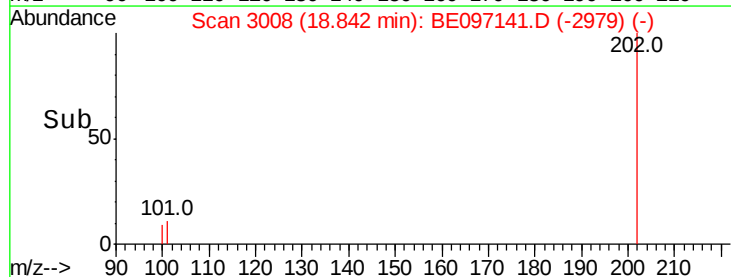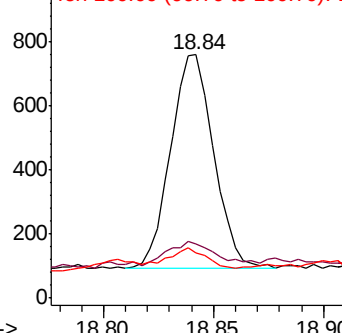

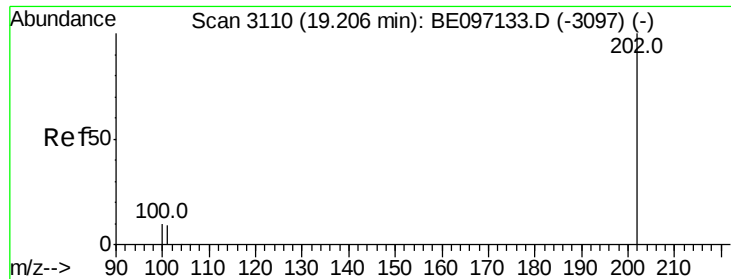

#17
 Pvrene
 Concen: 0.028 ng/ul
 RT: 19.20 min Scan# 3109
 Delta R.T. -0.00 min
 Lab File: BE097141.D
 Acq: 1 Aug 2018 22:32

Instrument :
 BNA_E
 ClientSampleId :
 JJ1H9

Tot Ion:	202	Resp:	1023
Ion	Ratio	Lower	Upper
202	100		
101	25.0	18.2	27.4
100	23.1	15.6	23.4

