

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097146.D
 Acq On : 2 Aug 2018 11:53
 Operator : SJ/JU
 Sample : PB111539BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 02 14:35:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 13:51:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1307	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6548	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3979	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	608340	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.20	264	16348	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	2440	0.23	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.02	166	855	0.060	ng/ul#	23
23) Benzo(a)pyrene	23.06	252	2513	0.056	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097146.D
Acq On : 2 Aug 2018 11:53
Operator : SJ/JU
Sample : PB111539BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 02 14:35:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 13:51:00 2018
Response via : Initial Calibration

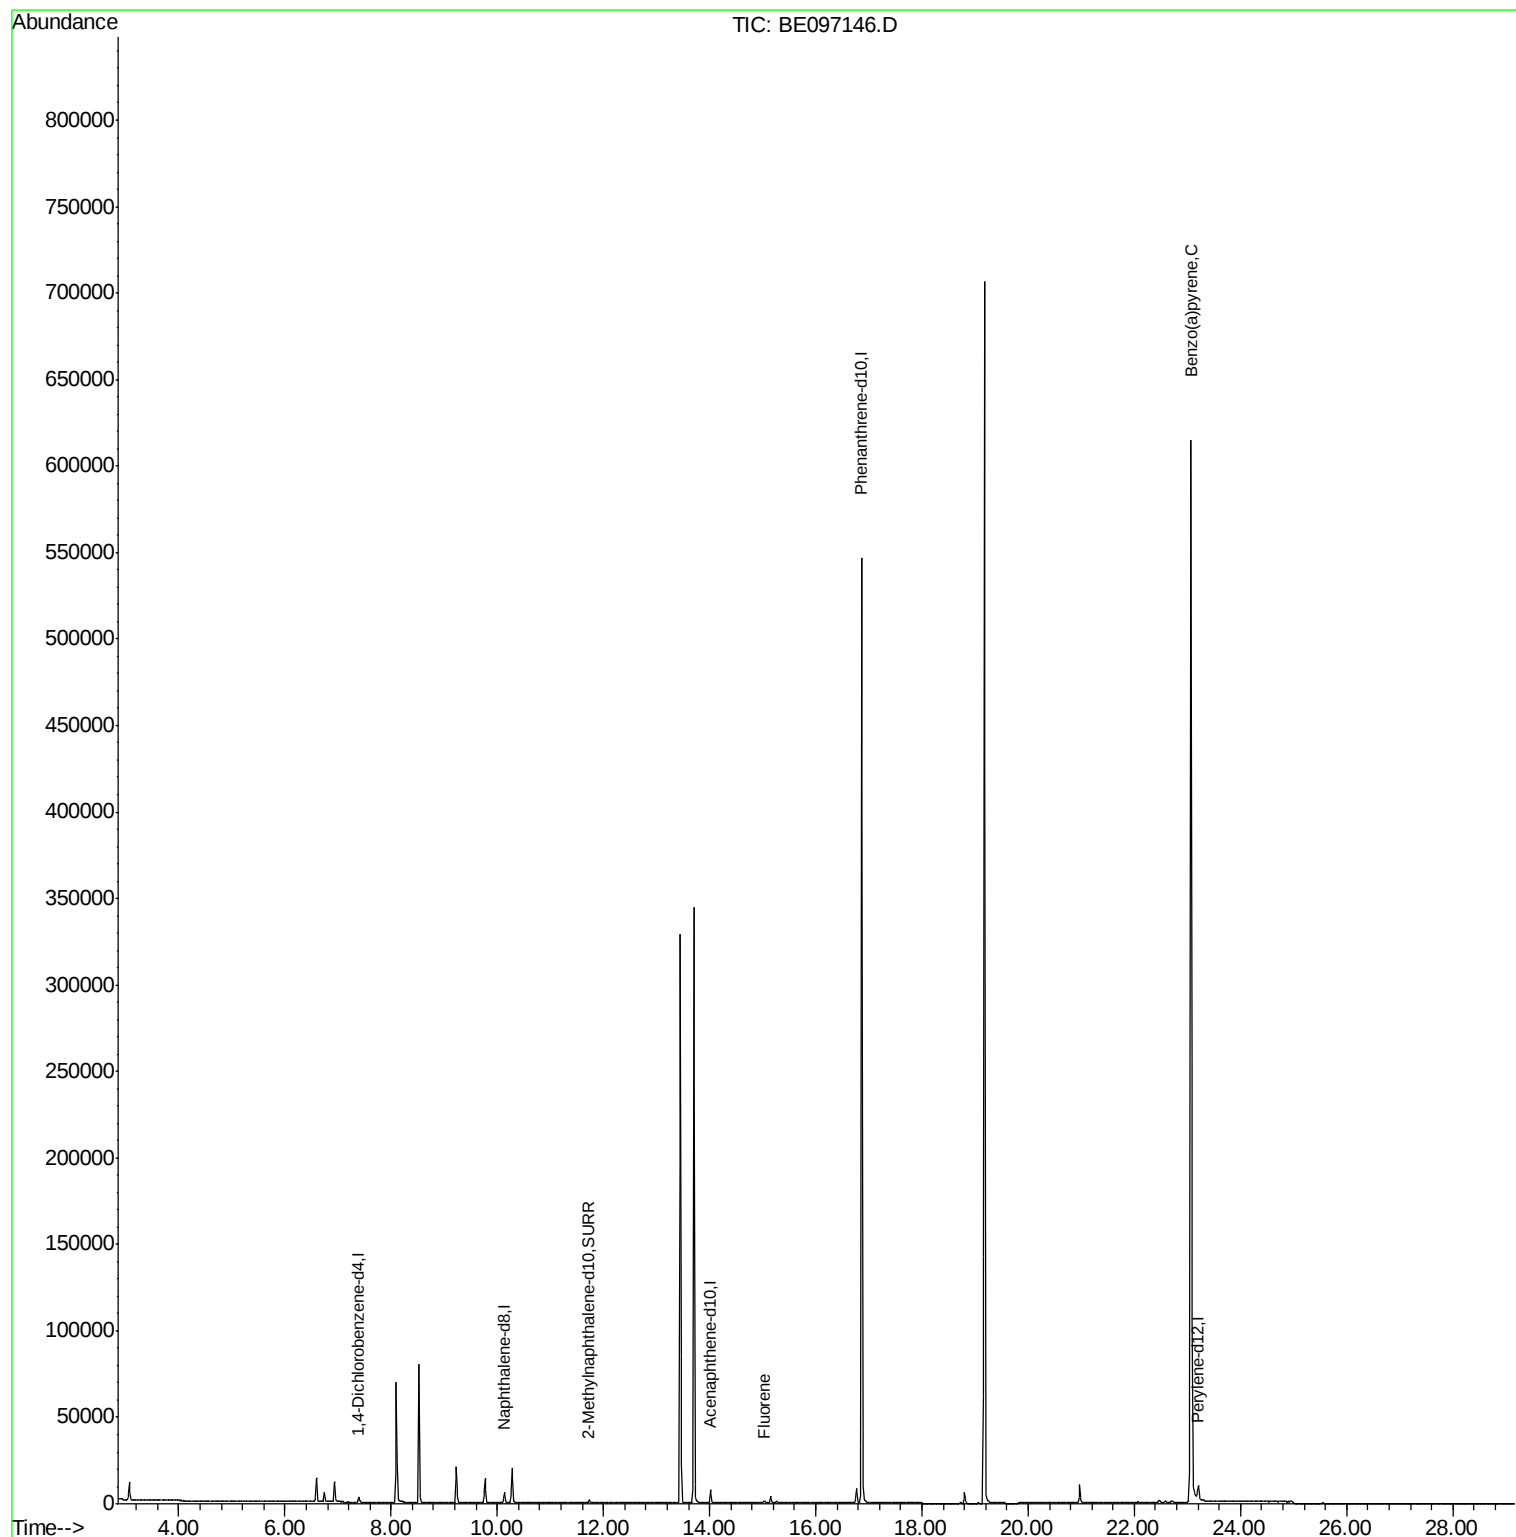

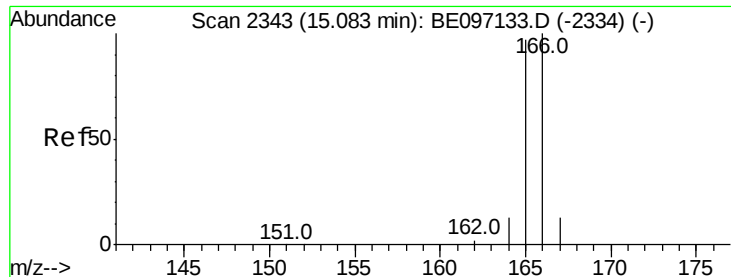

#9

Fluorene

Concen: 0.060 ng/ul

RT: 15.02 min Scan# 2332

Delta R.T. -0.06 min

Lab File: BE097146.D

Acq: 2 Aug 2018 11:53

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 855

Ion Ratio Lower Upper




166 100

165 12.0 73.4 110.2#

167 36.3 14.6 22.0#

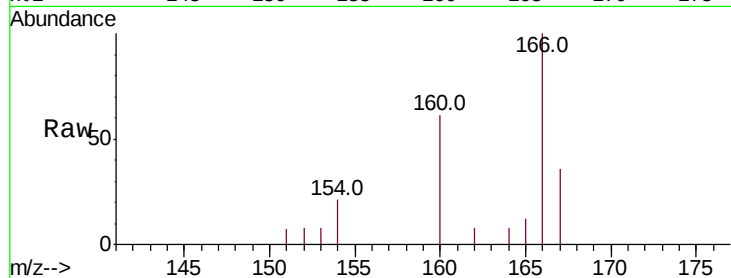

Abundance Ion 166.00 (165.70 to 166.70): E

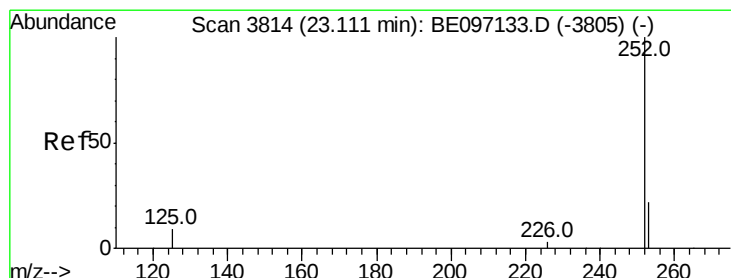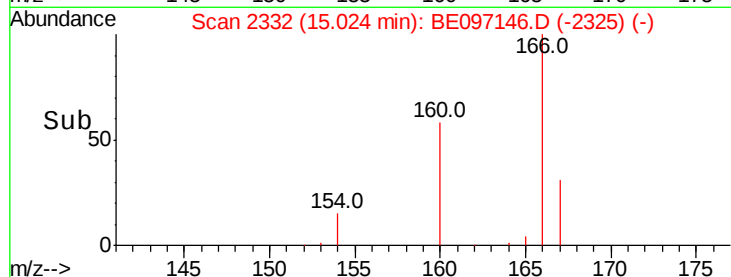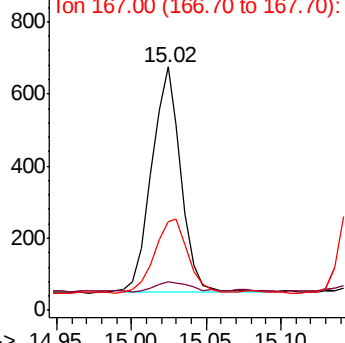

#23

Benzo(a)pyrene

Concen: 0.056 ng/ul

RT: 23.06 min Scan# 3806

Delta R.T. -0.05 min

Lab File: BE097146.D

Acq: 2 Aug 2018 11:53


Tgt Ion:252 Resp: 2513

Ion Ratio Lower Upper

252 100

253 31.8 28.5 42.7

125 23.0 18.1 27.1

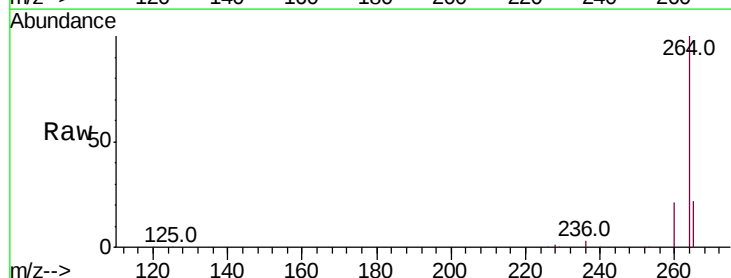

Abundance Ion 252.00 (251.70 to 252.70): E

