

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097150.D
 Acq On : 2 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4149-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1G2

Quant Time: Aug 02 15:05:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1284	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6503	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4076	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	866269	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	17356	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3272	0.31	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.03	166	1118	0.076	ng/ul#	21
23) Benzo(a)pyrene	23.07	252	3582	0.076	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097150.D
Acq On : 2 Aug 2018 14:26
Operator : SJ/JU
Sample : J4149-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1G2

Quant Time: Aug 02 15:05:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

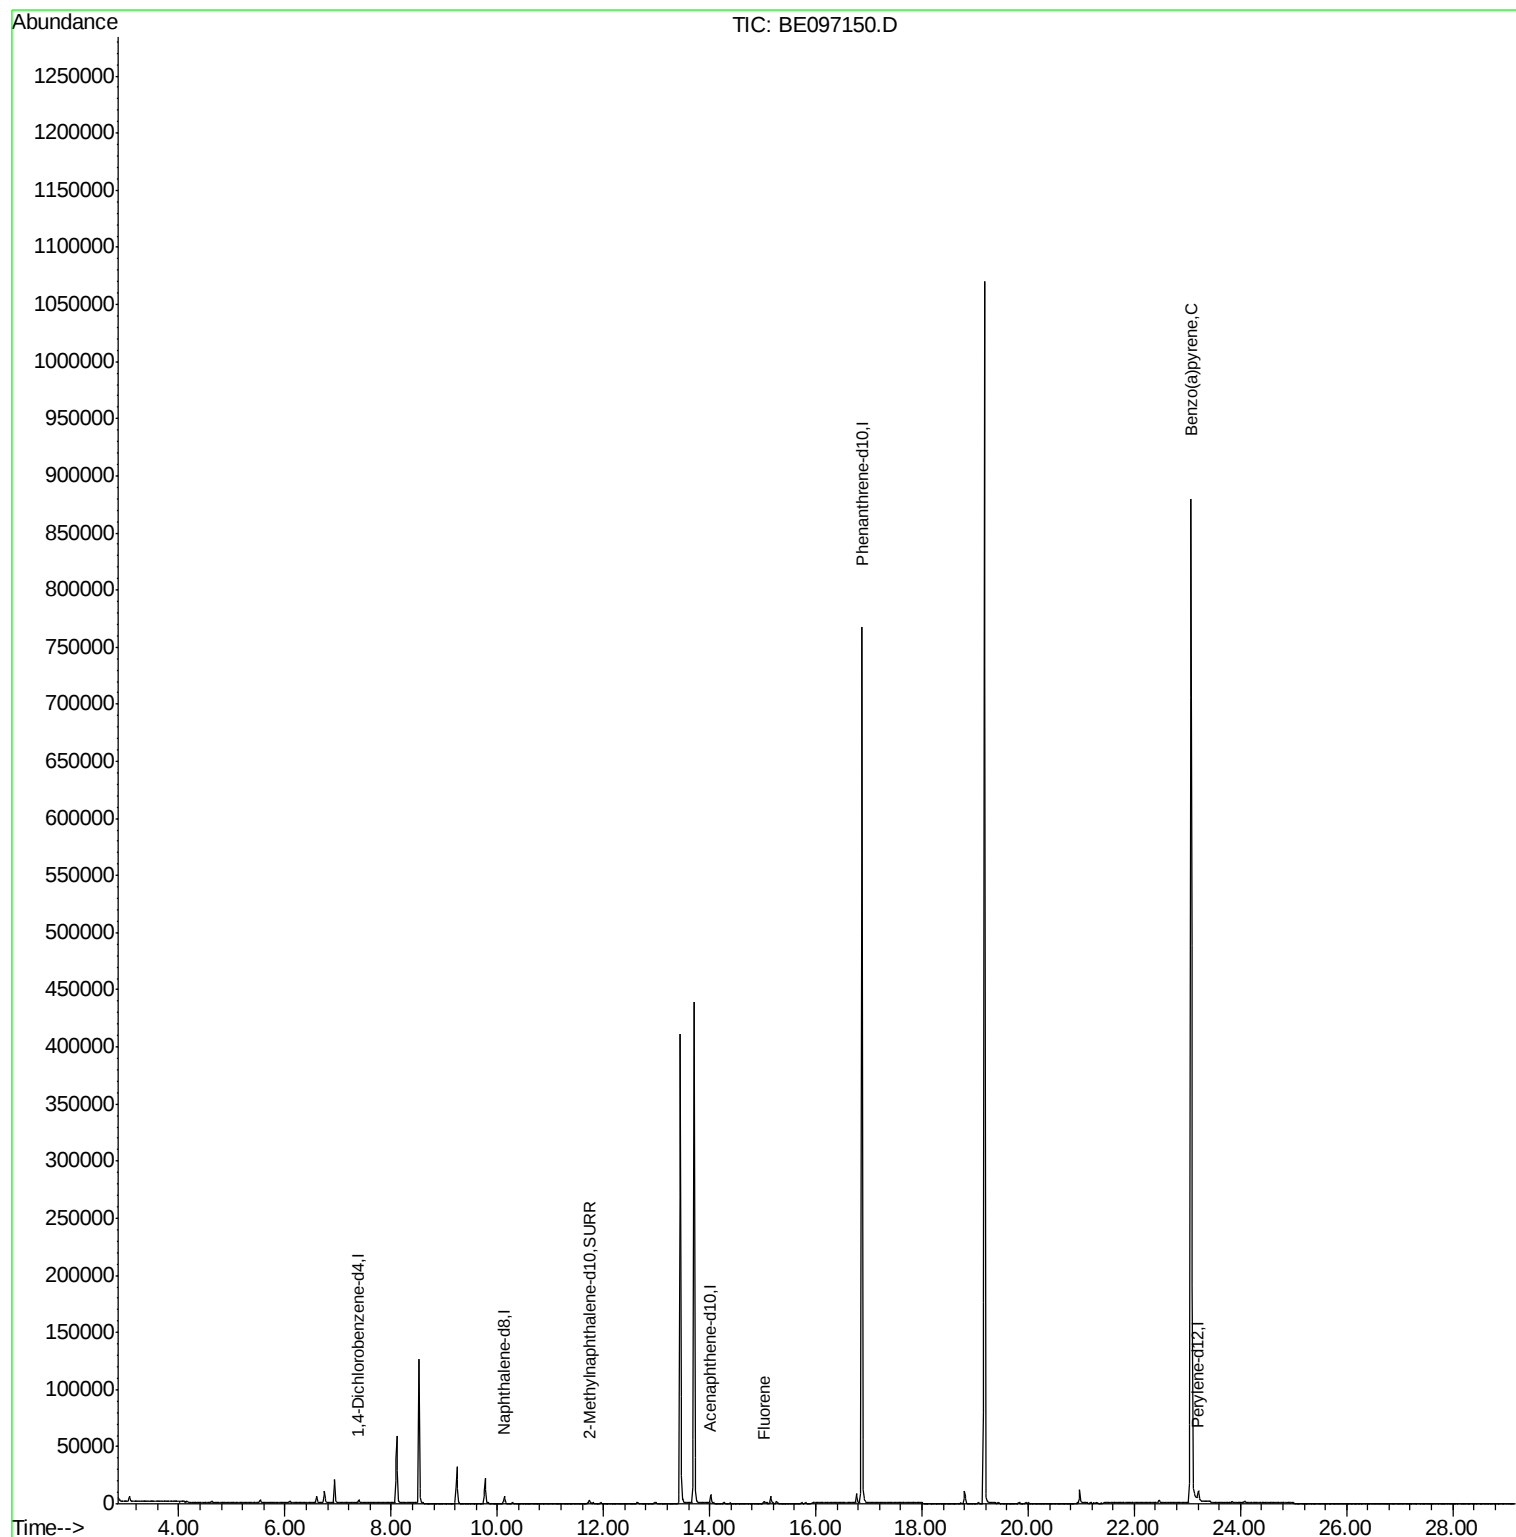

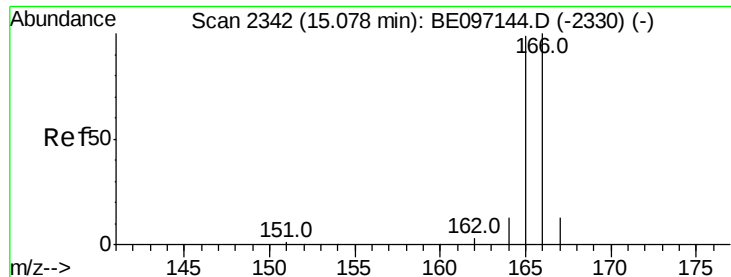

#9

Fluorene

Concen: 0.076 ng/ul

RT: 15.03 min Scan# 2333

Delta R.T. -0.06 min

Lab File: BE097150.D

Acq: 2 Aug 2018 14:26

Instrument :

BNA_E

ClientSampleId :

JJ1G2





Tot Ion:166 Resp: 1118

Ion Ratio Lower Upper

166 100

165 10.6 73.4 110.2#

167 39.6 14.6 22.0#

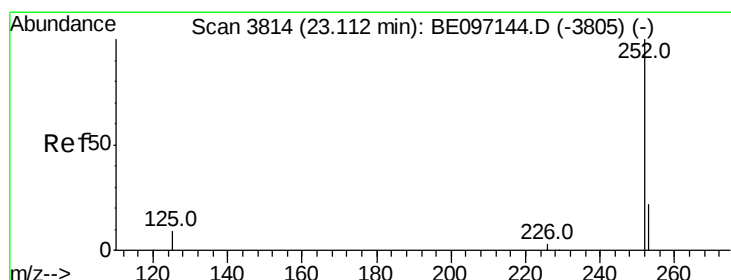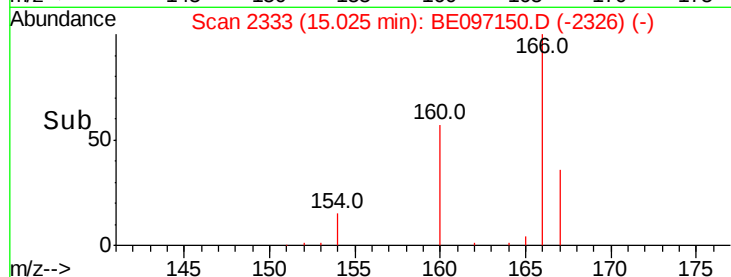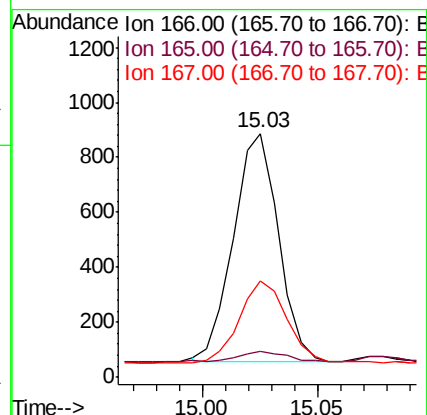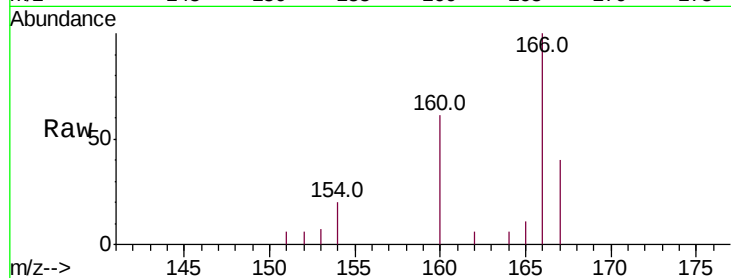

#23

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 23.07 min Scan# 3808

Delta R.T. -0.04 min

Lab File: BE097150.D

Acq: 2 Aug 2018 14:26

Tgt Ion:252 Resp: 3582

Ion Ratio Lower Upper

252 100

253 32.0 28.5 42.7

125 23.6 18.1 27.1

