

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097153.D
 Acq On : 2 Aug 2018 16:19
 Operator : SJ/JU
 Sample : J4149-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1G9

Quant Time: Aug 02 16:59:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1316	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6652	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4258	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	980416	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	18737	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3937	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.03	166	1334	0.087	ng/ul#	20
23) Benzo(a)pyrene	23.08	252	4042	0.079	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097153.D
Acq On : 2 Aug 2018 16:19
Operator : SJ/JU
Sample : J4149-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1G9

Quant Time: Aug 02 16:59:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

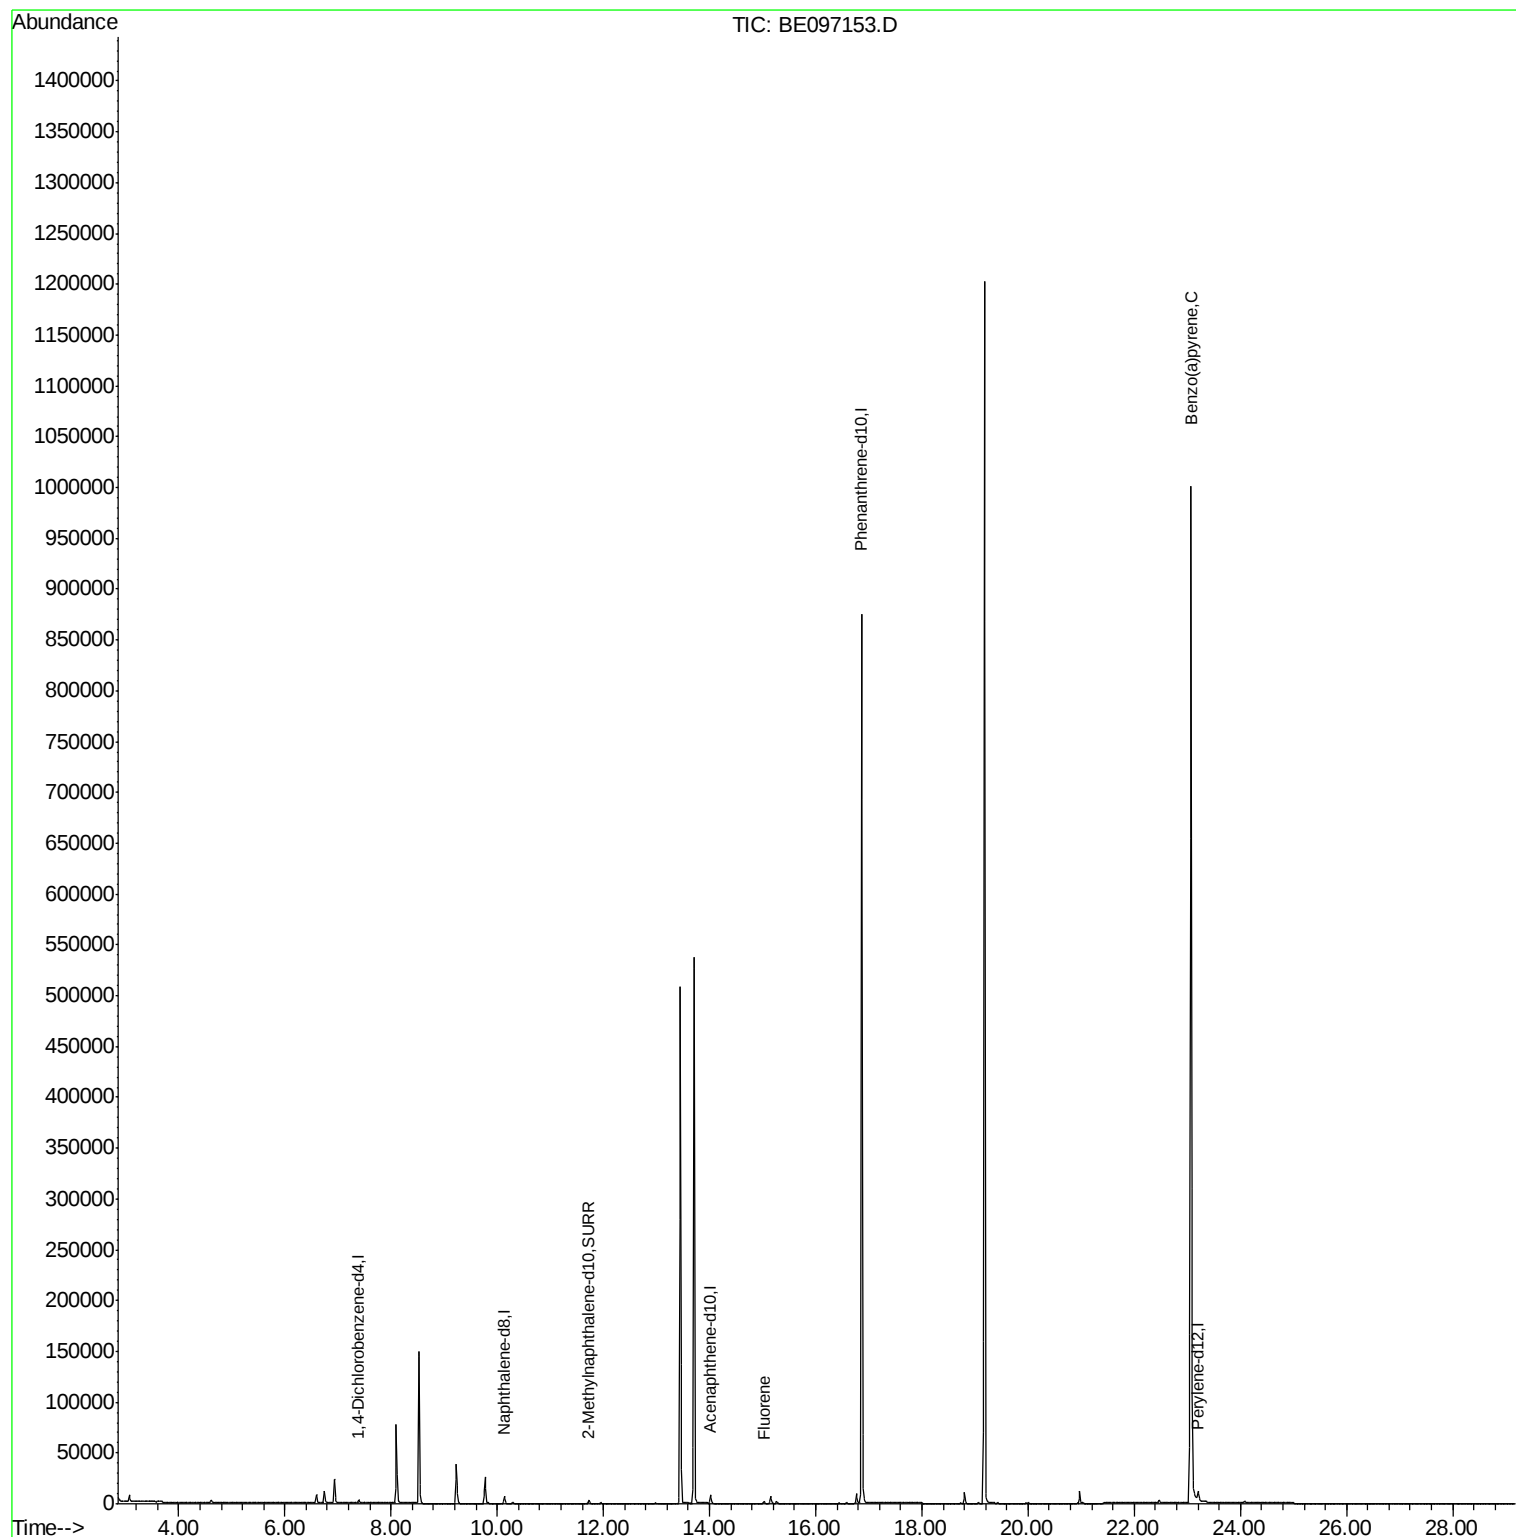

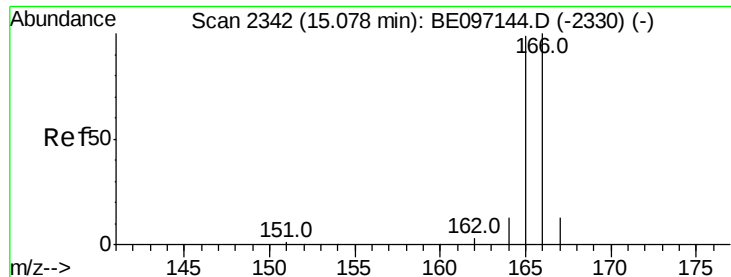

#9

Fluorene

Concen: 0.087 ng/ul

RT: 15.03 min Scan# 2333

Delta R.T. -0.06 min

Lab File: BE097153.D

Acq: 2 Aug 2018 16:19

Instrument :

BNA_E

ClientSampleId :

JJ1G9


Tot Ion:166 Resp: 1334

Ion Ratio Lower Upper

166 100

165 8.7 73.4 110.2#




167 38.1 14.6 22.0#

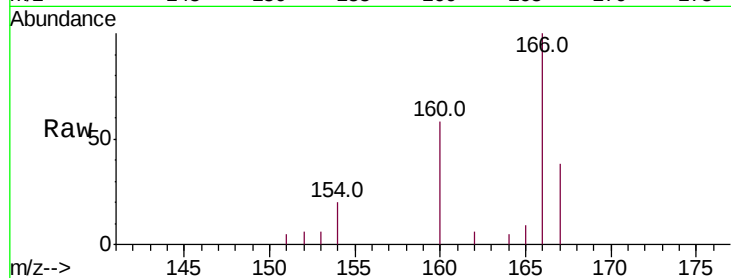

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

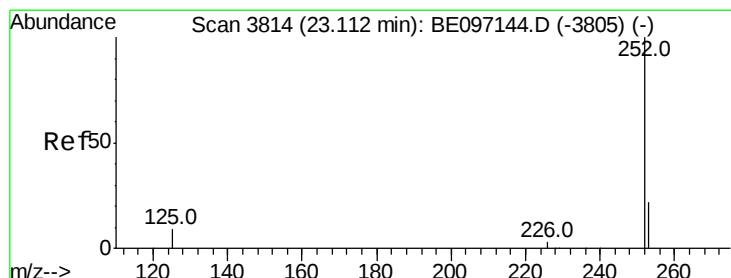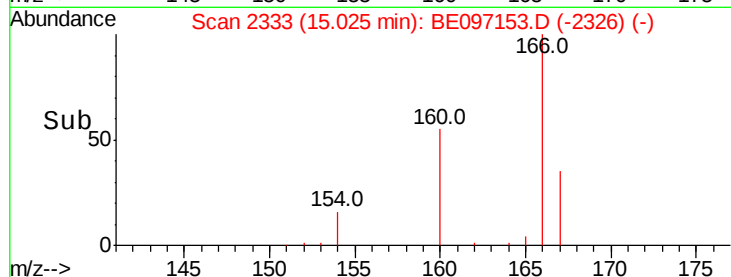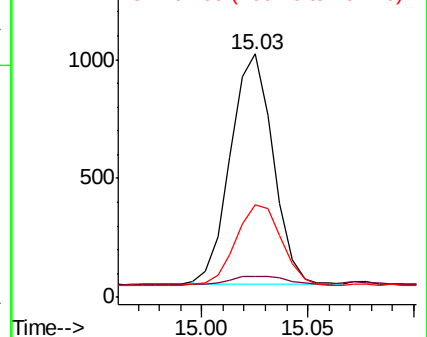

#23

Benzo(a)pyrene

Concen: 0.079 ng/ul

RT: 23.08 min Scan# 3809

Delta R.T. -0.04 min

Lab File: BE097153.D

Acq: 2 Aug 2018 16:19


Tgt Ion:252 Resp: 4042

Ion Ratio Lower Upper

252 100

253 31.2 28.5 42.7

125 19.8 18.1 27.1

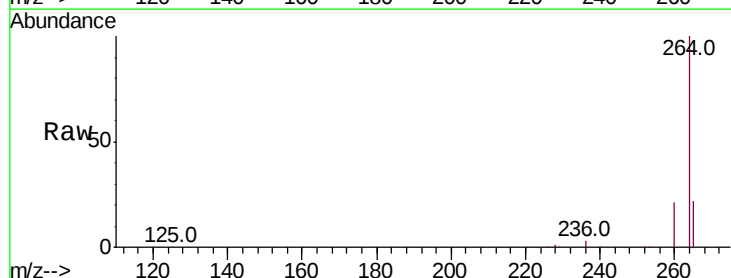

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

