

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097155.D
 Acq On : 2 Aug 2018 17:34
 Operator : SJ/JU
 Sample : J4149-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1G7

Quant Time: Aug 02 18:13:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1230	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6117	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3982	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	876676	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	17296	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3679	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.07	252	3673	0.078	ng/ul	Ovalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097155.D
Acq On : 2 Aug 2018 17:34
Operator : SJ/JU
Sample : J4149-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1G7

Quant Time: Aug 02 18:13:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

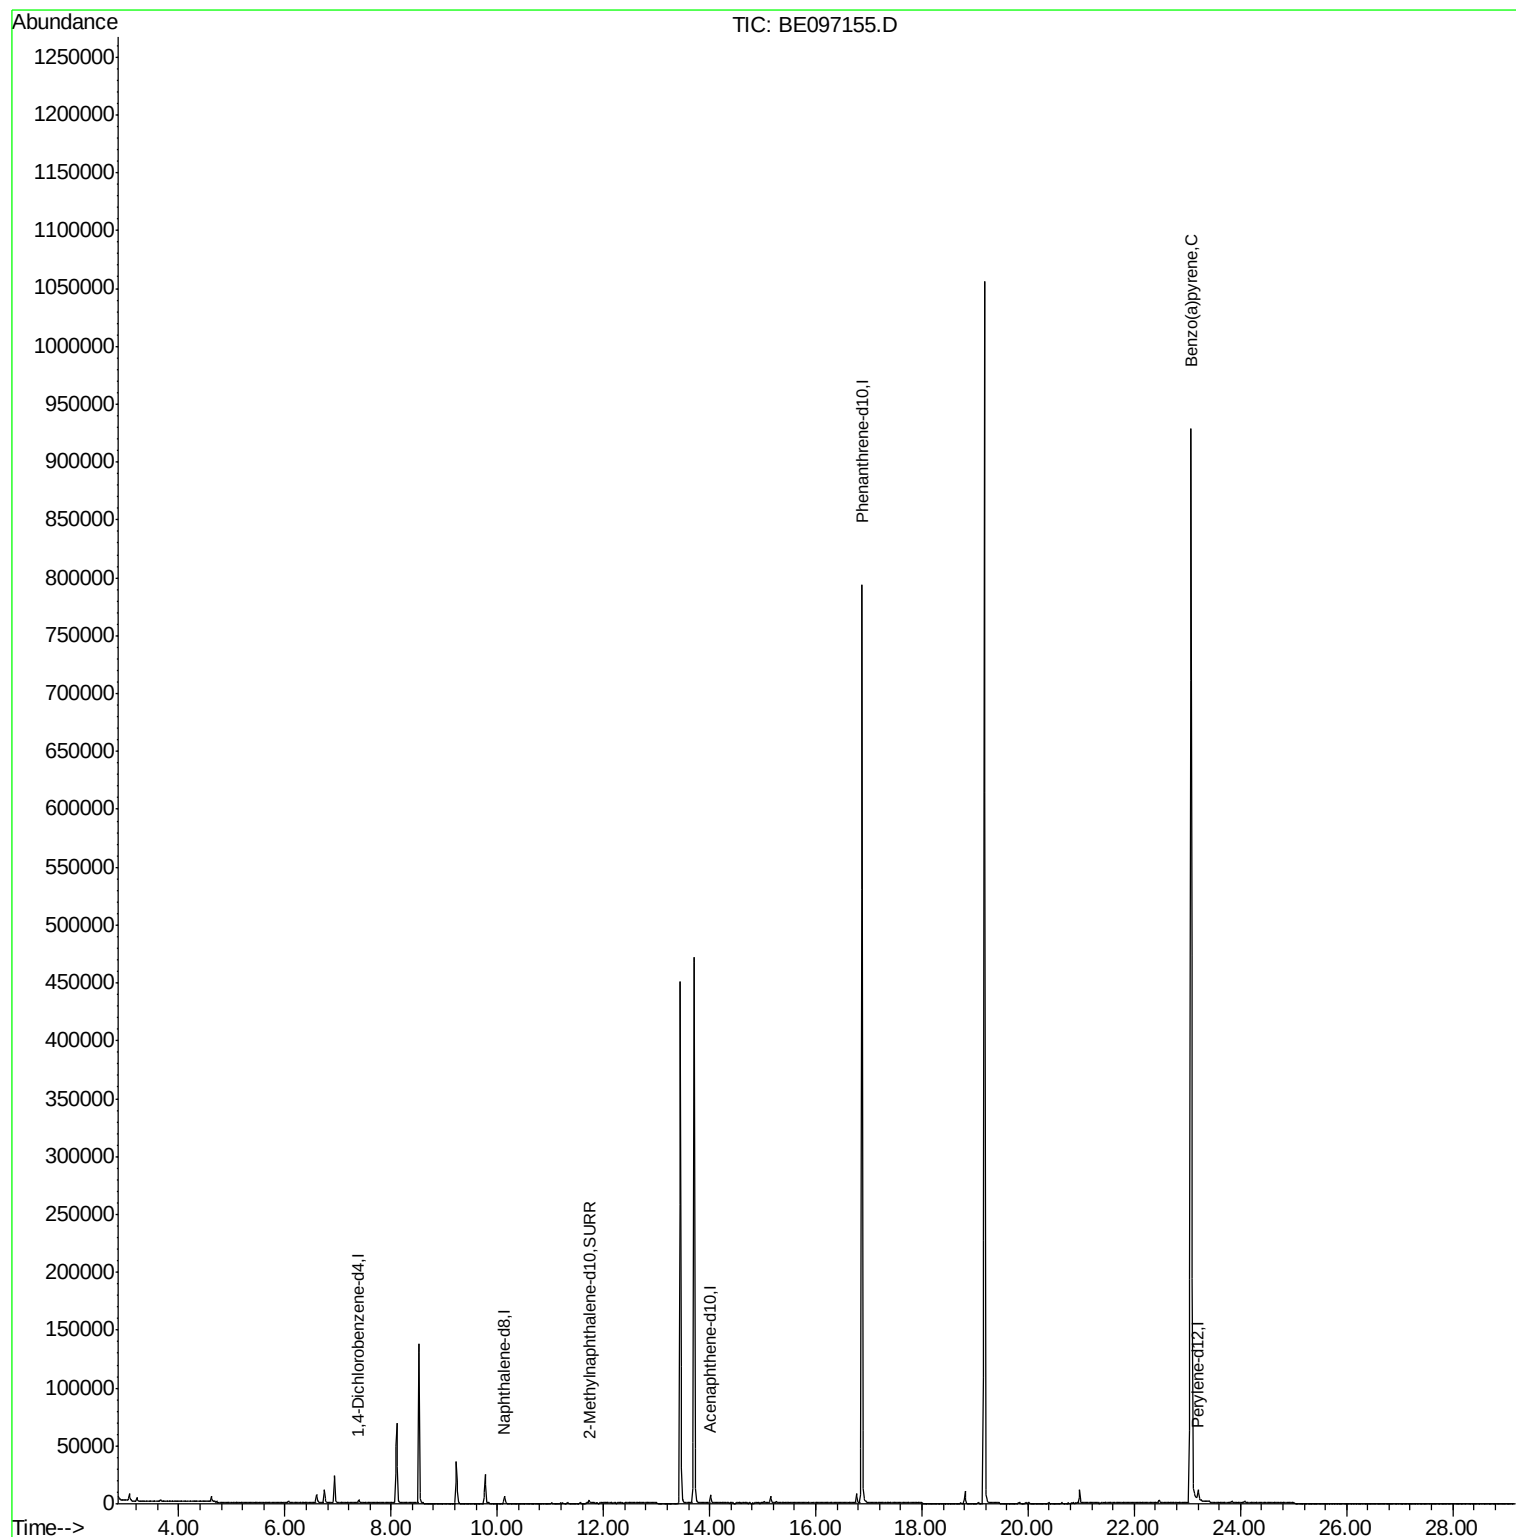

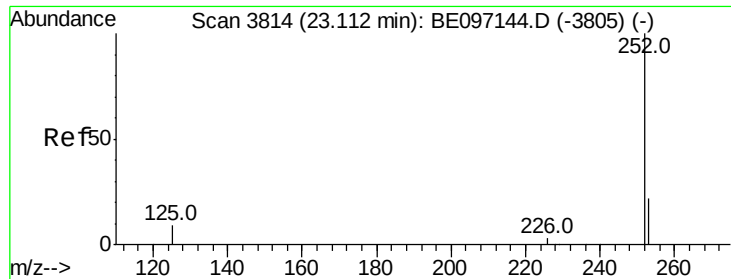

#23

Benzo(a)pyrene

Concen: 0.078 ng/ul

RT: 23.07 min Scan# 3808

Delta R.T. -0.04 min

Lab File: BE097155.D

Acq: 2 Aug 2018 17:34

Instrument :

BNA_E

ClientSampleId :

JJ1G7


Tot Ion: 252 Resp: 3673

Ion Ratio Lower Upper

252 100

253 30.4 28.5 42.7

125 21.2 18.1 27.1

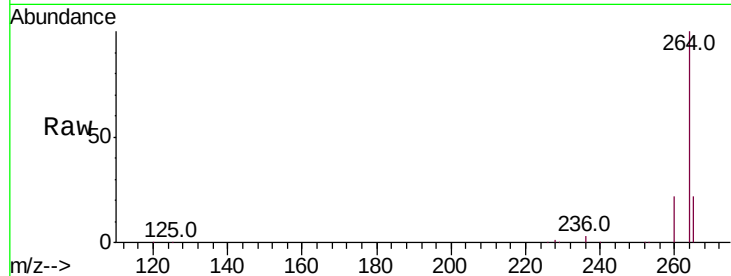

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

