

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097156.D
 Acq On : 2 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4149-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1G3

Quant Time: Aug 02 18:57:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1248	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6305	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4043	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	770304	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	16721	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	2953	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.02	166	1002	0.069	ng/ul#	23
23) Benzo(a)pyrene	23.07	252	3081	0.068	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097156.D
Acq On : 2 Aug 2018 18:13
Operator : SJ/JU
Sample : J4149-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1G3

Quant Time: Aug 02 18:57:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration




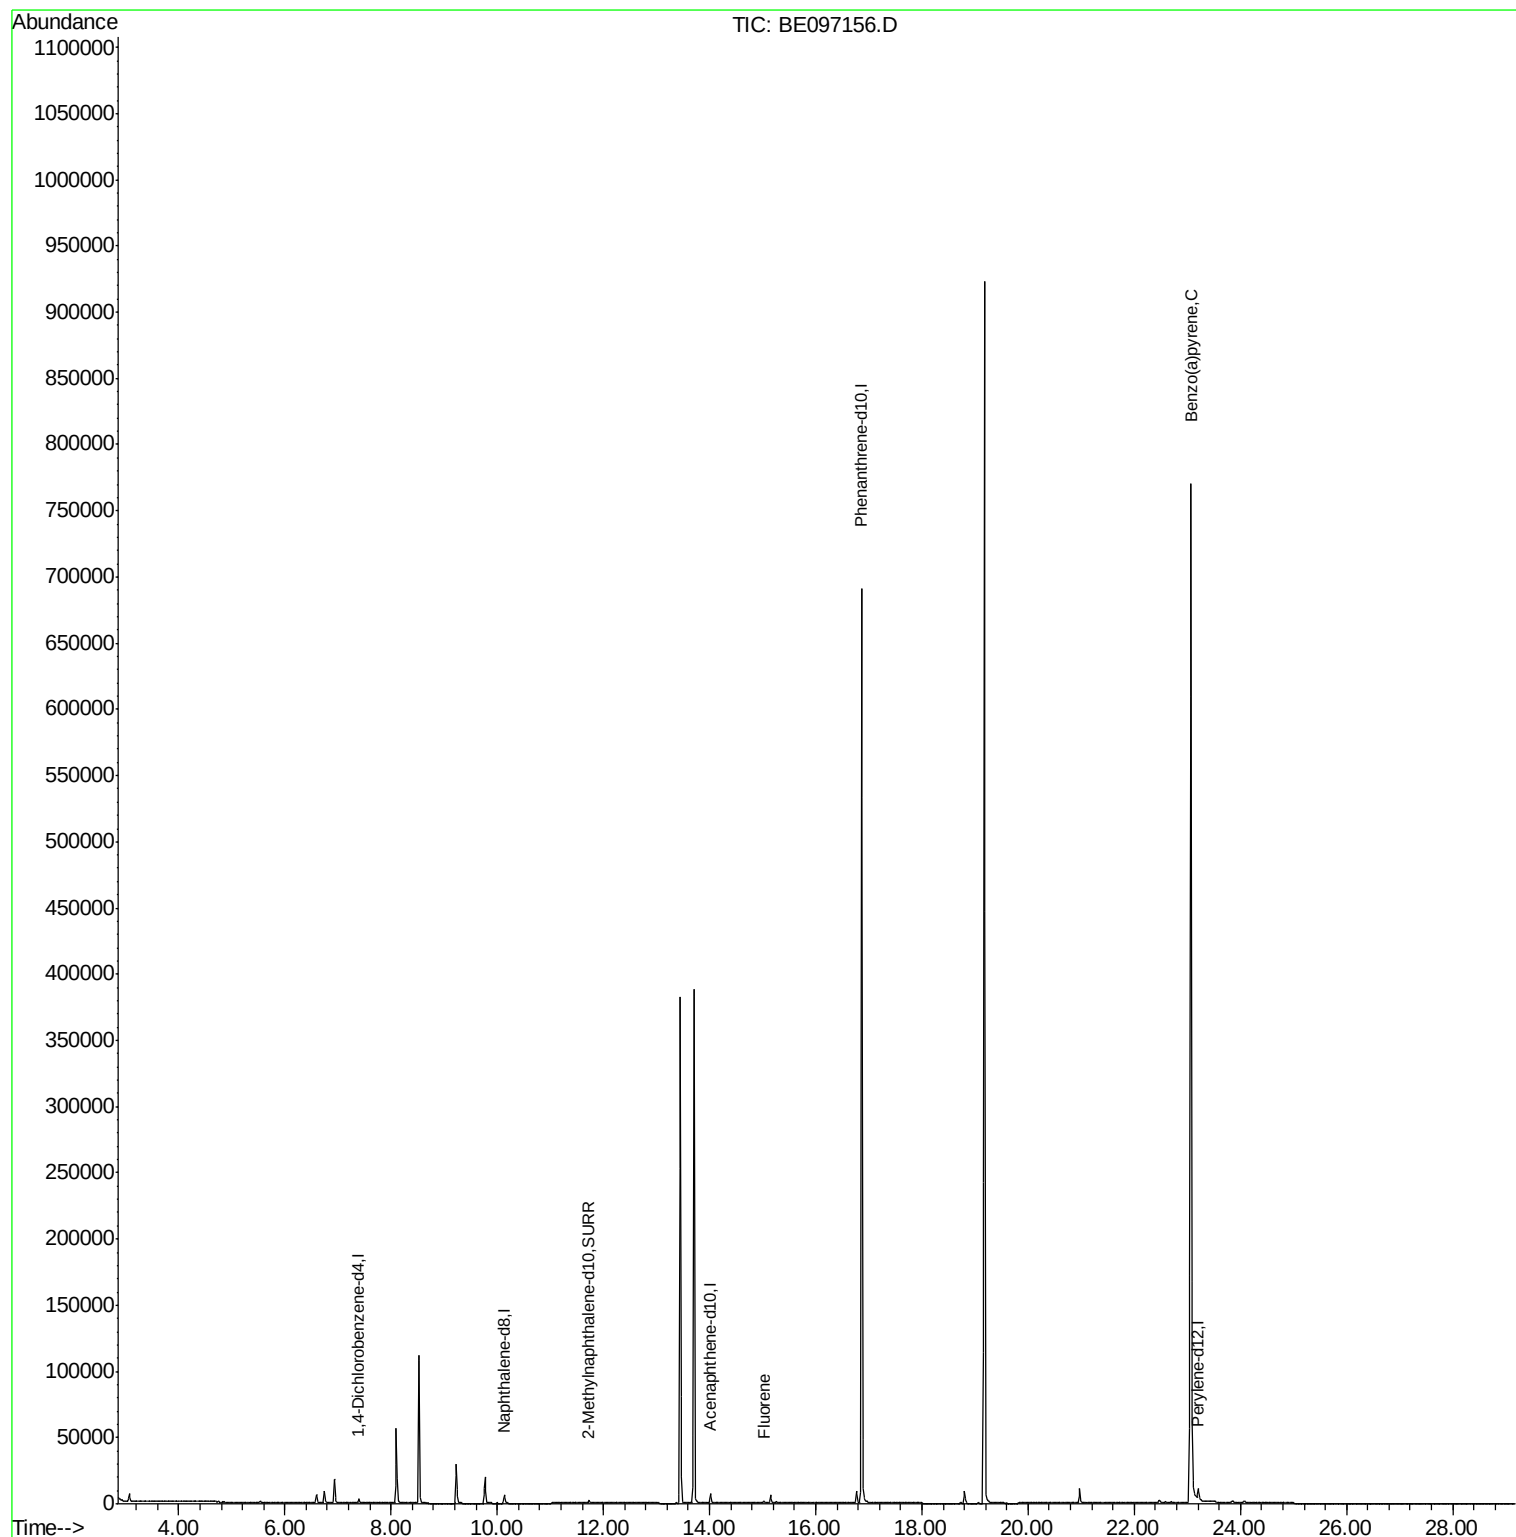


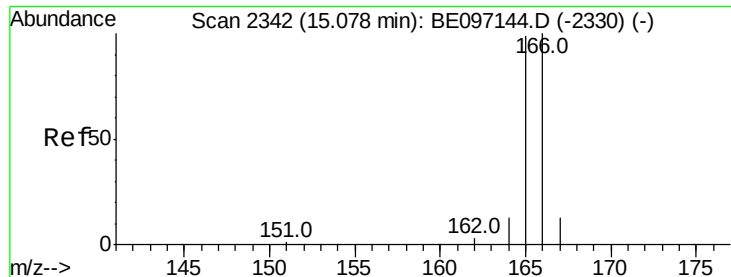

#9
Fluorene
 Concen: 0.069 ng/ul
 RT: 15.02 min Scan# 2333
 Delta R.T. -0.06 min
 Lab File: BE097156.D
 Acq: 2 Aug 2018 18:13

Instrument :
 BNA_E
 ClientSampled :
 JJ1G3

Tot Ion:166 Resp: 1002
 Ion Ratio Lower Upper
 166 100
 165 12.5 73.4 110.2#
 167 39.1 14.6 22.0#

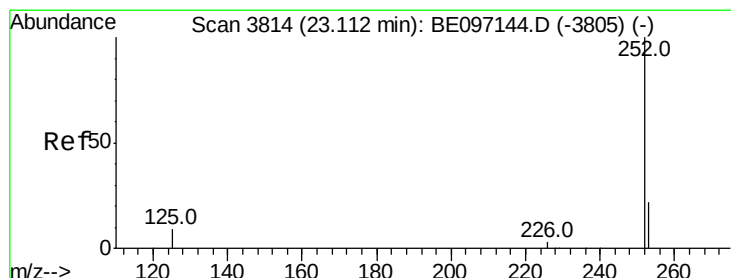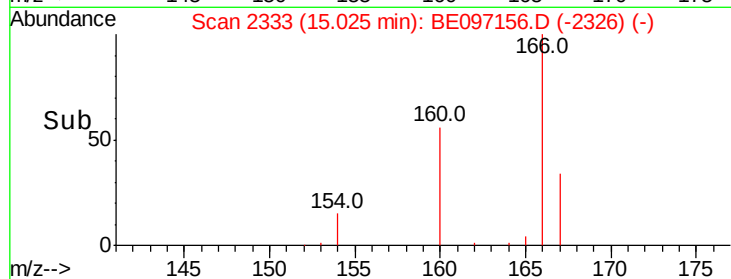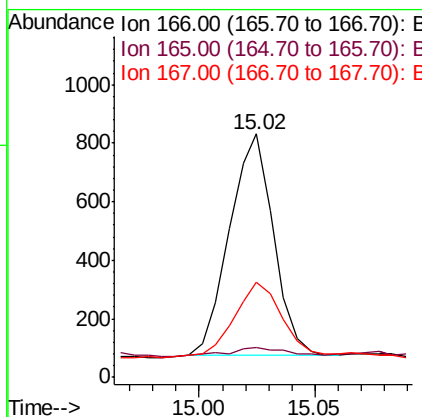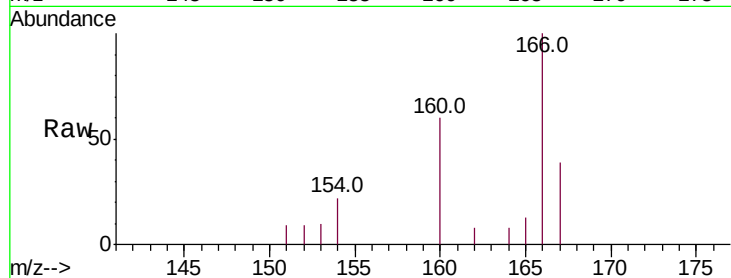

#23
Benzo(a)pyrene
 Concen: 0.068 ng/ul
 RT: 23.07 min Scan# 3808
 Delta R.T. -0.04 min
 Lab File: BE097156.D
 Acq: 2 Aug 2018 18:13

Tgt Ion:252 Resp: 3081
 Ion Ratio Lower Upper
 252 100
 253 30.7 28.5 42.7
 125 23.0 18.1 27.1

