

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097159.D
 Acq On : 2 Aug 2018 20:06
 Operator : SJ/JU
 Sample : J4149-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 02 23:29:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1288	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6898	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	5665	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	994400	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	18174	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	4284	0.39	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
9) Fluorene	15.02	166	1707	0.084	ng/ul#	25
23) Benzo(a)pyrene	23.07	252	3835	0.077	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097159.D
Acq On : 2 Aug 2018 20:06
Operator : SJ/JU
Sample : J4149-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 02 23:29:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration




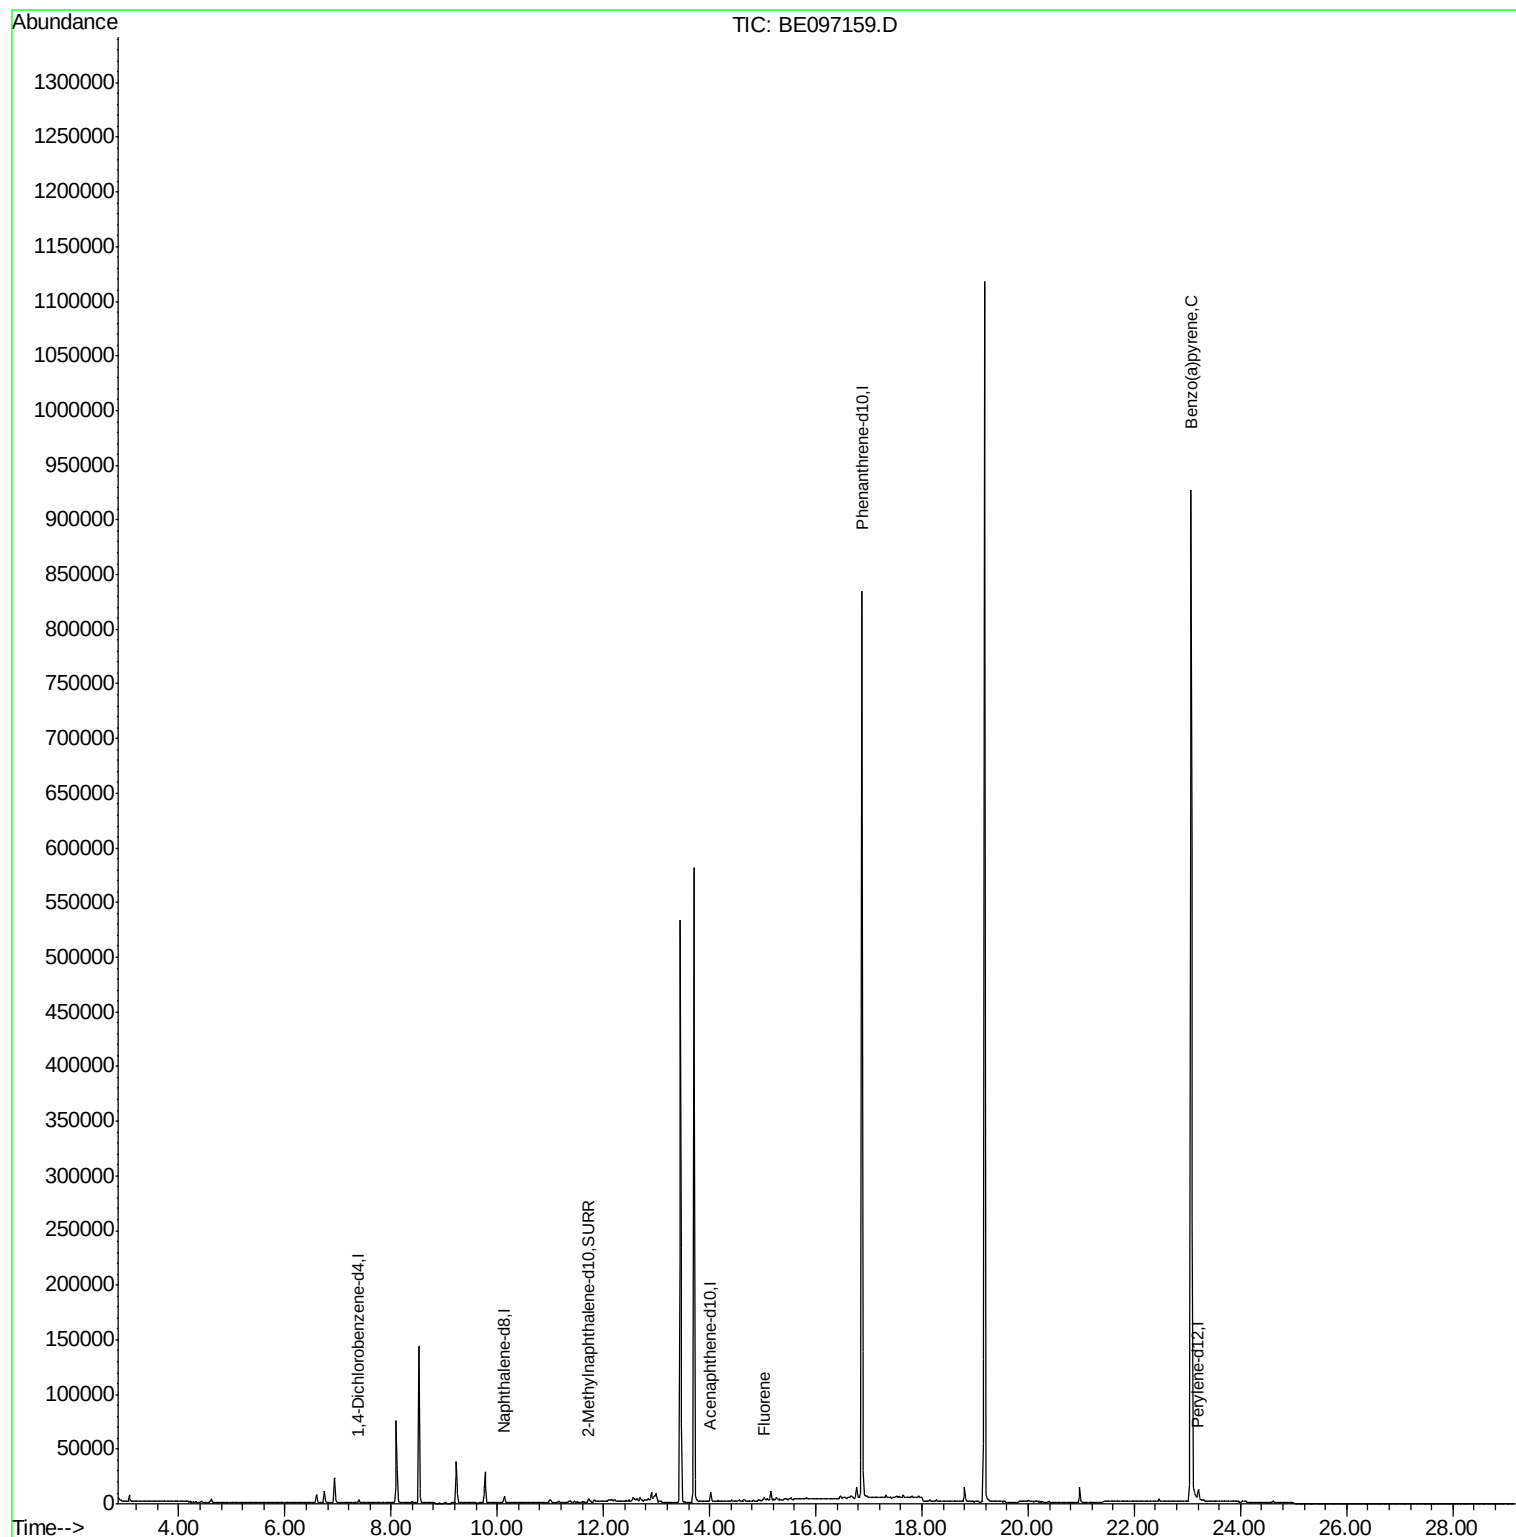


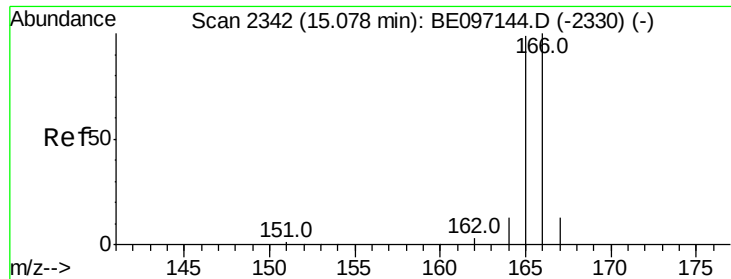

#9
Fluorene
 Concen: 0.084 ng/ul
 RT: 15.02 min Scan# 2332
 Delta R.T. -0.06 min
 Lab File: BE097159.D
 Acq: 2 Aug 2018 20:06

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 1707
 Ion Ratio Lower Upper
 166 100
 165 28.4 73.4 110.2#
 167 70.6 14.6 22.0#

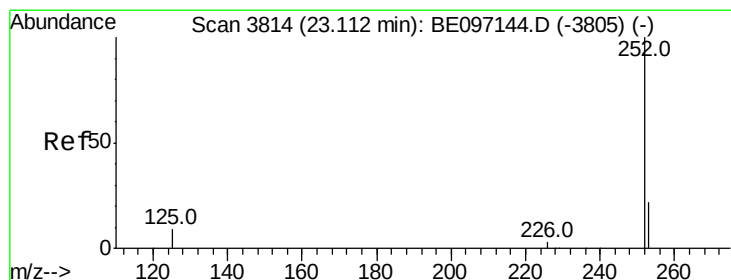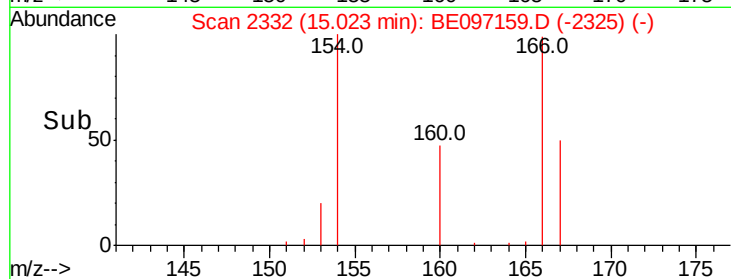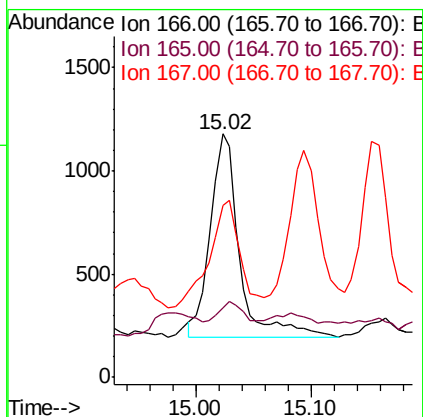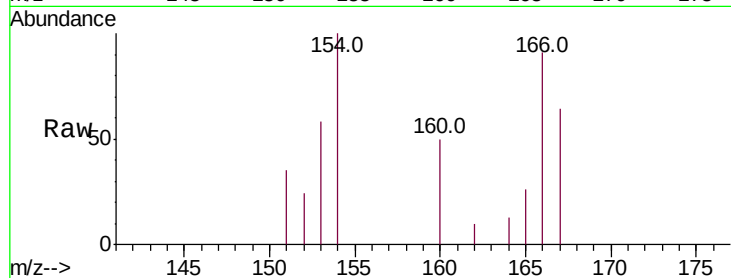

#23
Benzo(a)pyrene
 Concen: 0.077 ng/ul
 RT: 23.07 min Scan# 3807
 Delta R.T. -0.04 min
 Lab File: BE097159.D
 Acq: 2 Aug 2018 20:06

Tgt Ion:252 Resp: 3835
 Ion Ratio Lower Upper
 252 100
 253 32.3 28.5 42.7
 125 28.3 18.1 27.1#

