

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097162.D
 Acq On : 2 Aug 2018 22:00
 Operator : SJ/JU
 Sample : J4171-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 02 23:29:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1287	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6625	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4233	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	842280	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.20	264	18208	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3925	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.18	128	796	0.050	ng/ul#	83
23) Benzo(a)pyrene	23.07	252	3689	0.074	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097162.D
Acq On : 2 Aug 2018 22:00
Operator : SJ/JU
Sample : J4171-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 02 23:29:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

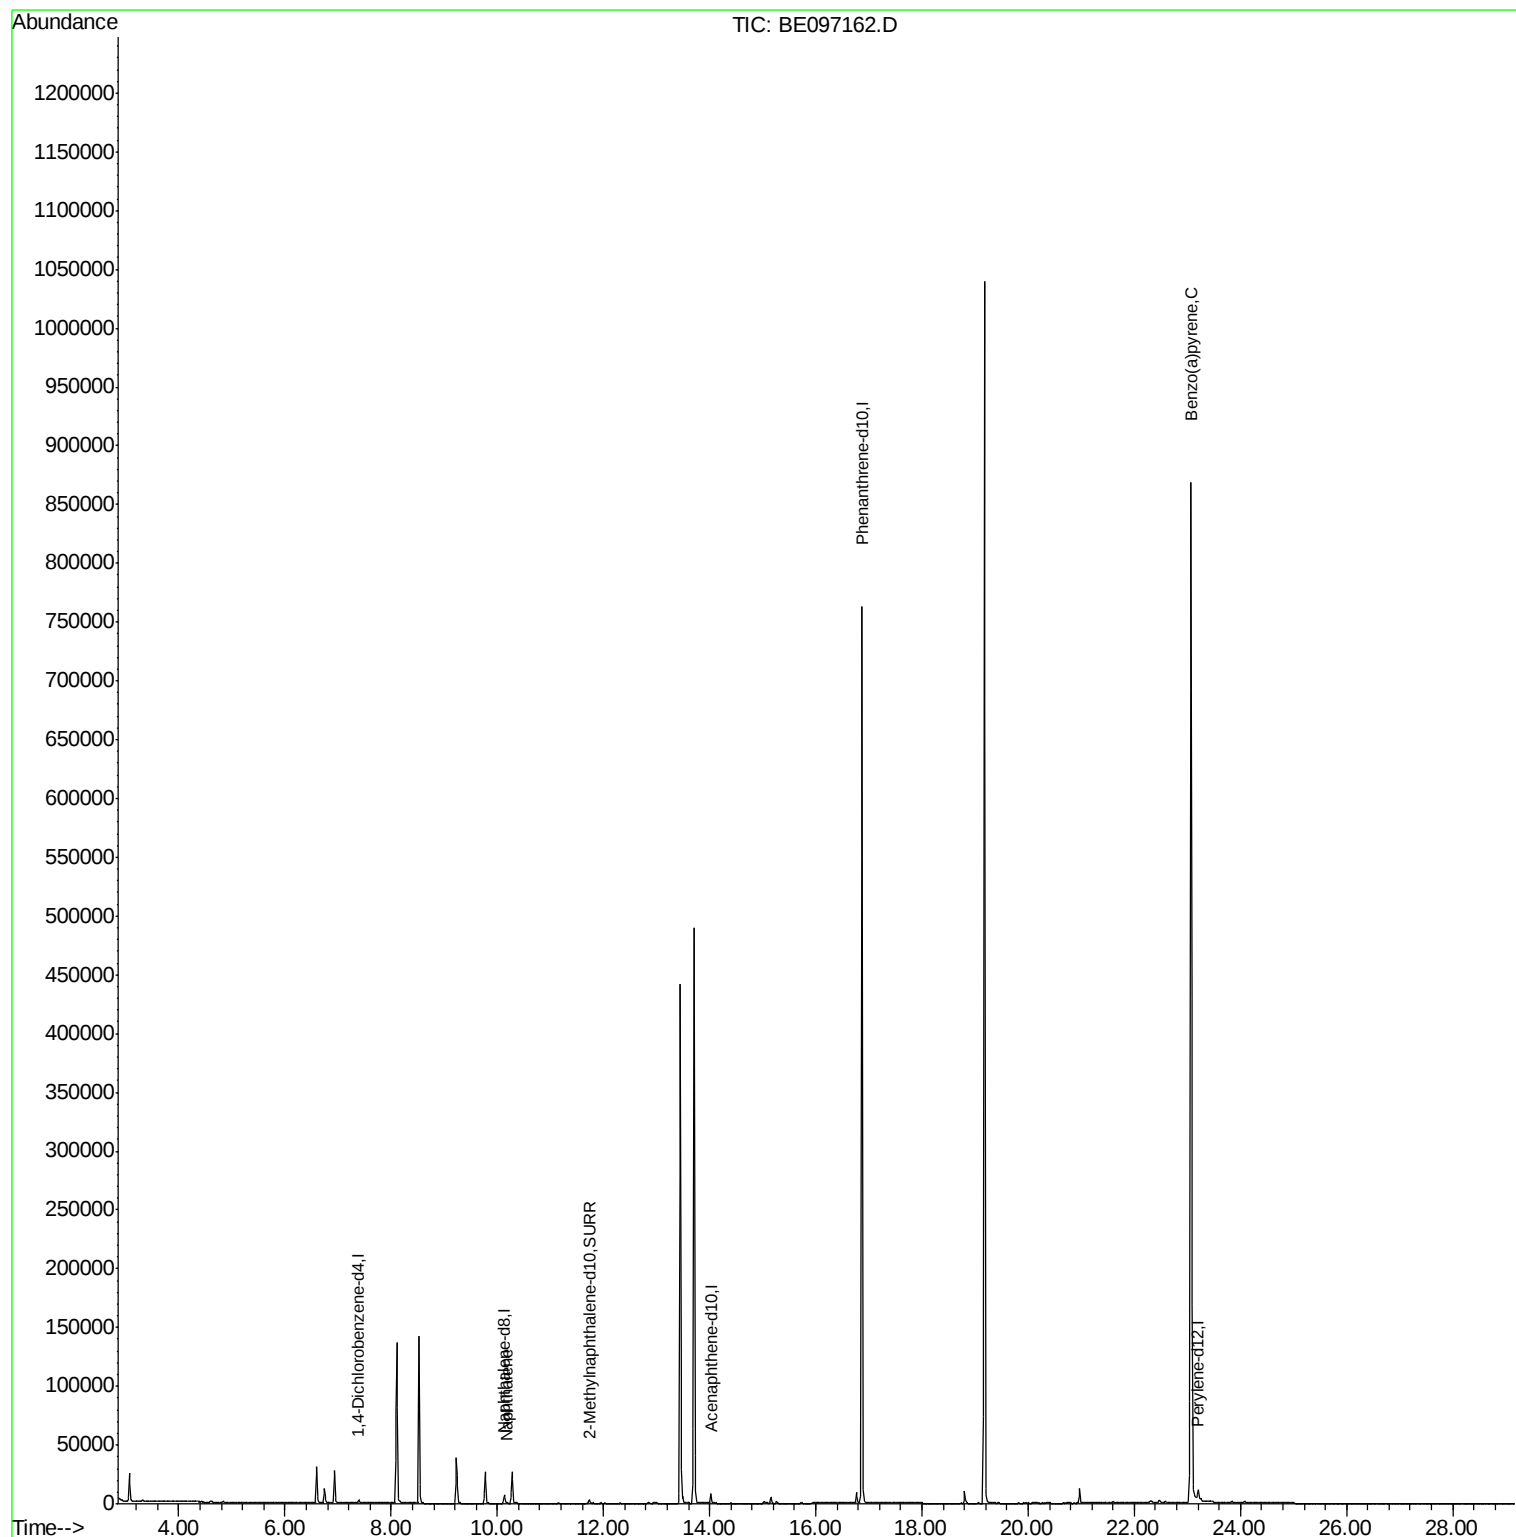

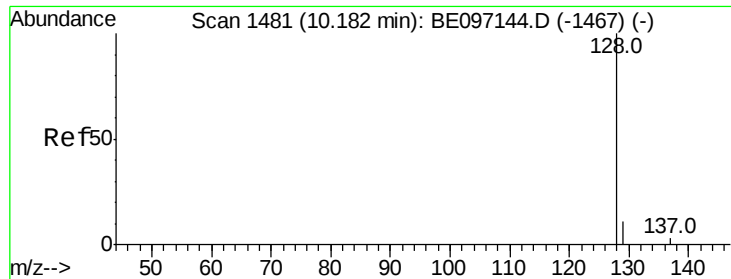

#3

Naphthalene

Concen: 0.050 ng/ul

RT: 10.18 min Scan# 1482

Delta R.T. -0.00 min

Lab File: BE097162.D

Acq: 2 Aug 2018 22:00

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 796

Ion Ratio Lower Upper

128 100

129 21.1 11.3 16.9#




127 0.0 4.0 6.0#

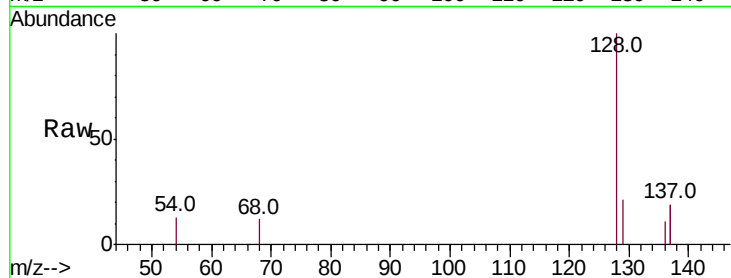

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

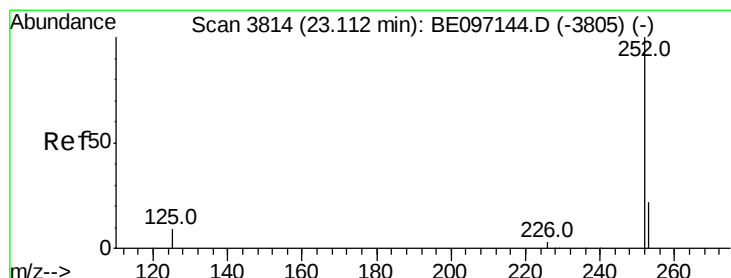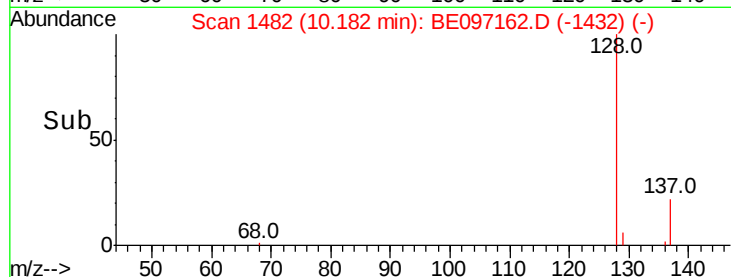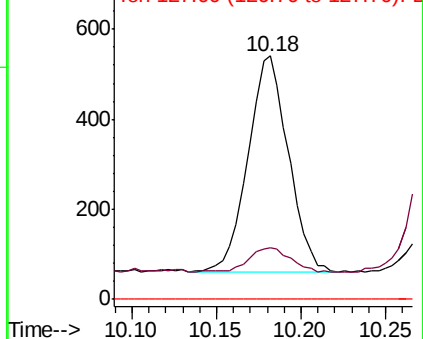

#23

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.07 min Scan# 3809

Delta R.T. -0.04 min

Lab File: BE097162.D

Acq: 2 Aug 2018 22:00


Tgt Ion:252 Resp: 3689

Ion Ratio Lower Upper

252 100

253 31.6 28.5 42.7

125 21.5 18.1 27.1

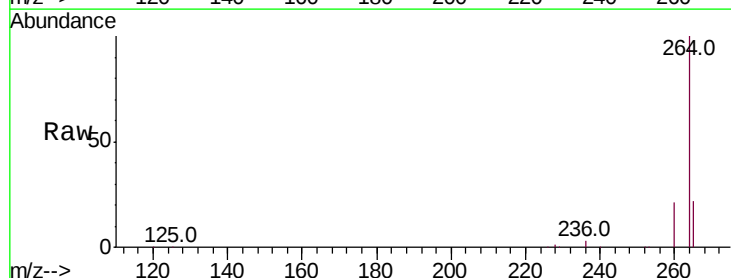

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

