

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097164.D
 Acq On : 2 Aug 2018 23:14
 Operator : SJ/JU
 Sample : J4171-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 03 03:07:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1369	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6984	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4353	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	604625	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.20	264	16745	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	2838	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.07	252	2870	0.063	ng/ul#	Ovalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097164.D
Acq On : 2 Aug 2018 23:14
Operator : SJ/JU
Sample : J4171-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 03 03:07:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 23:40:30 2018
Response via : Initial Calibration

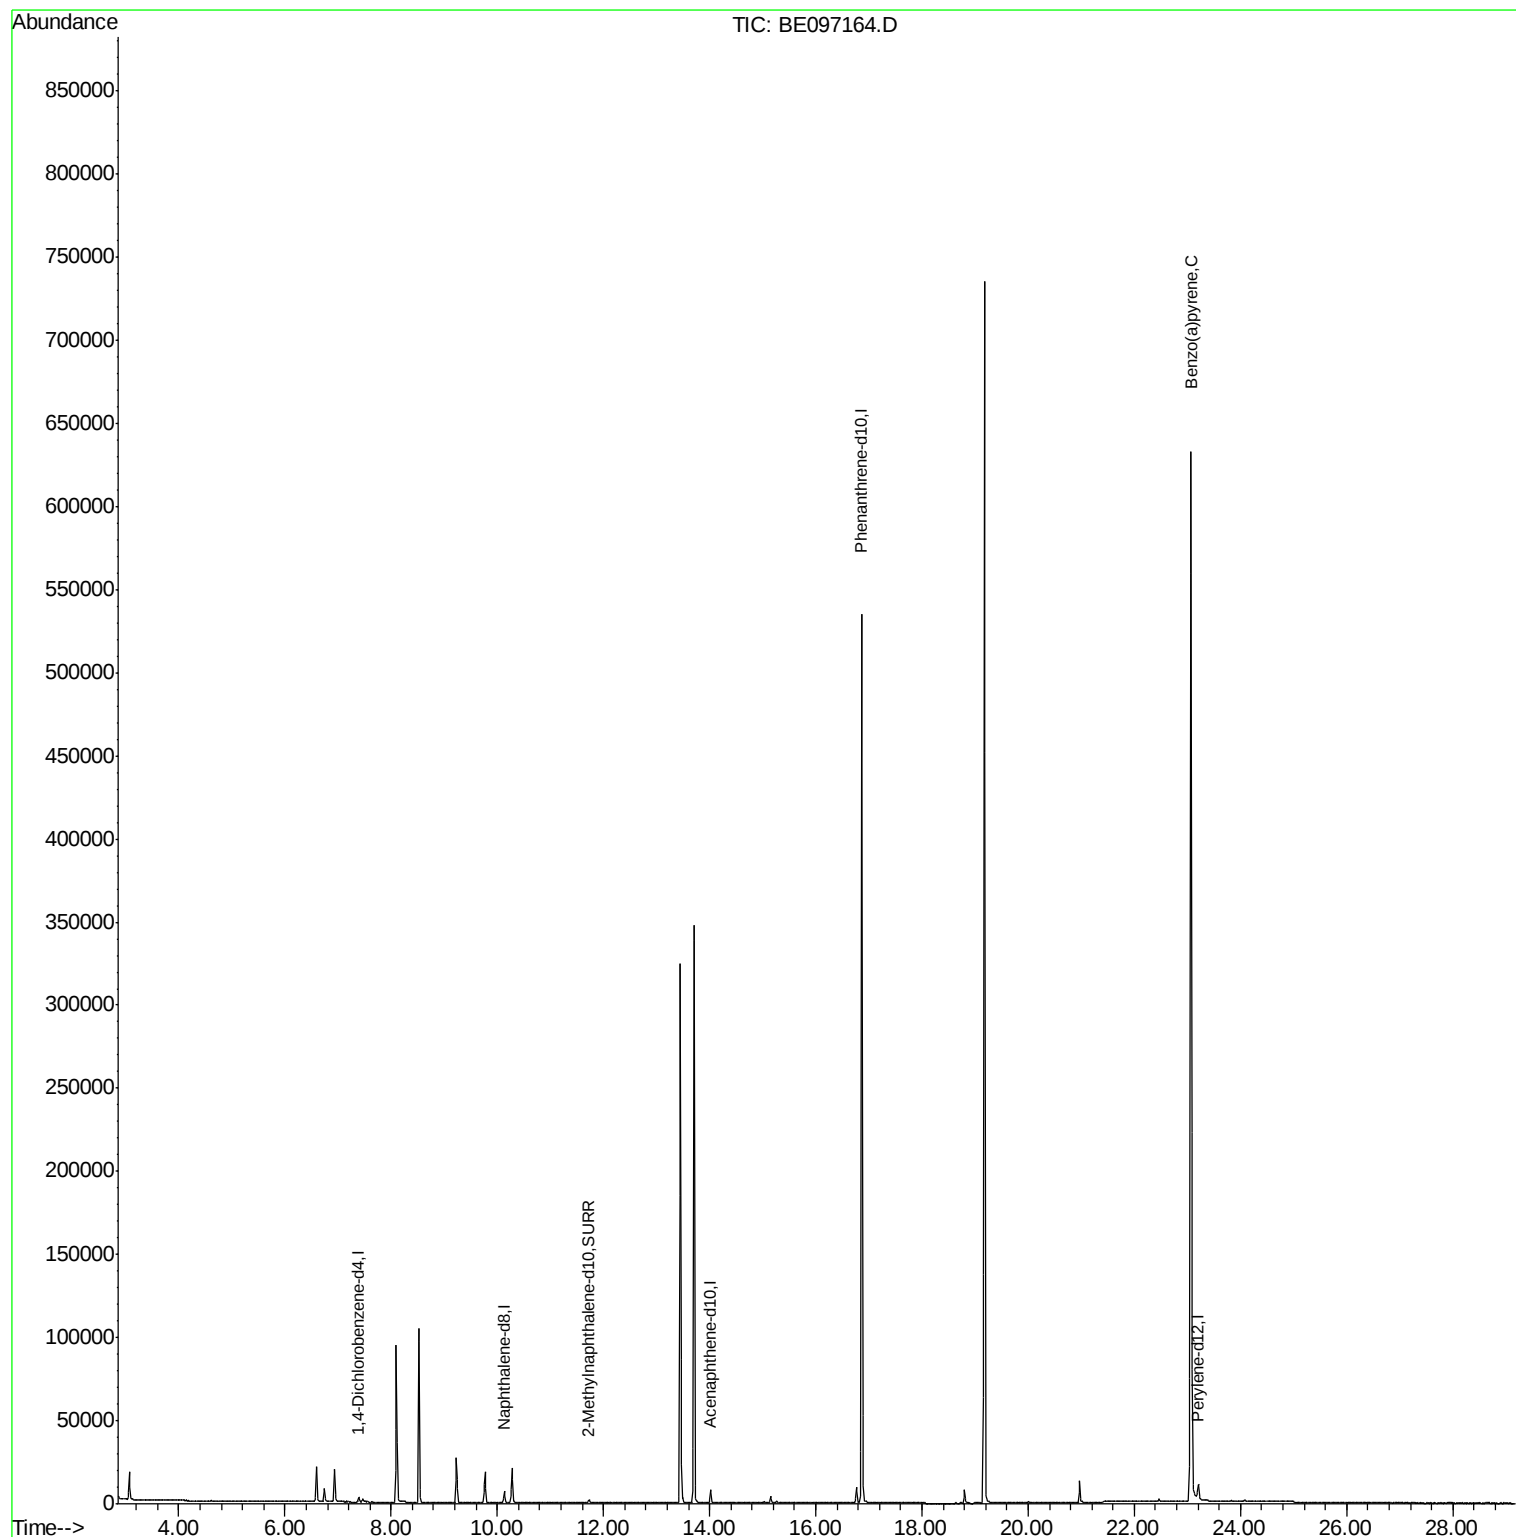

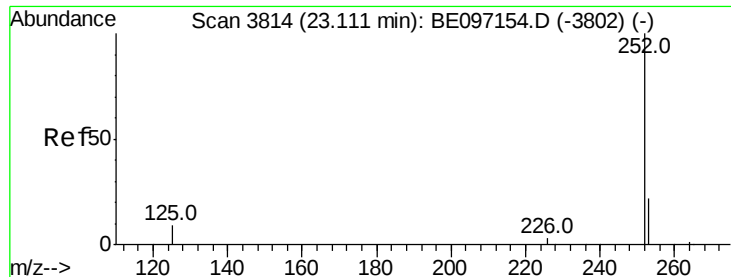

#23

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 23.07 min Scan# 3807

Delta R.T. -0.04 min


Lab File: BE097164.D

Acq: 2 Aug 2018 23:14

Instrument :

BNA_E

ClientSampleId :

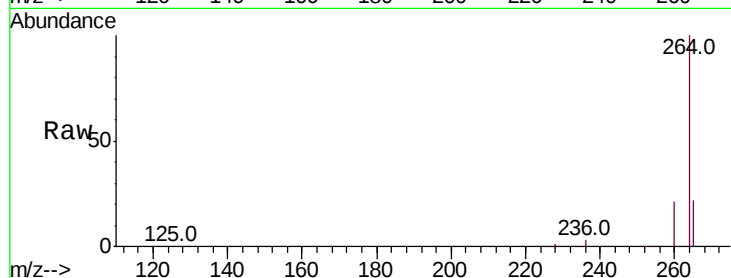


Tot Ion: 252 Resp: 2870

Ion Ratio Lower Upper

252 100

253 35.3 28.5 42.7

125 29.4 18.1 27.1#

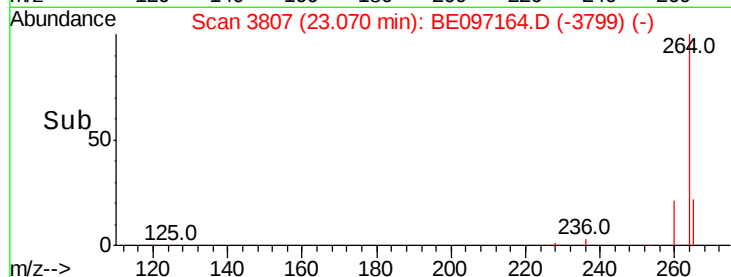

Abundance Ion 252.00 (251.70 to 252.70): E

2000 Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

