

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097166.D
 Acq On : 3 Aug 2018 00:29
 Operator : SJ/JU
 Sample : J4171-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 03 03:07:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1329	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6727	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4344	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	790760	0.40	ng/ul	0.10
16) Chrysene-d12	21.17	240	17	0.40	ng/ul	0.20
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.21
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3665	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
17) Pyrene	19.20	202	3650	80.127	ng/ul#	86
18) Benzo(a)anthracene	21.12	228	205	4.220	ng/ul#	18
19) Chrysene	21.12	228	205	4.095	ng/ul#	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097166.D
Acq On : 3 Aug 2018 00:29
Operator : SJ/JU
Sample : J4171-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 03 03:07:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 23:40:30 2018
Response via : Initial Calibration

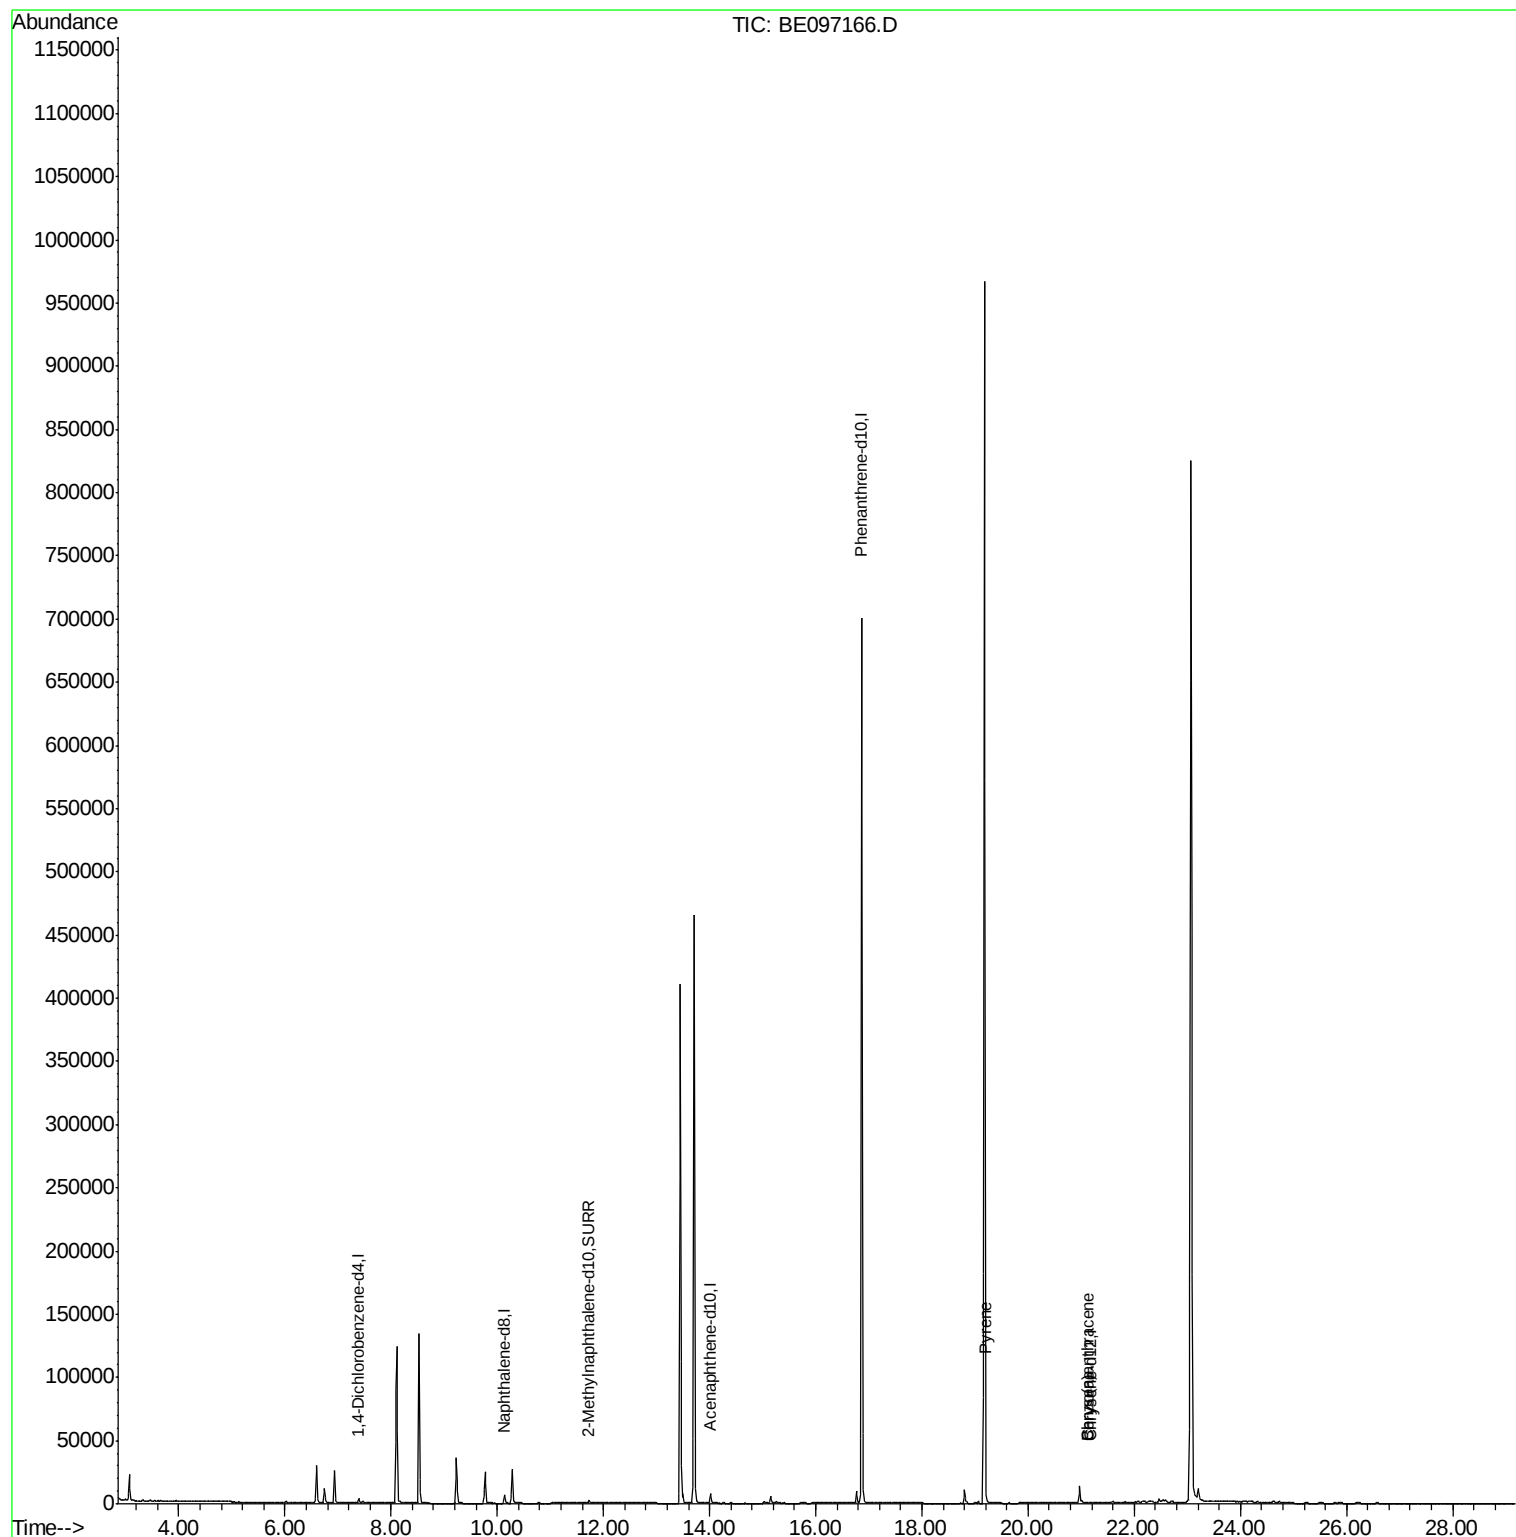


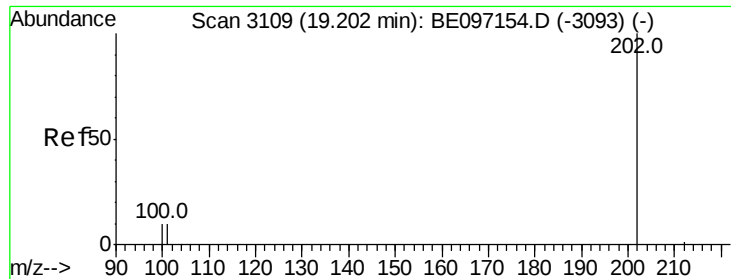




#17
Pvrene
Concen: 80.127 ng/ul
RT: 19.20 min Scan# 3109
Delta R.T. 0.00 min
Lab File: BE097166.D
Acq: 3 Aug 2018 00:29

Instrument :
BNA_E
ClientSampled :

Tot Ion:202 Resp: 3650
Ion Ratio Lower Upper
202 100
101 14.6 18.2 27.4#
100 14.7 15.6 23.4#

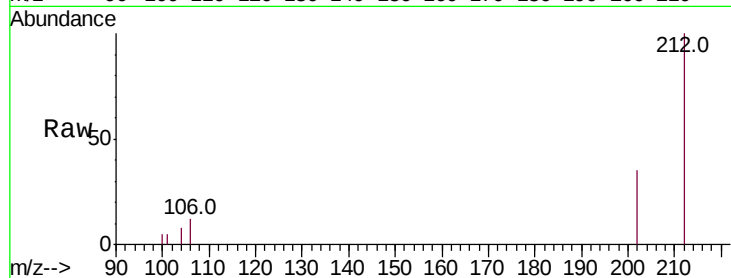


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

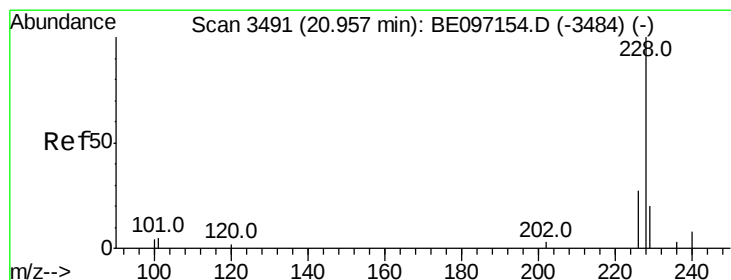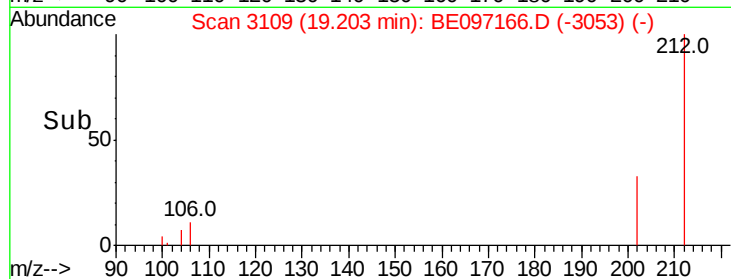
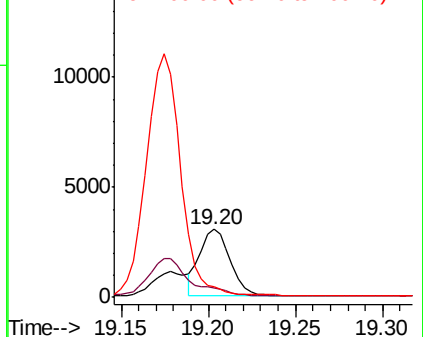





#18
Benzo(a)anthracene
Concen: 4.220 ng/ul
RT: 21.12 min Scan# 3522
Delta R.T. 0.17 min
Lab File: BE097166.D
Acq: 3 Aug 2018 00:29

Tgt Ion:228 Resp: 205
Ion Ratio Lower Upper
228 100
229 55.6 22.8 34.2#
226 79.3 17.0 25.6#

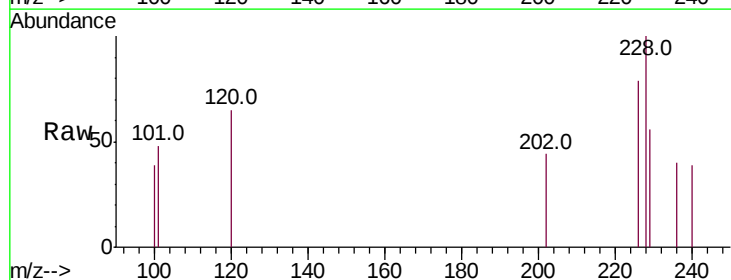

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

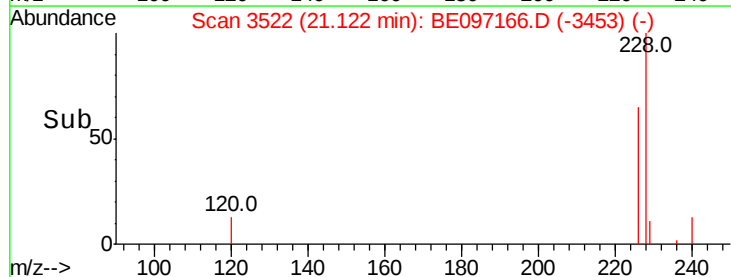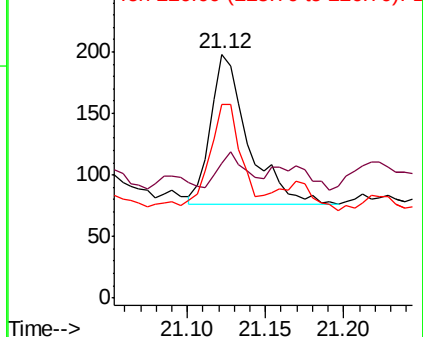

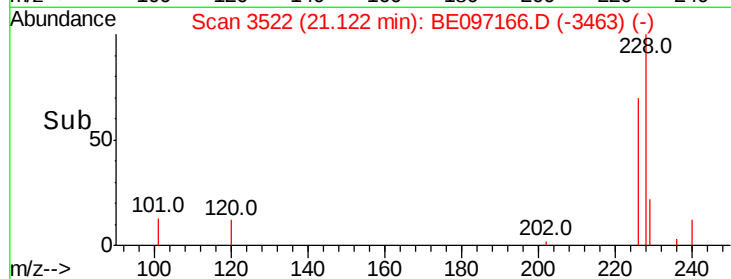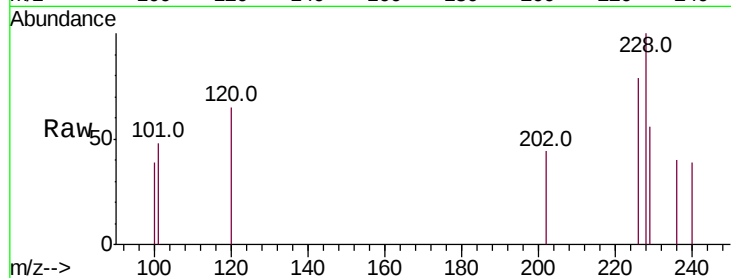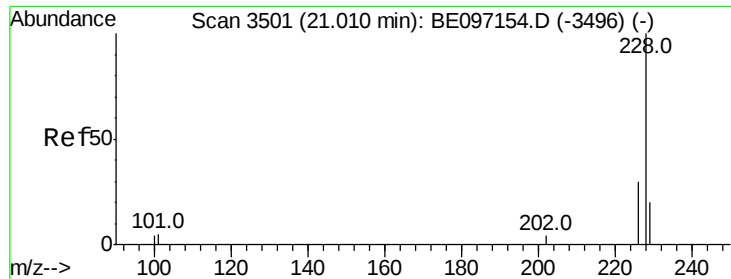

#19

Chrysene

Concen: 4.095 ng/ul

RT: 21.12 min Scan# 3522

Delta R.T. 0.11 min

Lab File: BE097166.D

Acq: 3 Aug 2018 00:29

Instrument :

BNA_E

ClientSampleId :

Tot Ion:228 Resp: 205

Ion Ratio Lower Upper

228 100

226 79.3 23.4 35.0#

229 55.6 17.7 26.5#

