

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:23:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

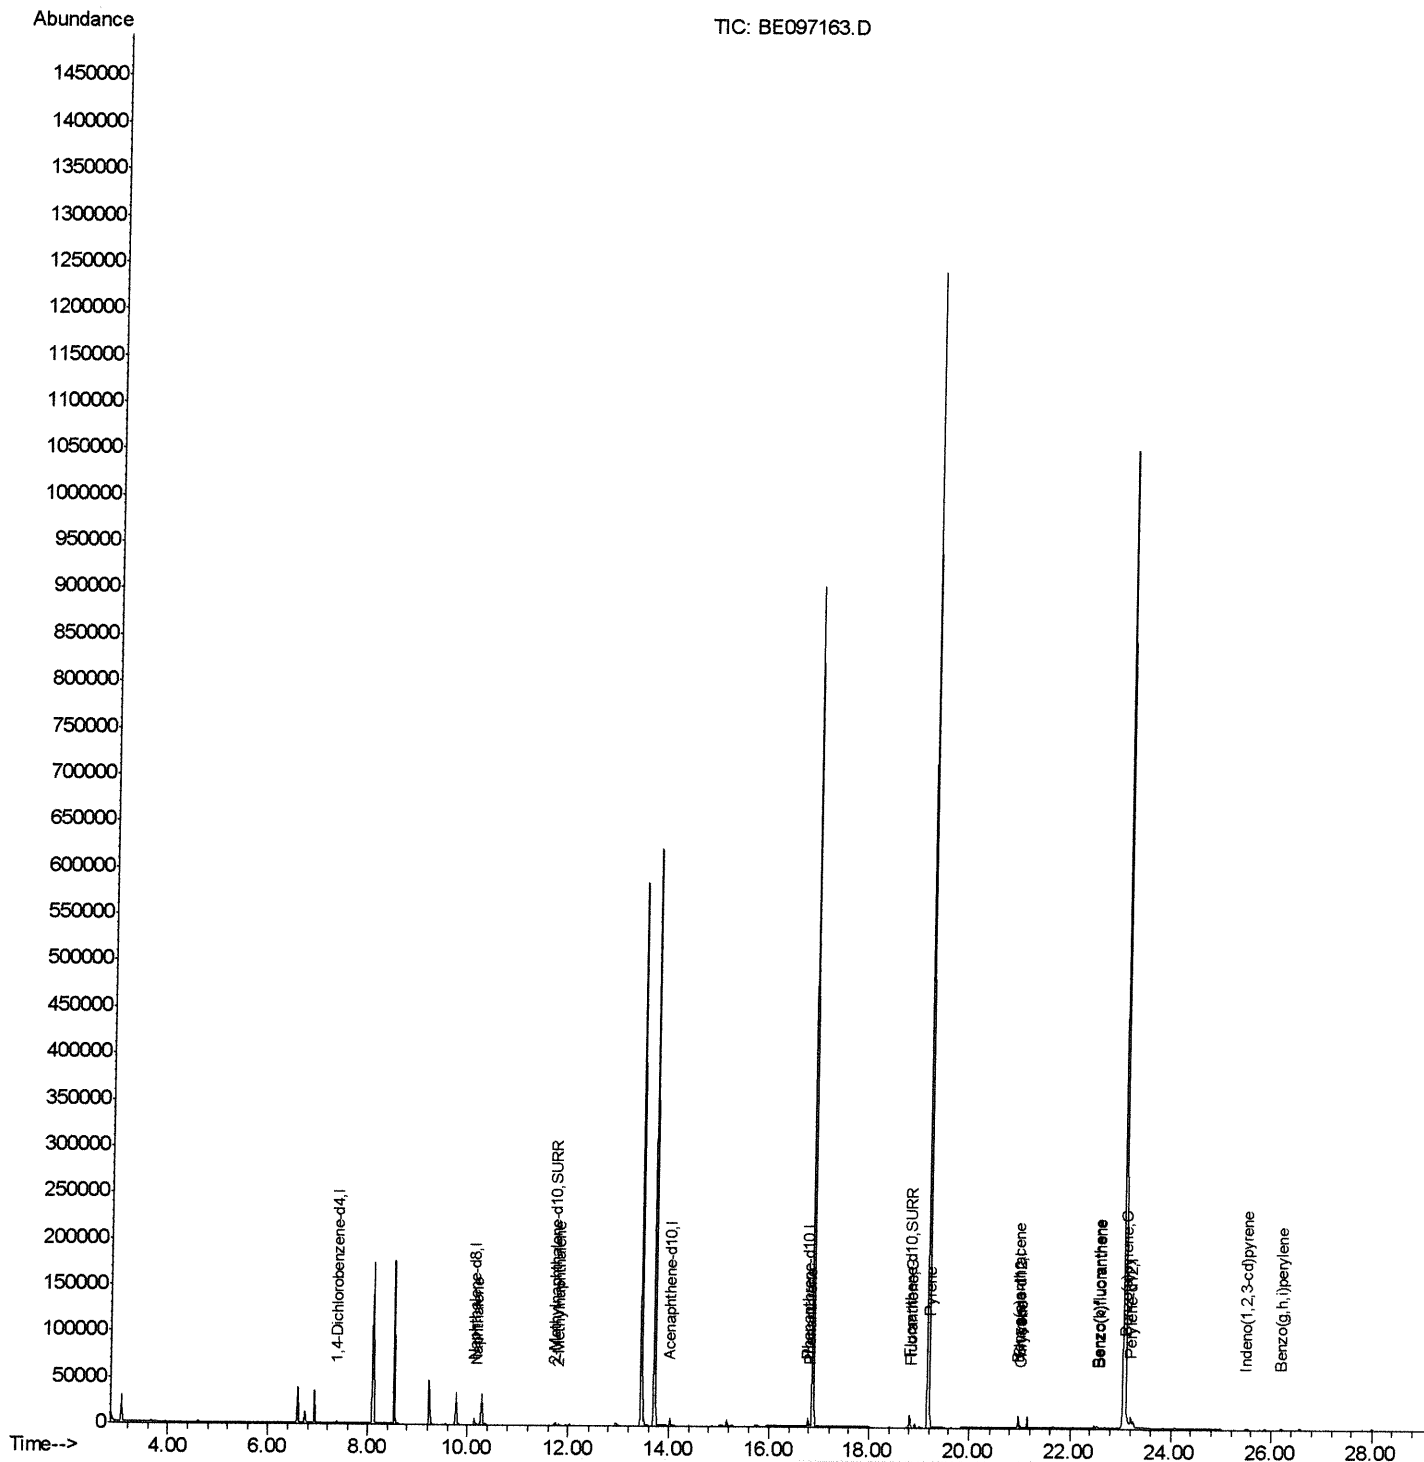

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 02 23:30:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

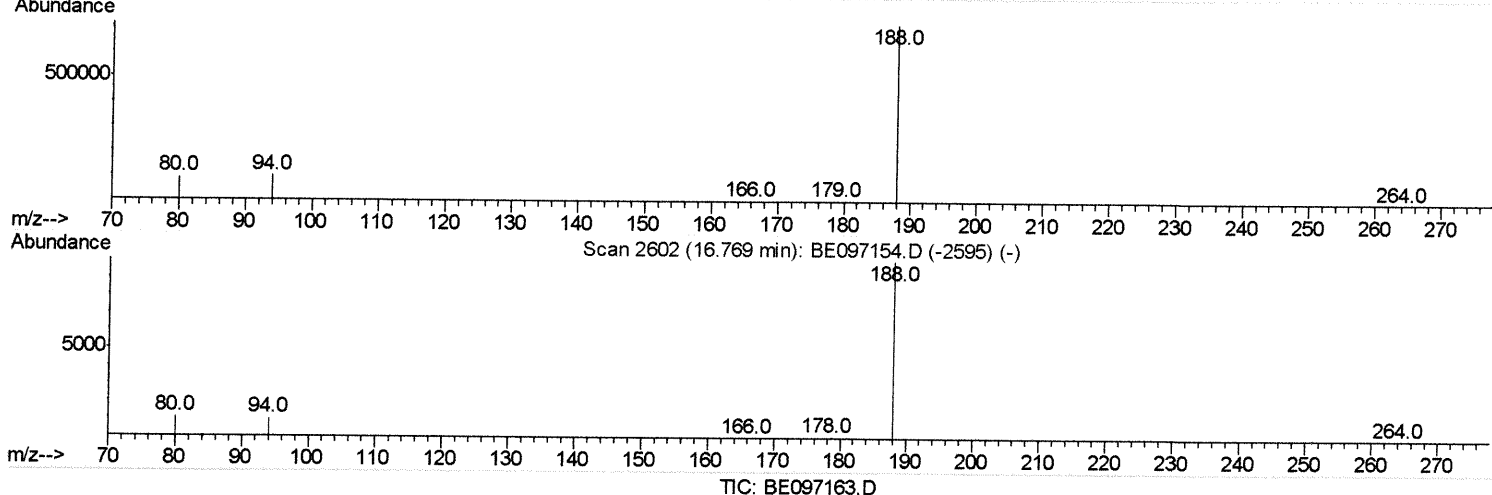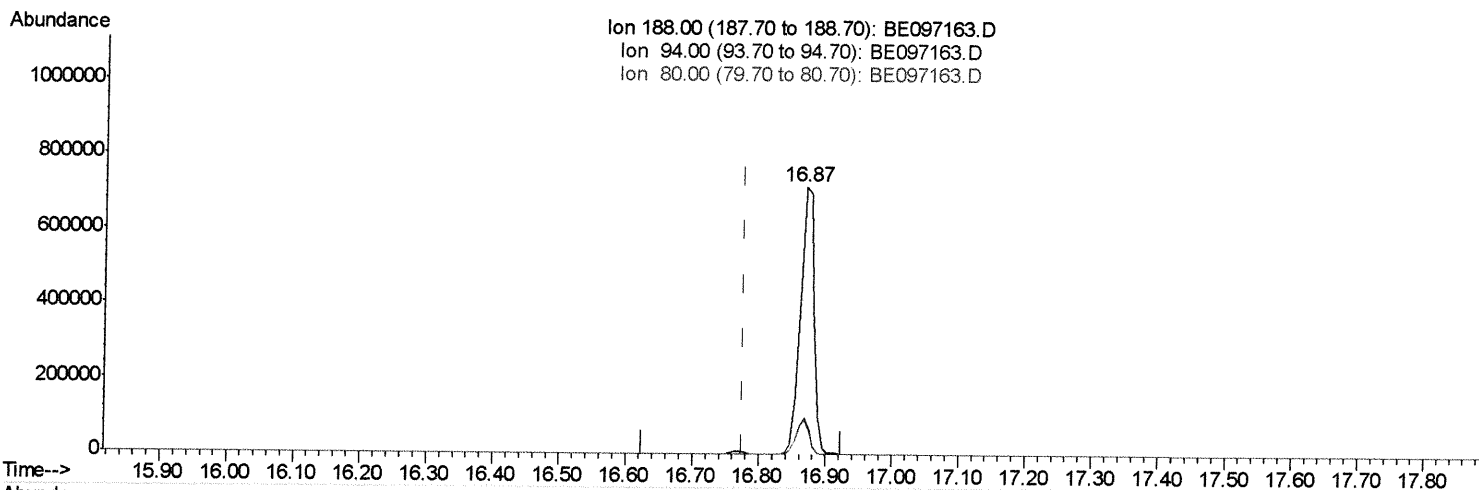

(10) Phenanthrene-d10 (I)

16.867min (+0.092) 0.40ng/ul

response 1061108

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.63#
80.00	11.80	12.60
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 02 23:30:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

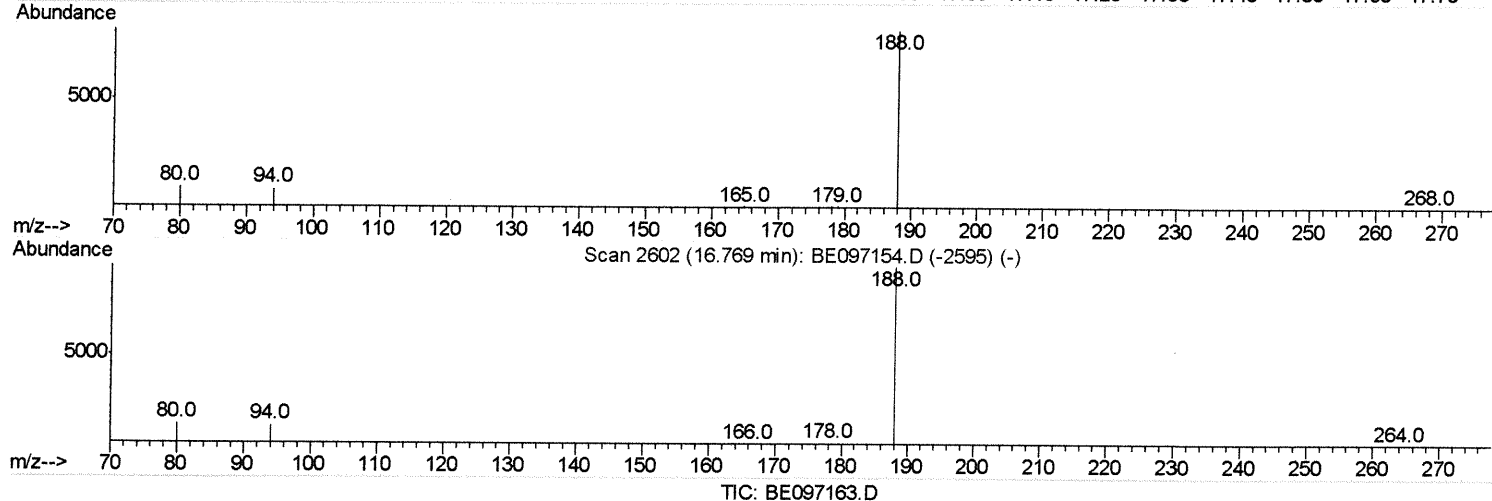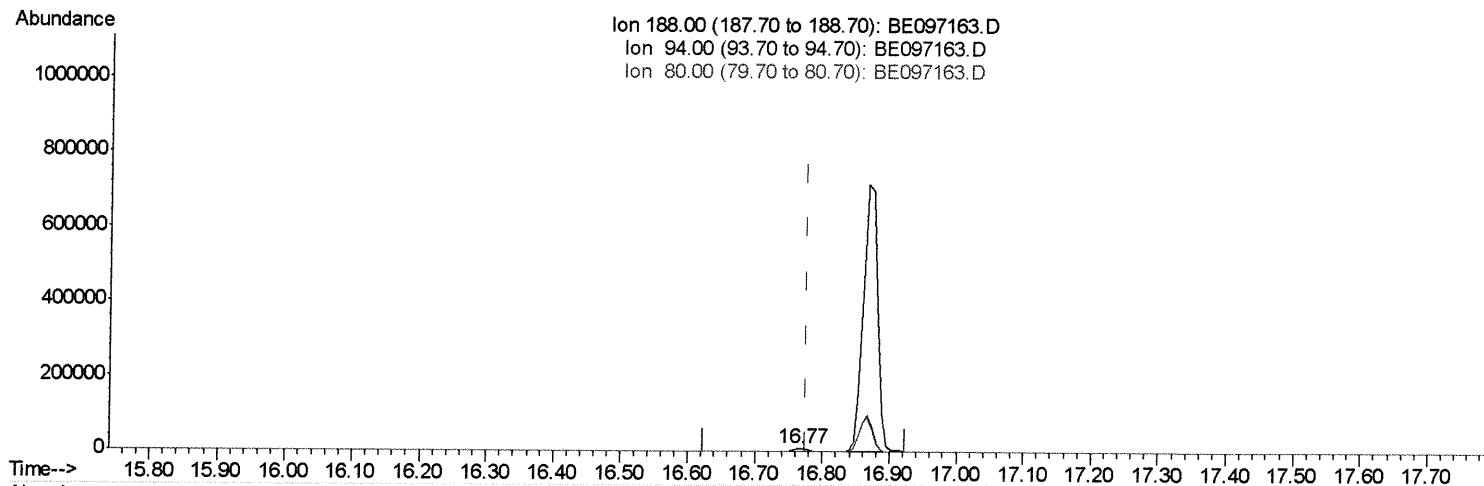

(10) Phenanthrene-d10 (I)

16.768min (-0.007) 0.40ng/ul m> SJ 8/9/18

response 11037

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.12
80.00	11.80	11.20
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

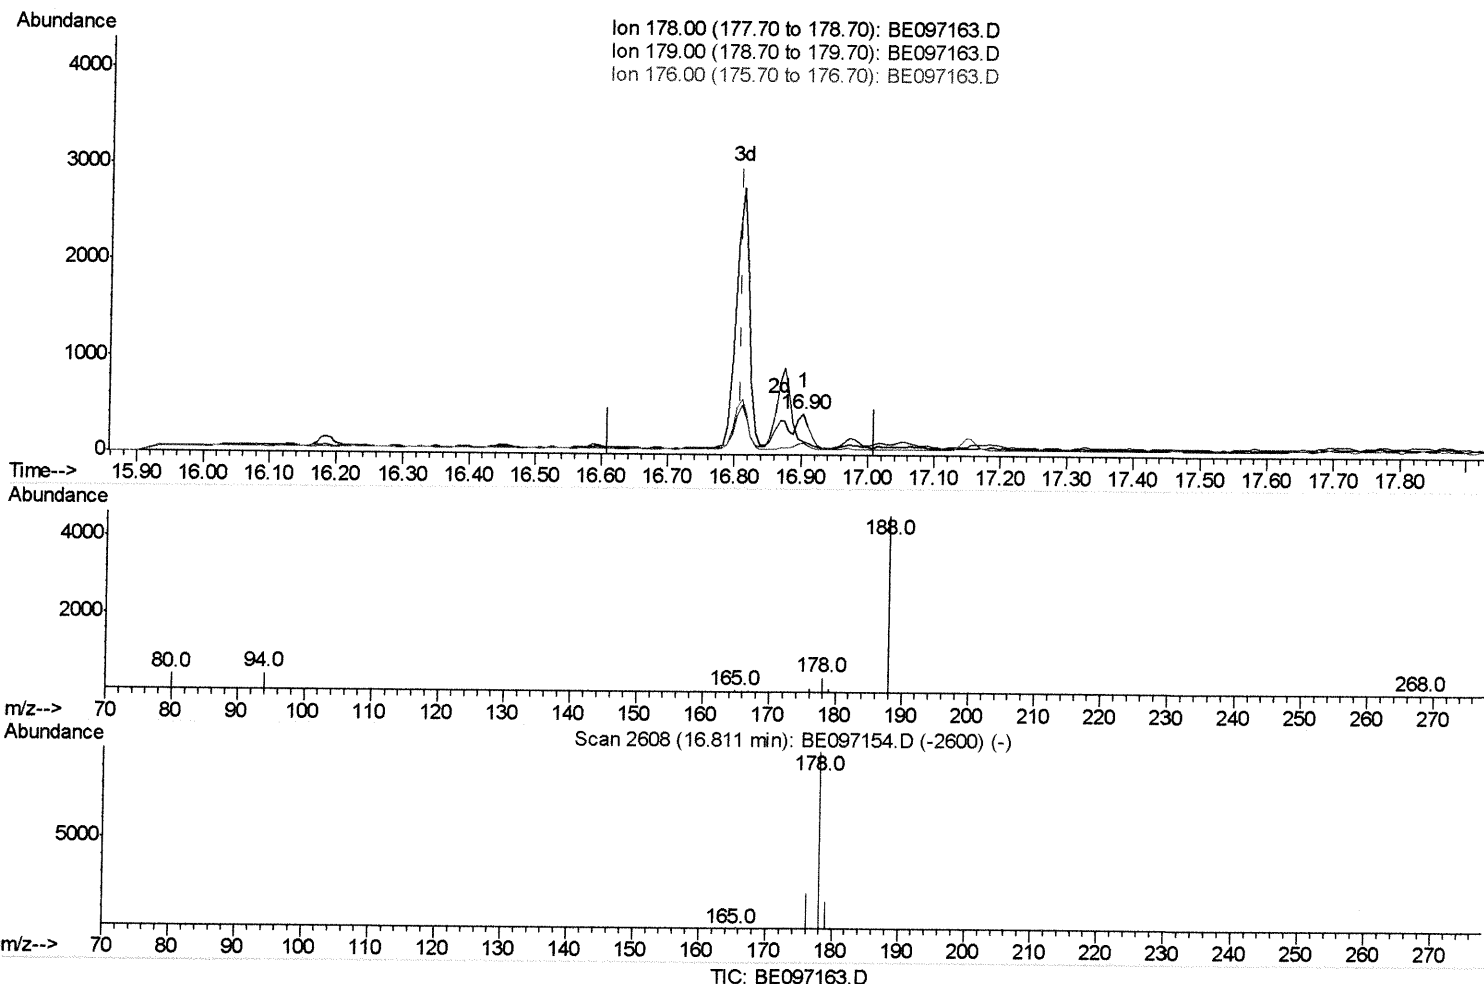

(12) Phenanthrene

16.902min (+0.092) 0.01ng/ul

response 421

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	33.25#
176.00	17.00	30.42#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

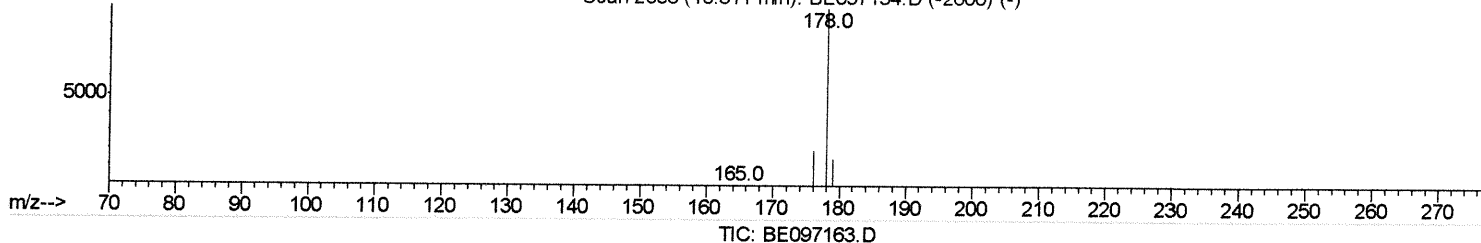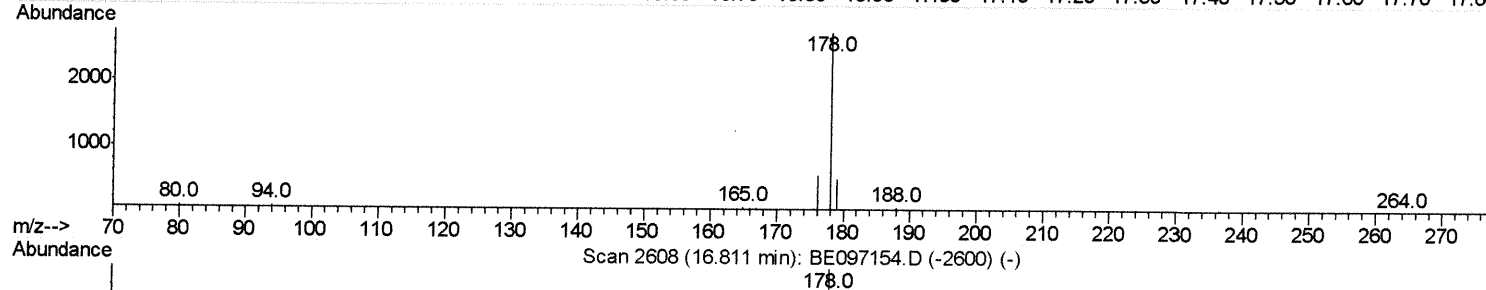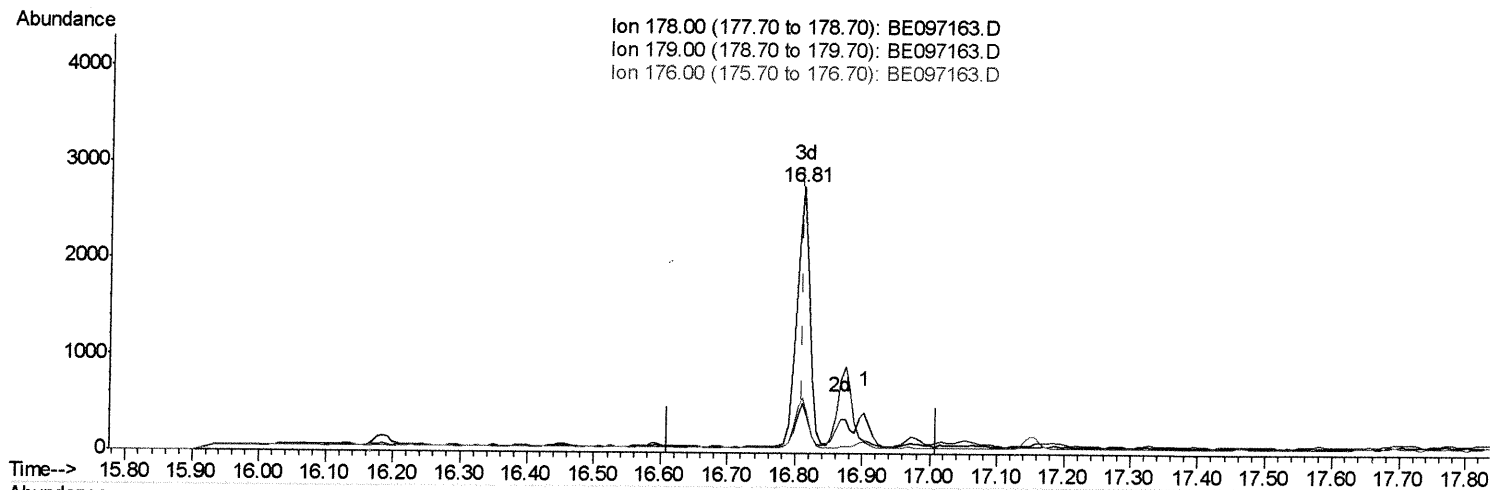

(12) Phenanthrene

16.810min (+0.000) 0.13ng/ul m

> SJ 8/9/18

response 3654

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	18.80
176.00	17.00	20.74#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

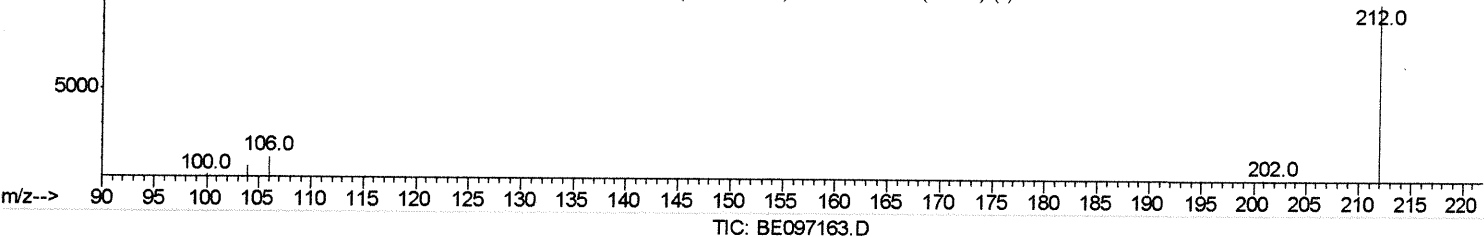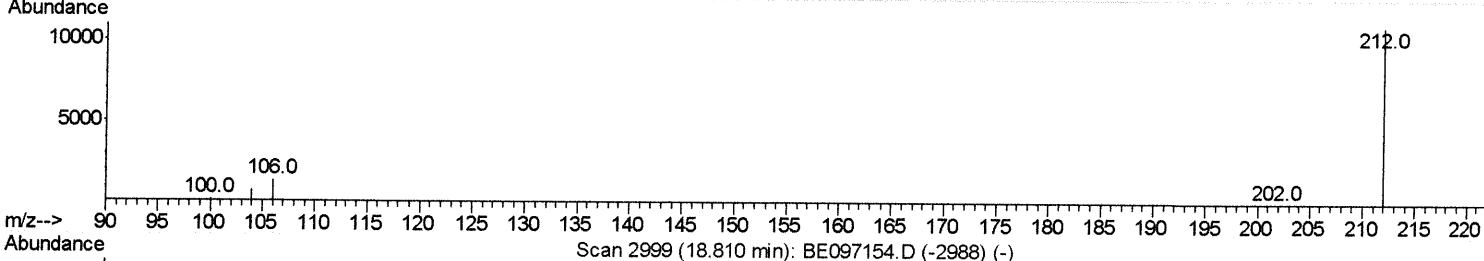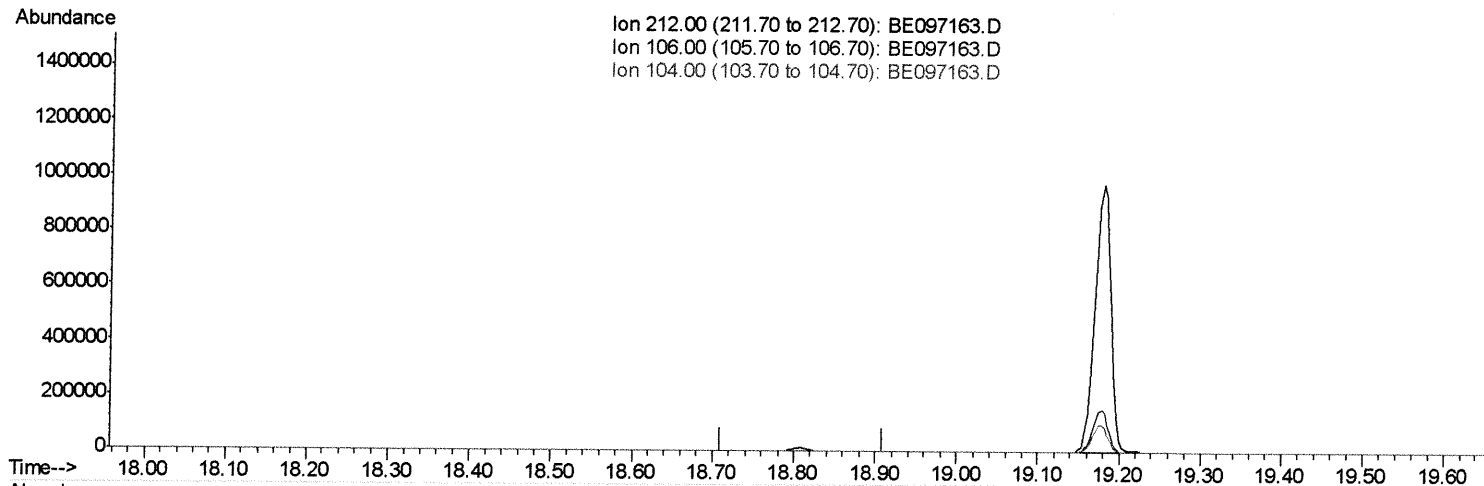

(14) Fluoranthene-d10 (SURR)

18.810min (-18.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Printed: 2018-08-03 00:18:04

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

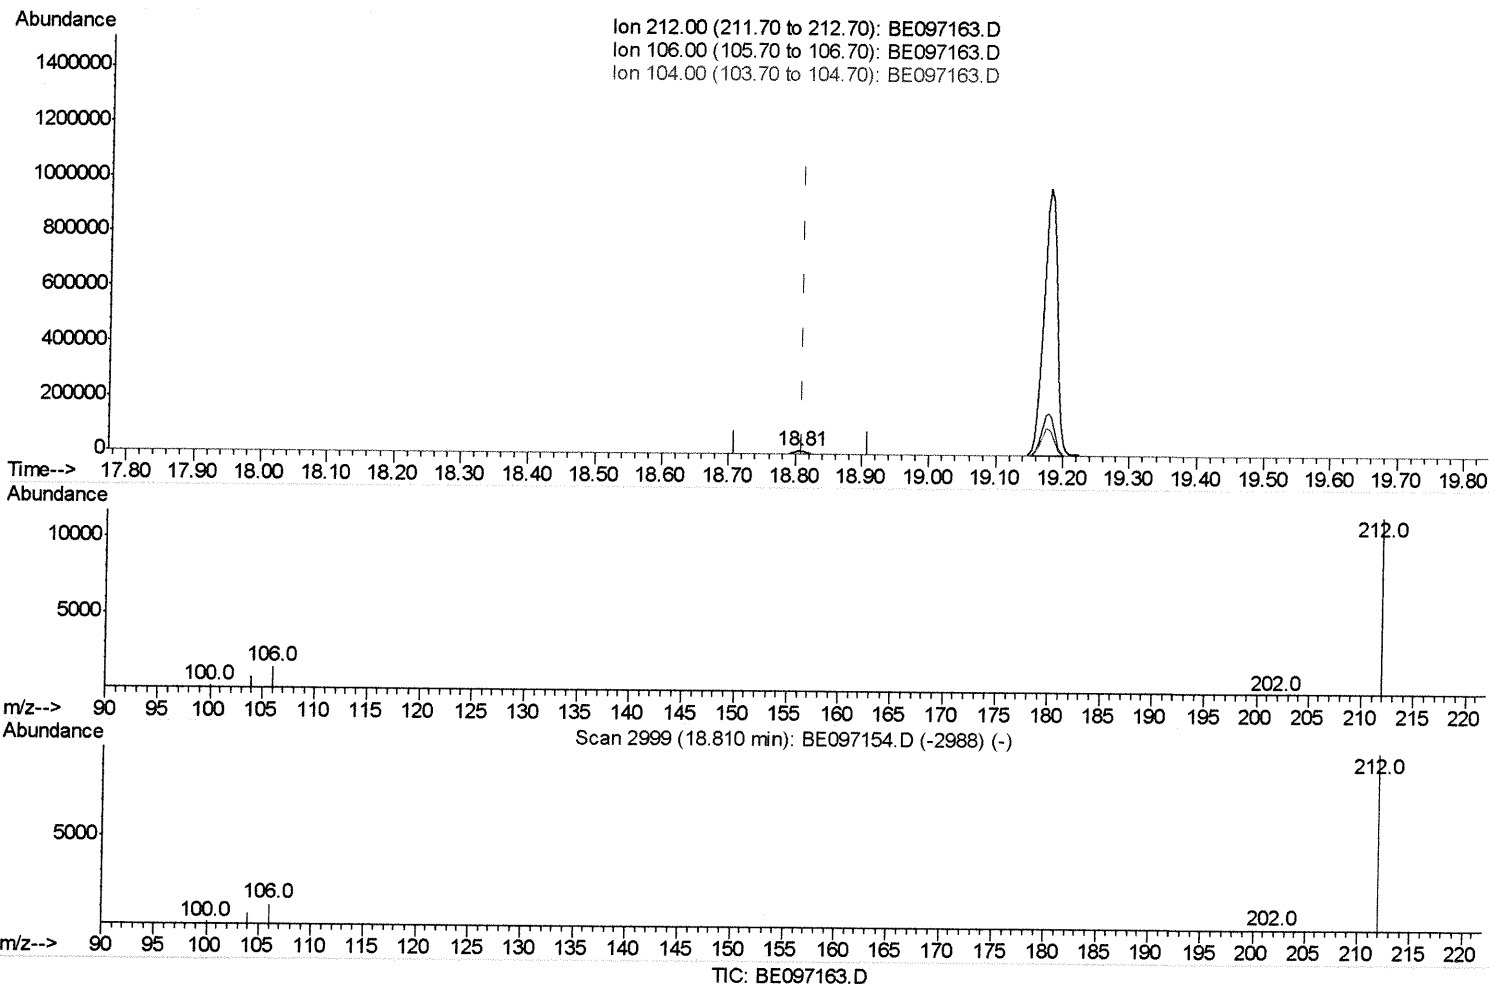

(14) Fluoranthene-d10 (SURR)

18.807min (-0.003) 0.40ng/ul m

> SJ 8/9/18

response 15286

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

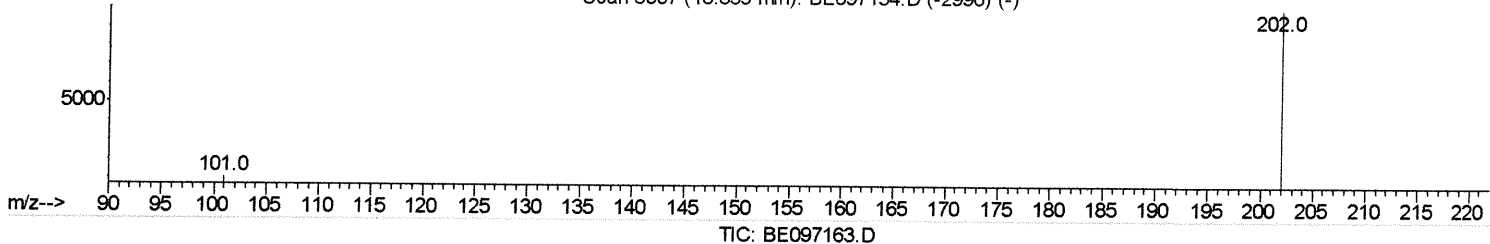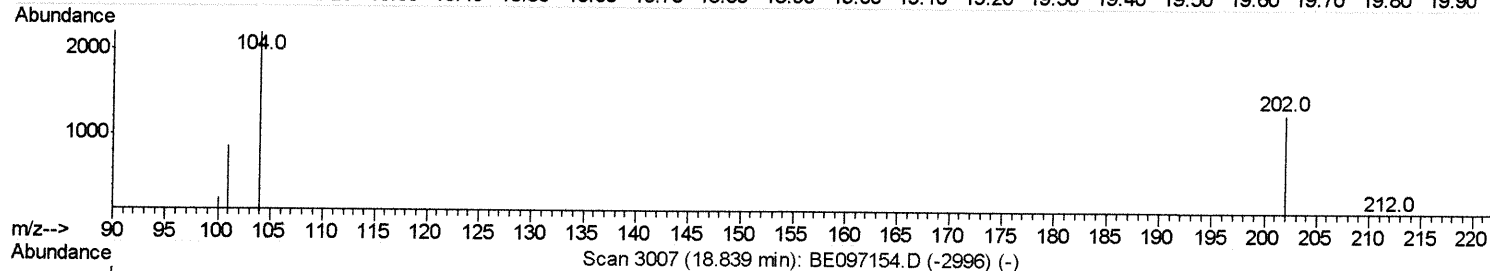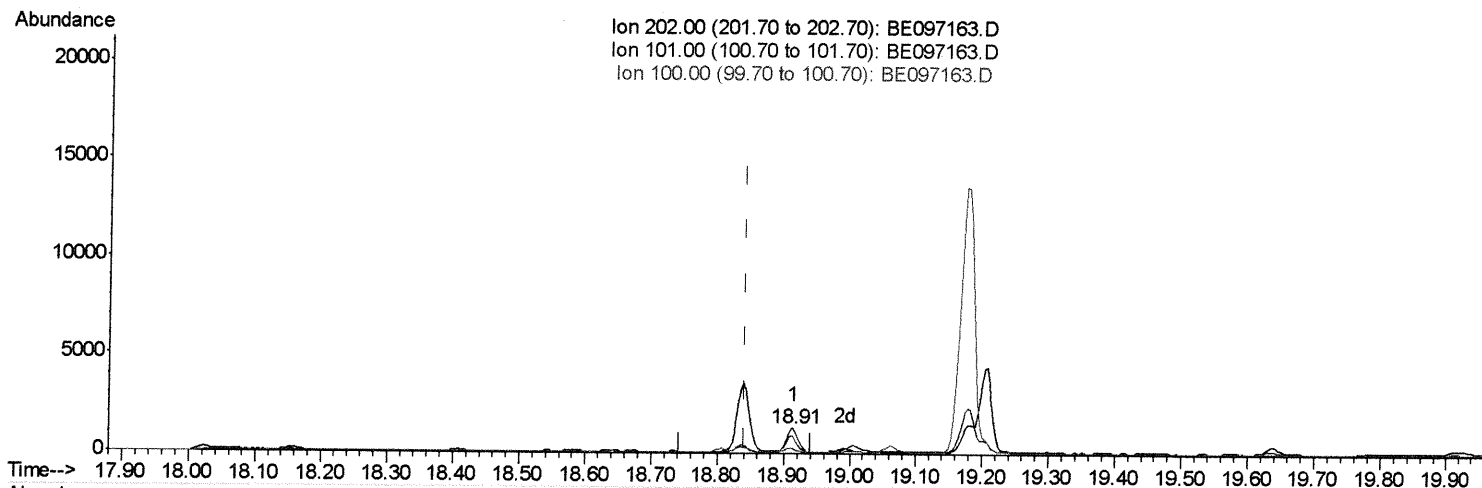

(15) Fluoranthene (C)

18.914min (+0.072) 0.04ng/ul

response 1468

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	67.29#
100.00	19.50	19.69
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

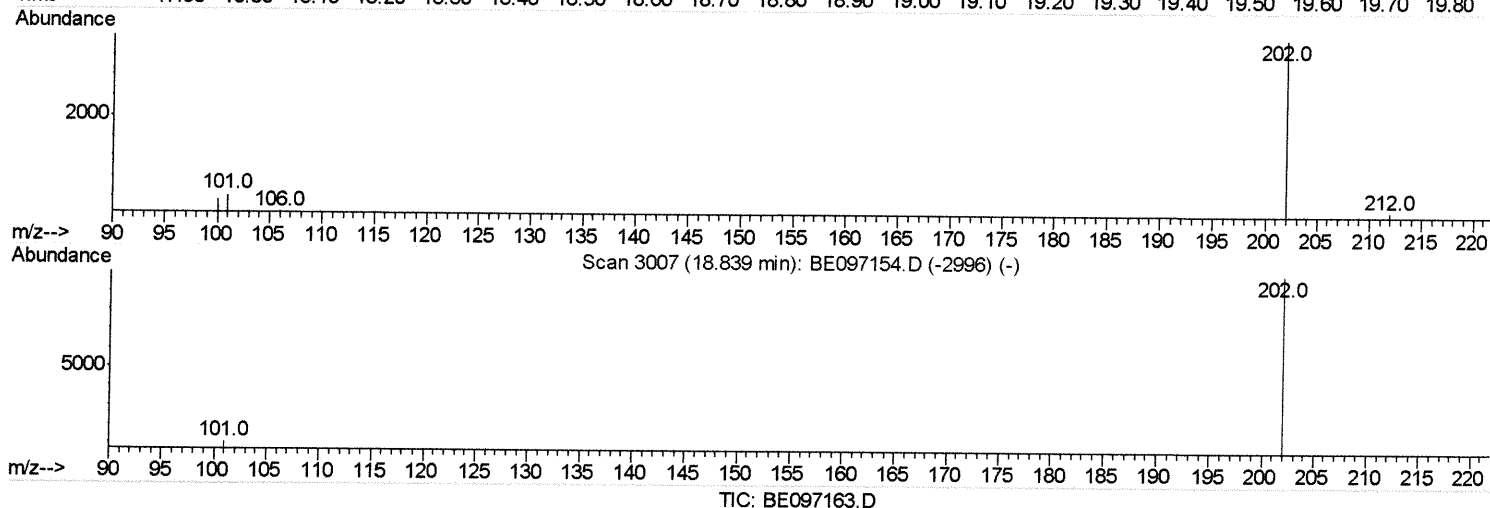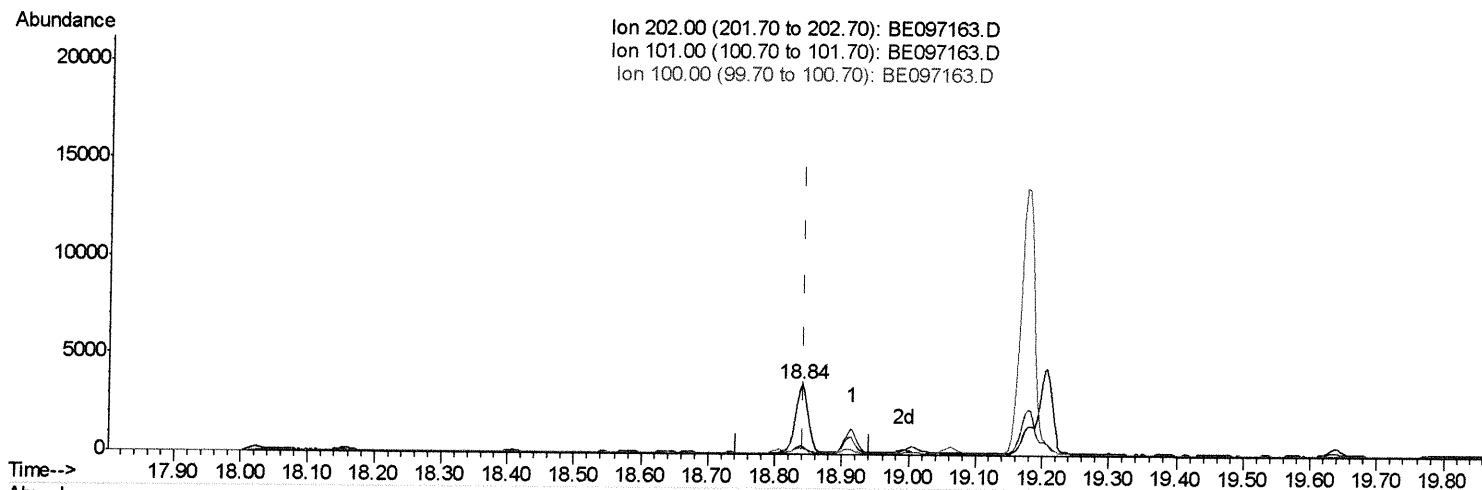

(15) Fluoranthene (C)

18.839min (-0.003) 0.12ng/ul m) SJ 8/9/18

response 4534

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.09
100.00	19.50	9.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

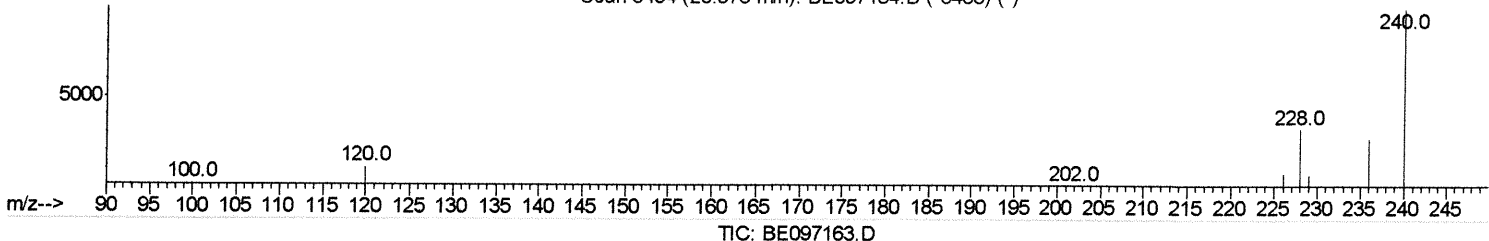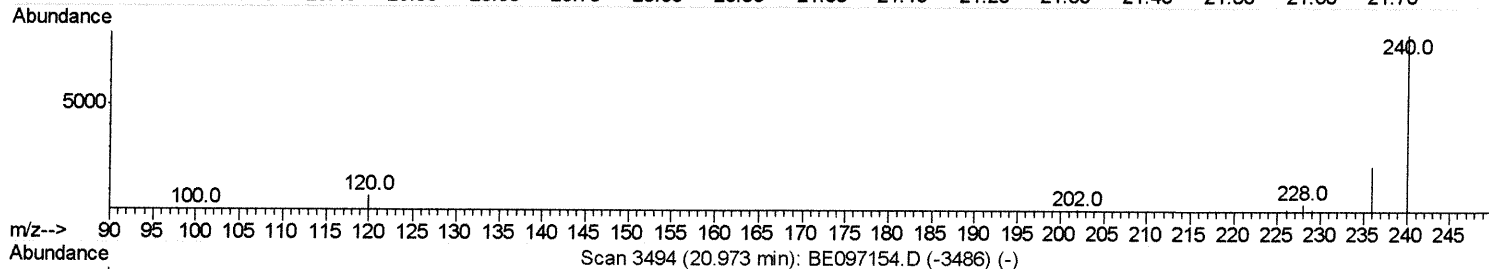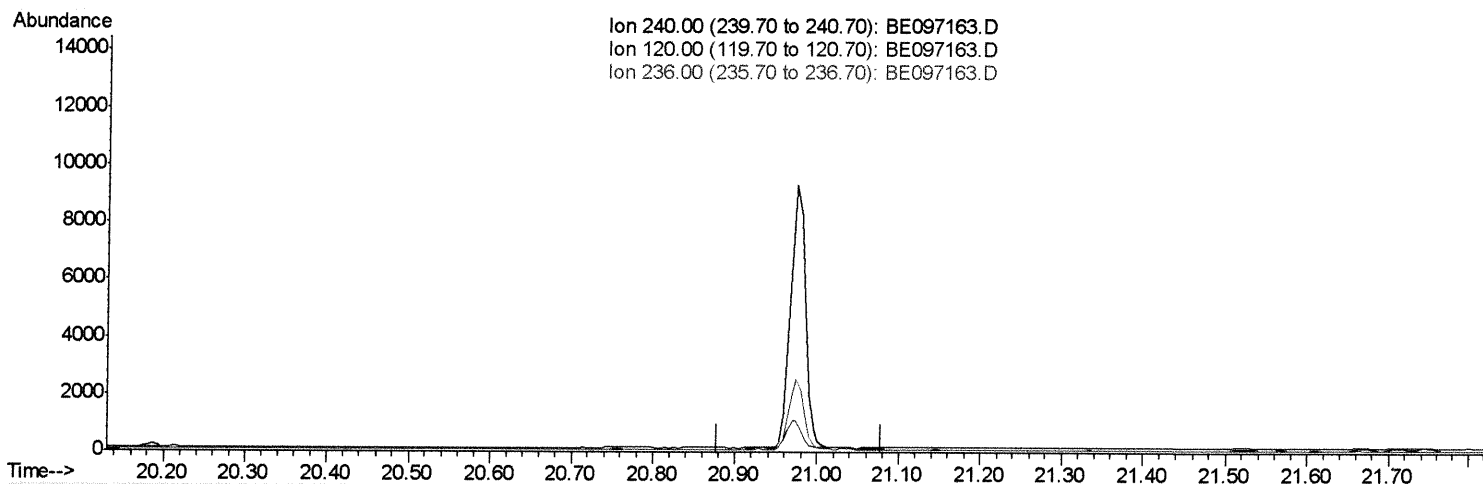

(16) Chrysene-d12 (I)

20.979min (-20.979) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:16:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

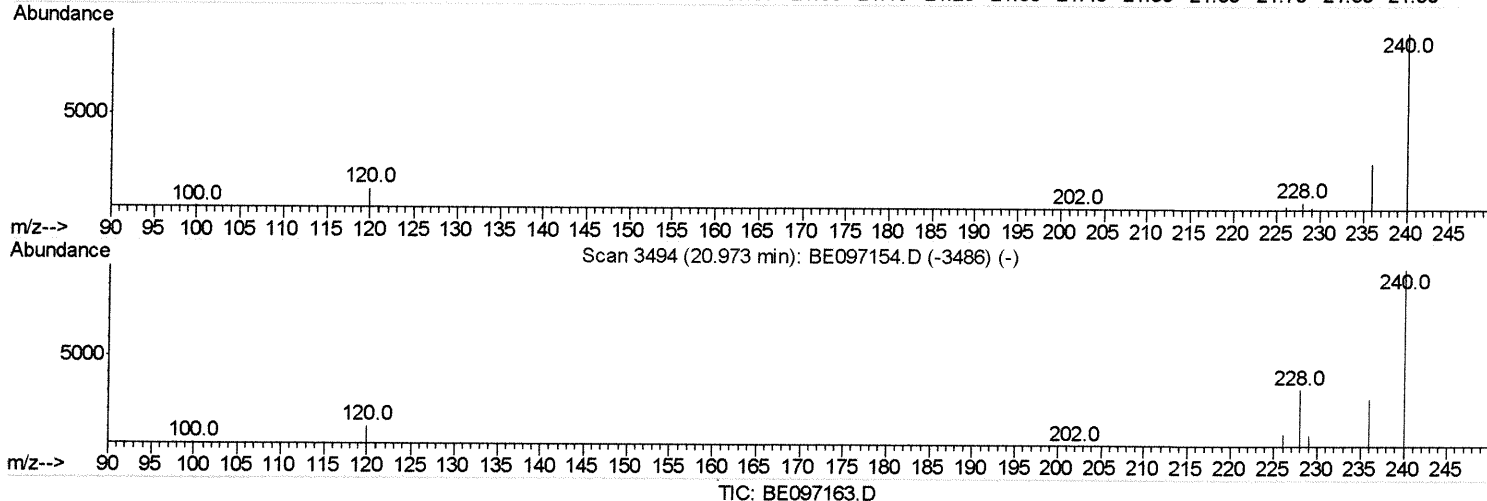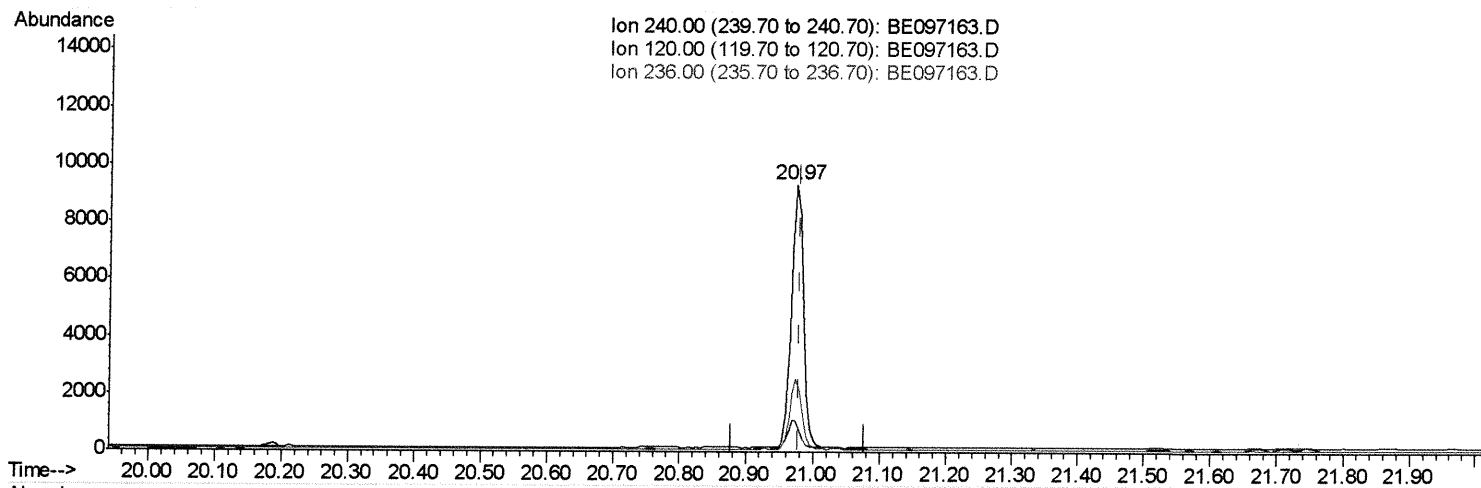

(16) Chrysene-d12 (I)

20.974min (-0.005) 0.40ng/ul m

SD 8/9/18

response 11942

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.74#
236.00	34.90	27.38#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:18:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

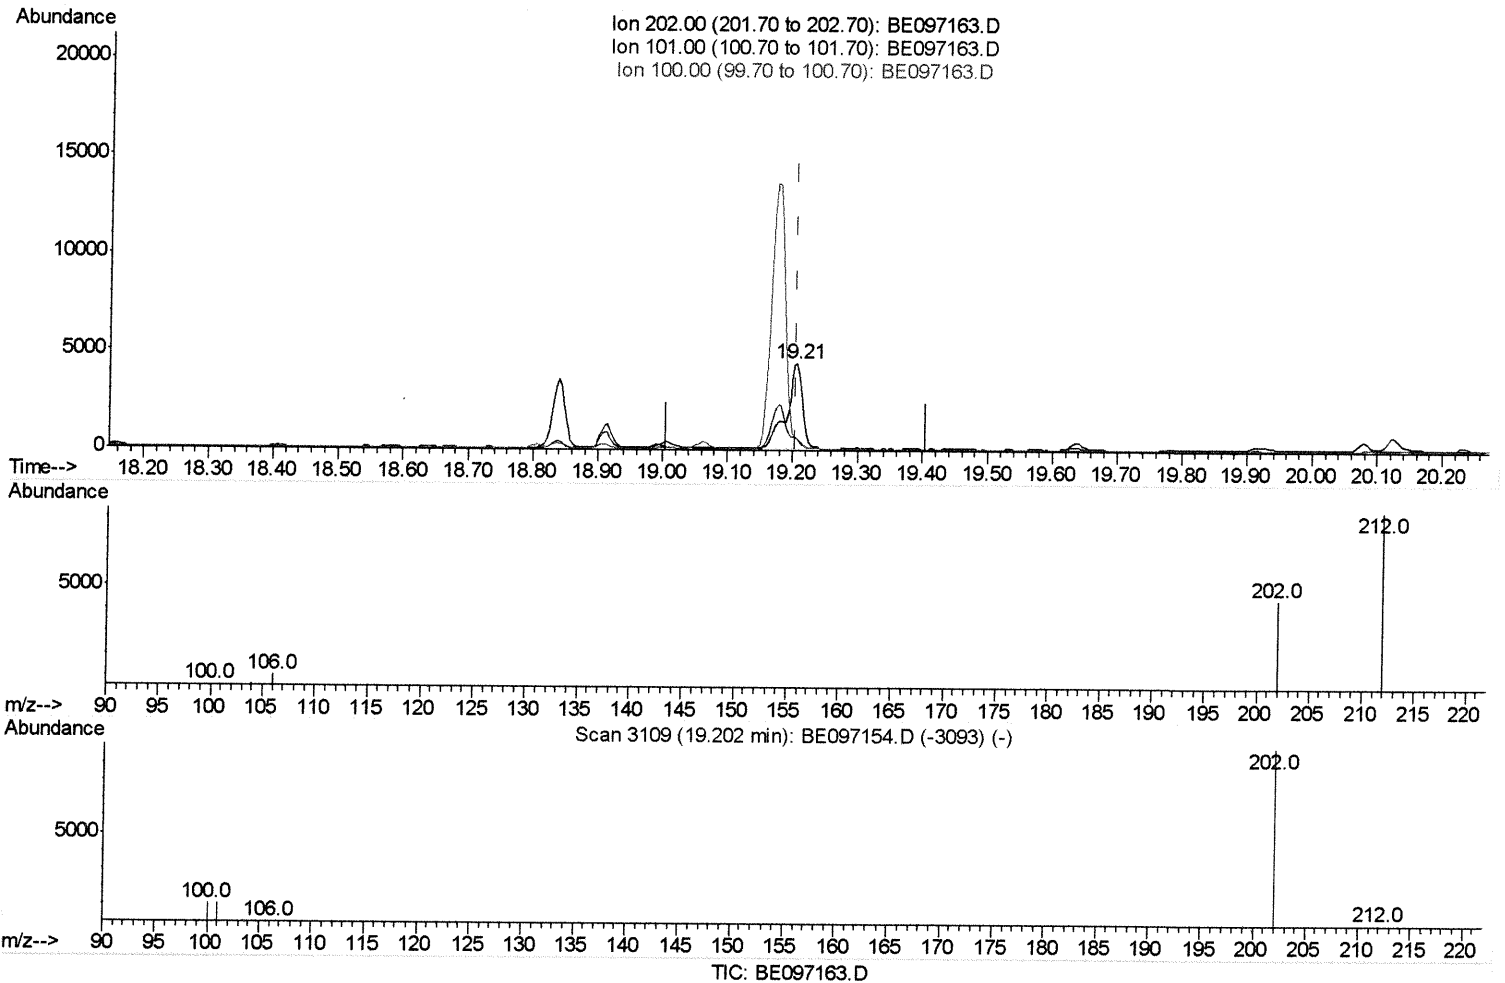

(17) Pyrene

19.206min (+0.001) 0.24ng/ul

response 7530

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	13.30#
100.00	19.50	13.44#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:18:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

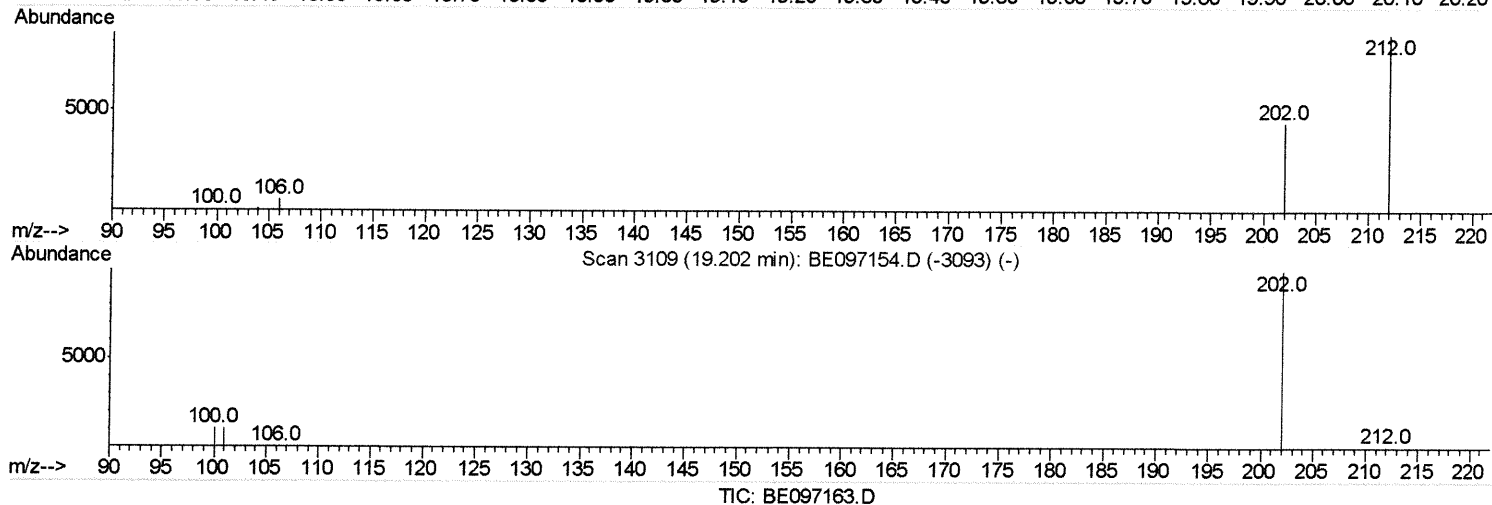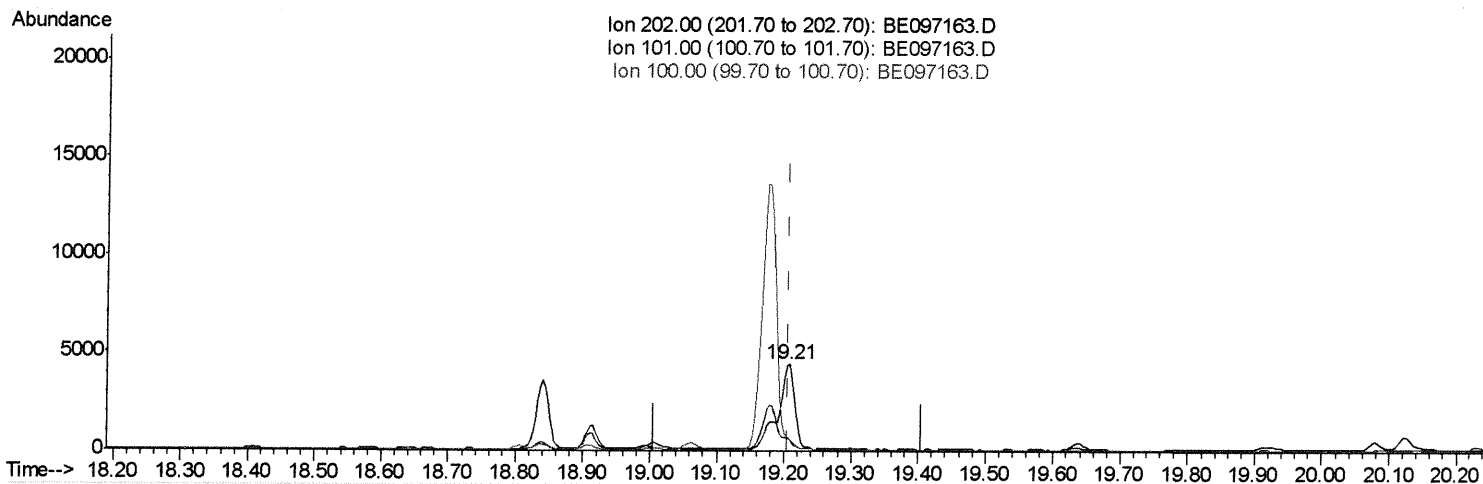

(17) Pyrene

19.206min (+0.001) 0.17ng/ul m > SJ 8/9/18

response 5566

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	13.30#
100.00	19.50	13.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:18:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

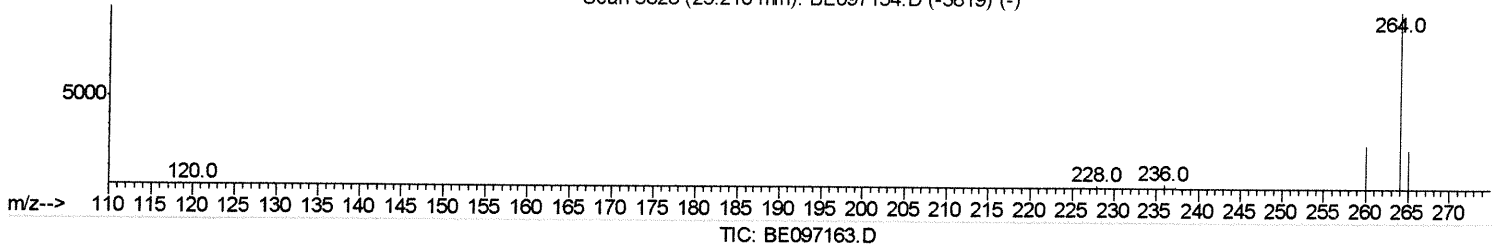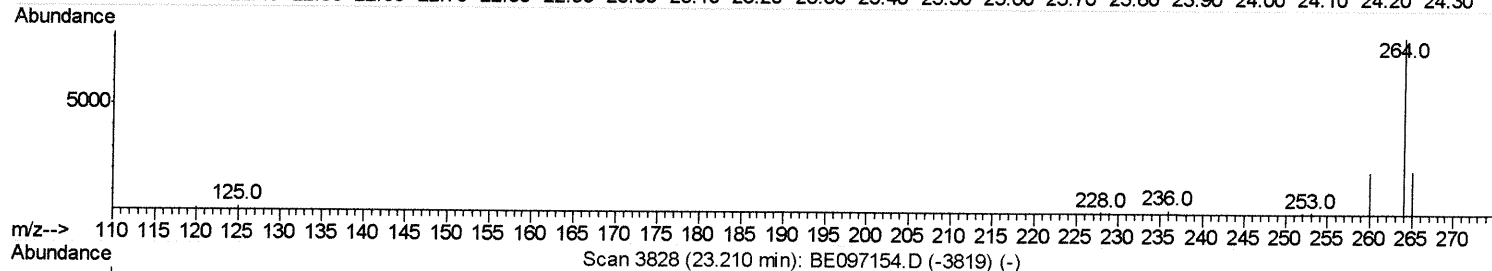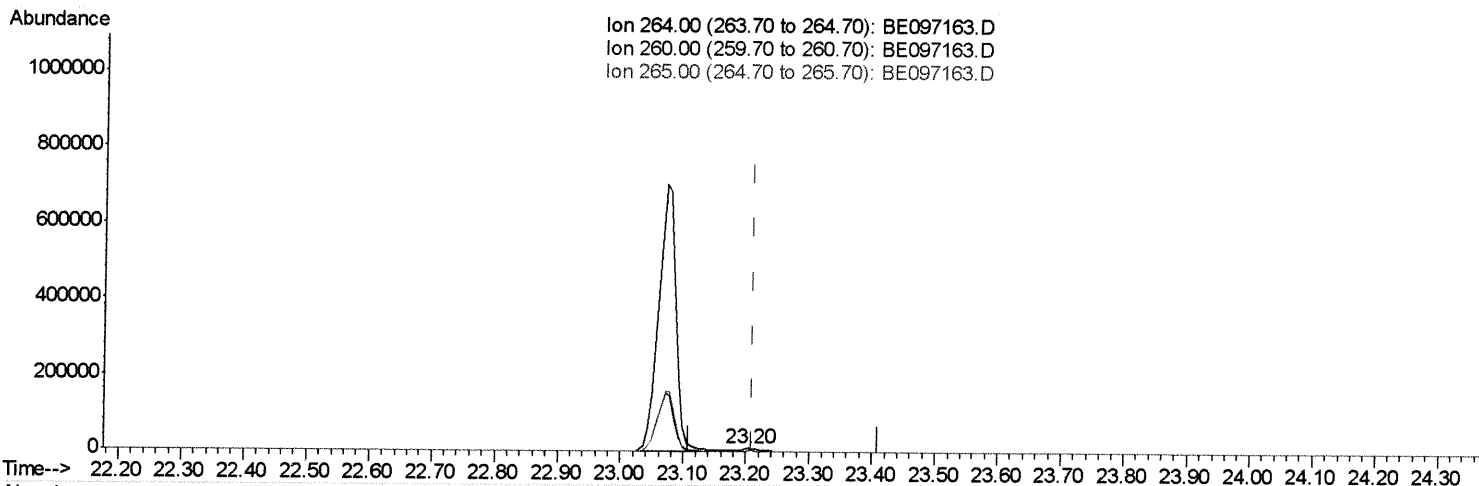

(20) Perylene-d12 (I)
 23.203min (-0.006) 0.40ng/ul
 response 19127

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.57
265.00	103.50	25.33#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:18:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

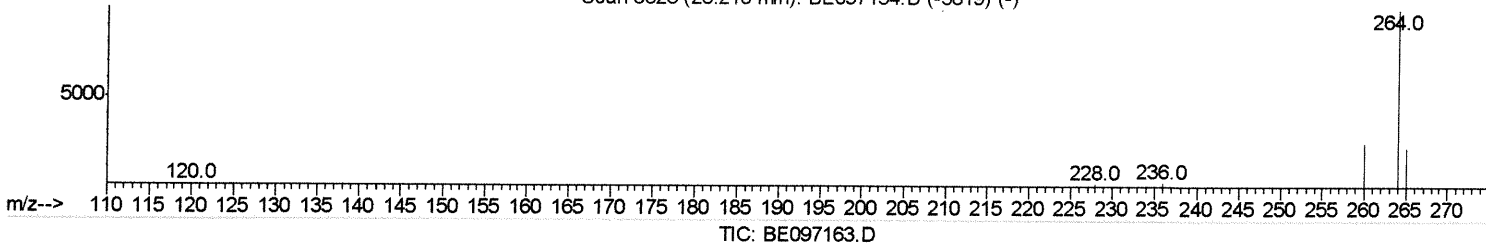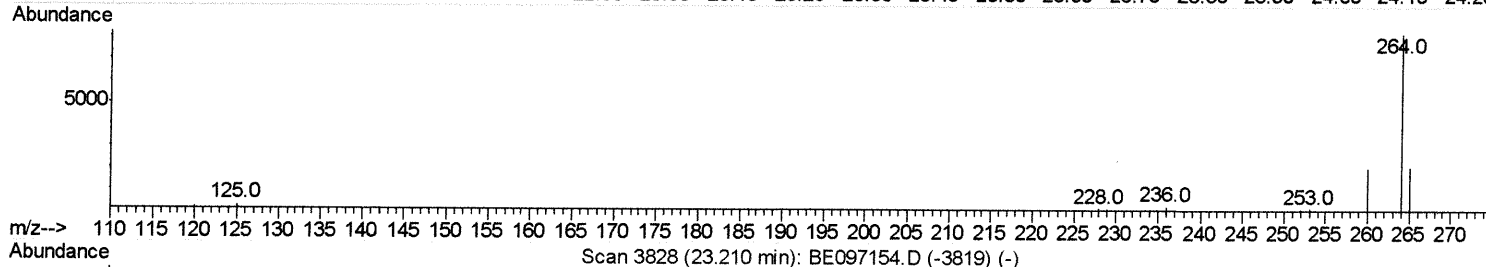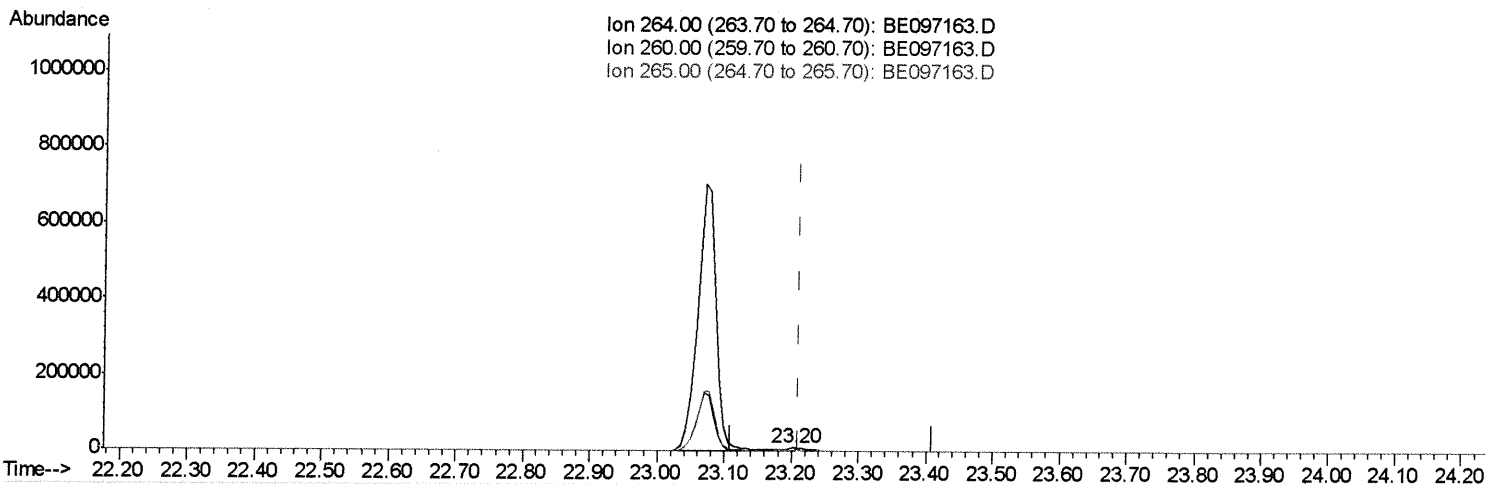

(20) Perylene-d12 (I)

23.203min (-0.006) 0.40ng/ul m

response 10244

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.57
265.00	103.50	25.33#
0.00	0.00	0.00

> 50 8/9/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:21:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

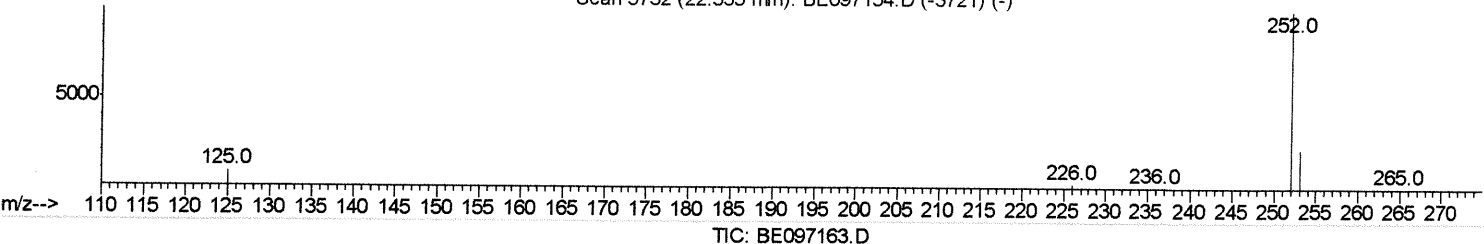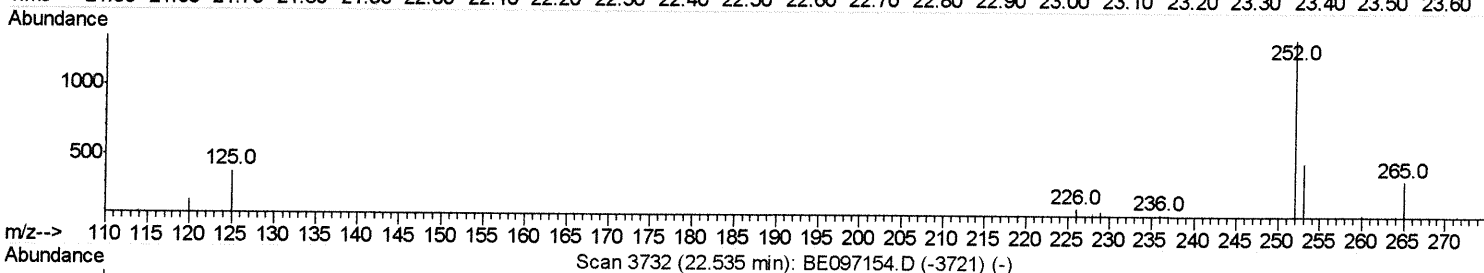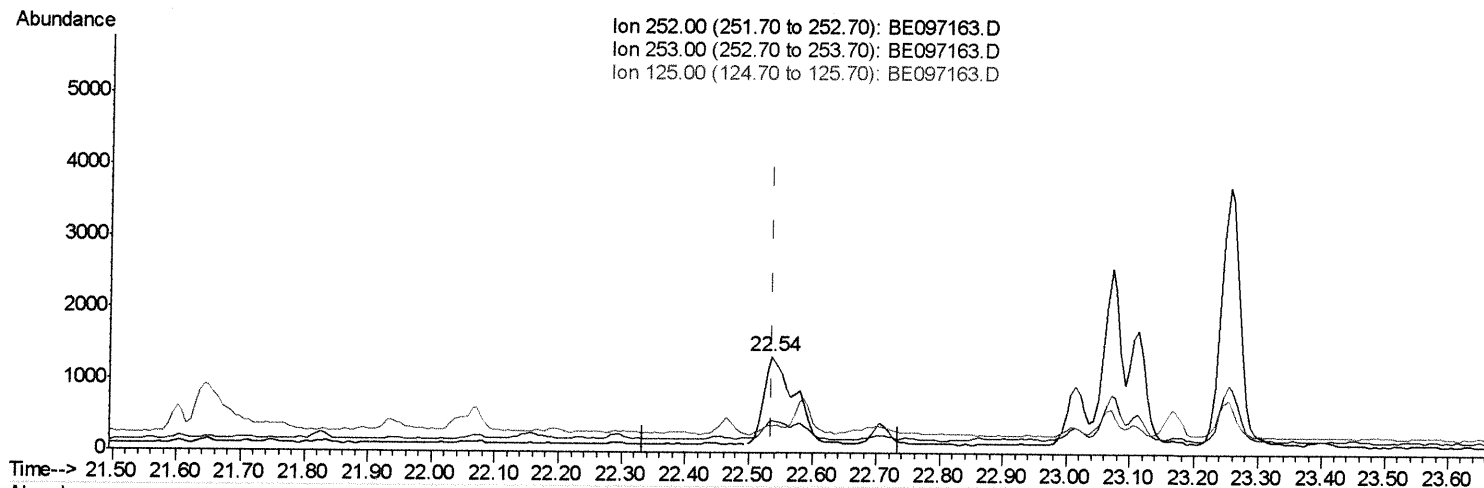

(21) Benzo(b)fluoranthene

22.535min (+0.001) 0.14ng/ul

response 4020

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	34.43
125.00	17.50	28.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097163.D
Acq On : 2 Aug 2018 22:36
Operator : SJ/JU
Sample : J4171-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1J4

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:21:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

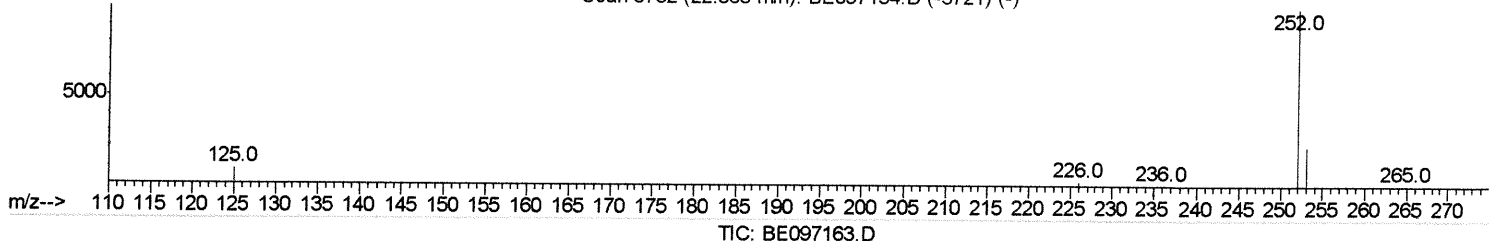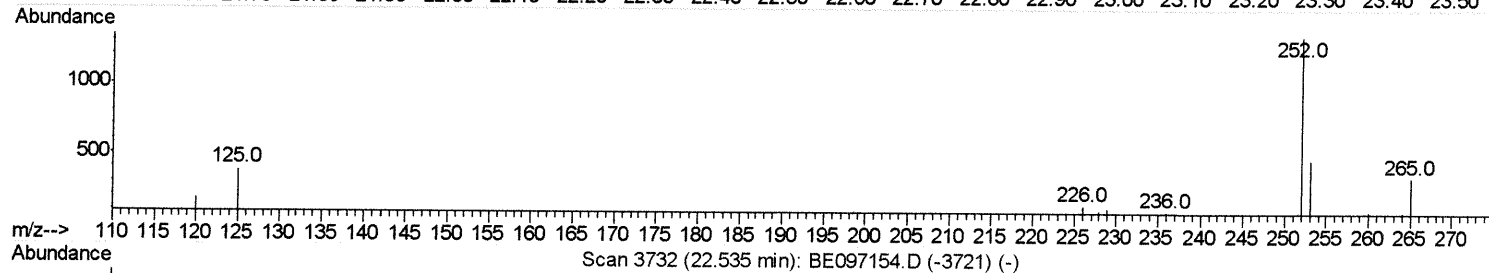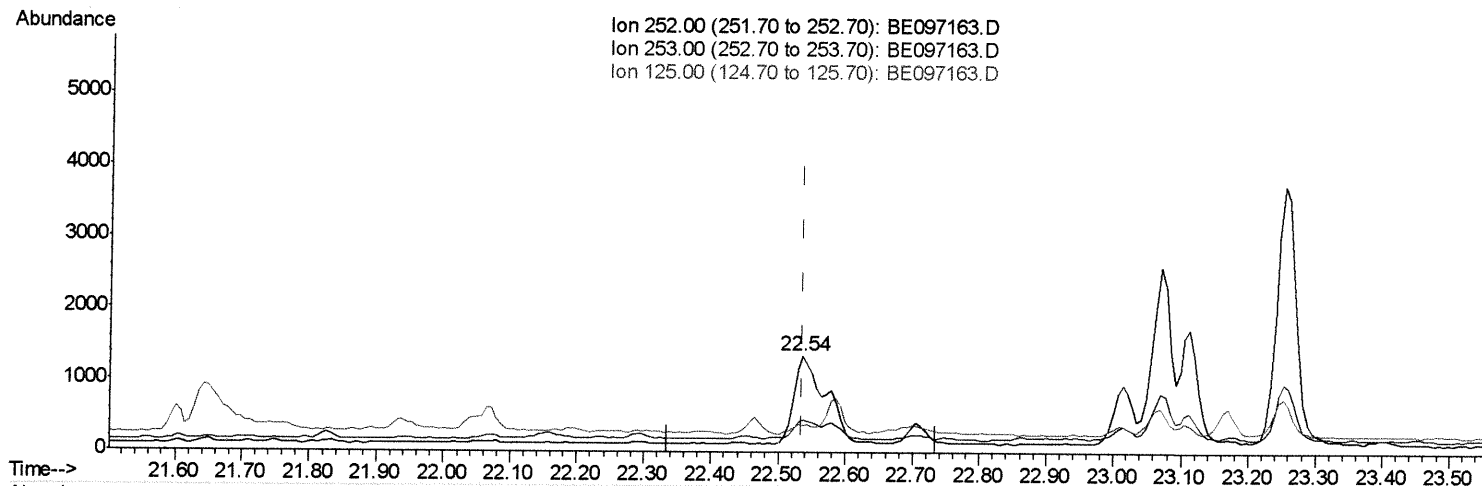

(21) Benzo(b)fluoranthene

22.535min (+0.001) 0.10ng/ul m > SJ 8/9/18

response 2867

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	34.43
125.00	17.50	28.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:21:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

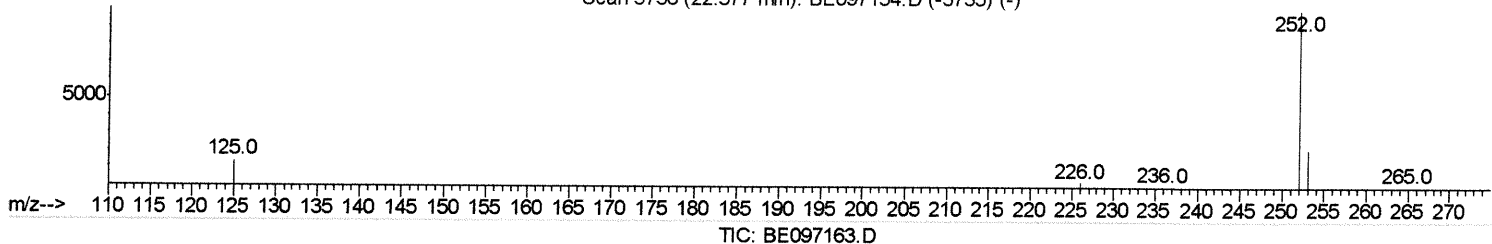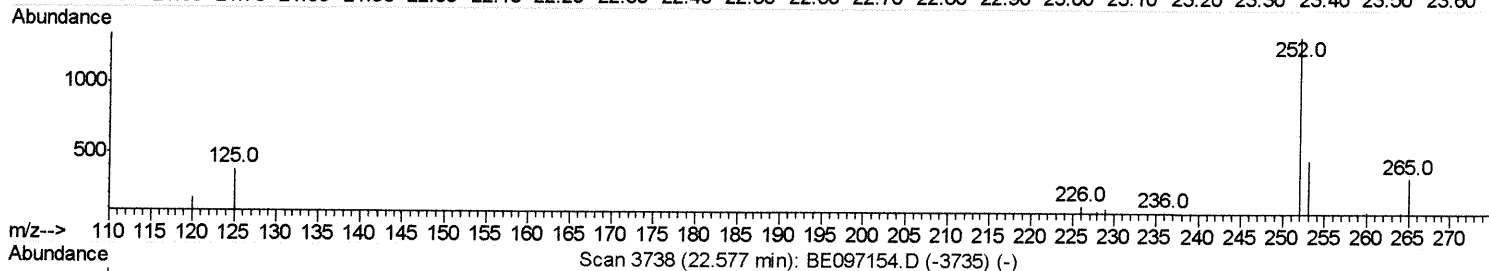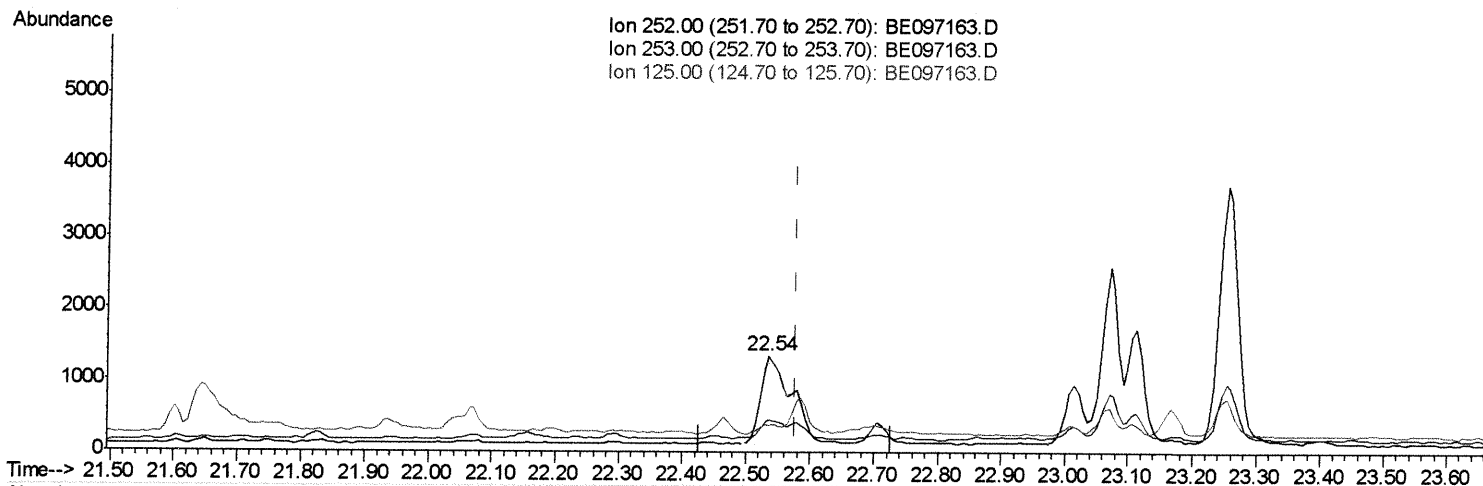

(22) Benzo(k)fluoranthene
 22.535min (-0.042) 0.13ng/ul
 response 4020

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	34.43
125.00	17.10	28.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:21:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

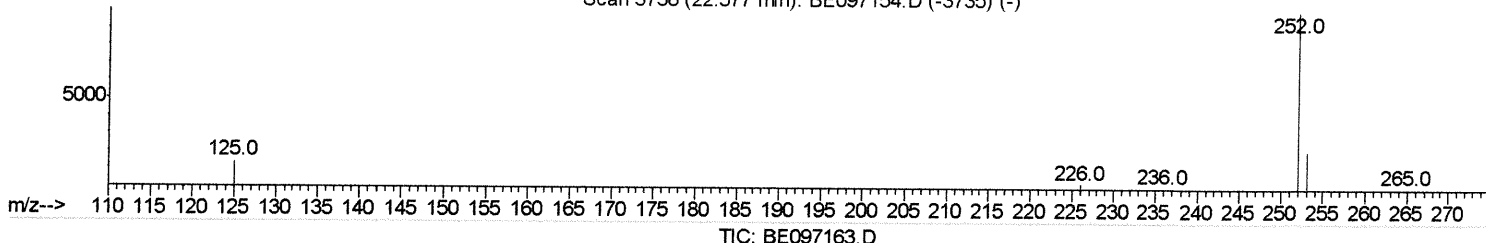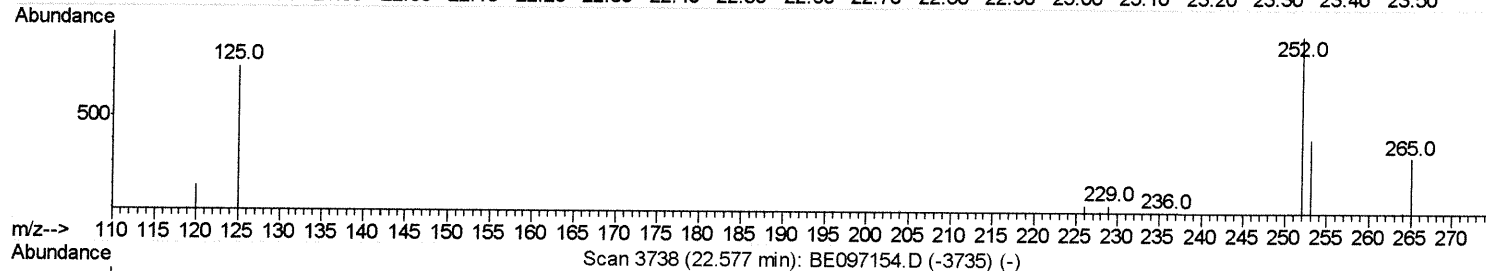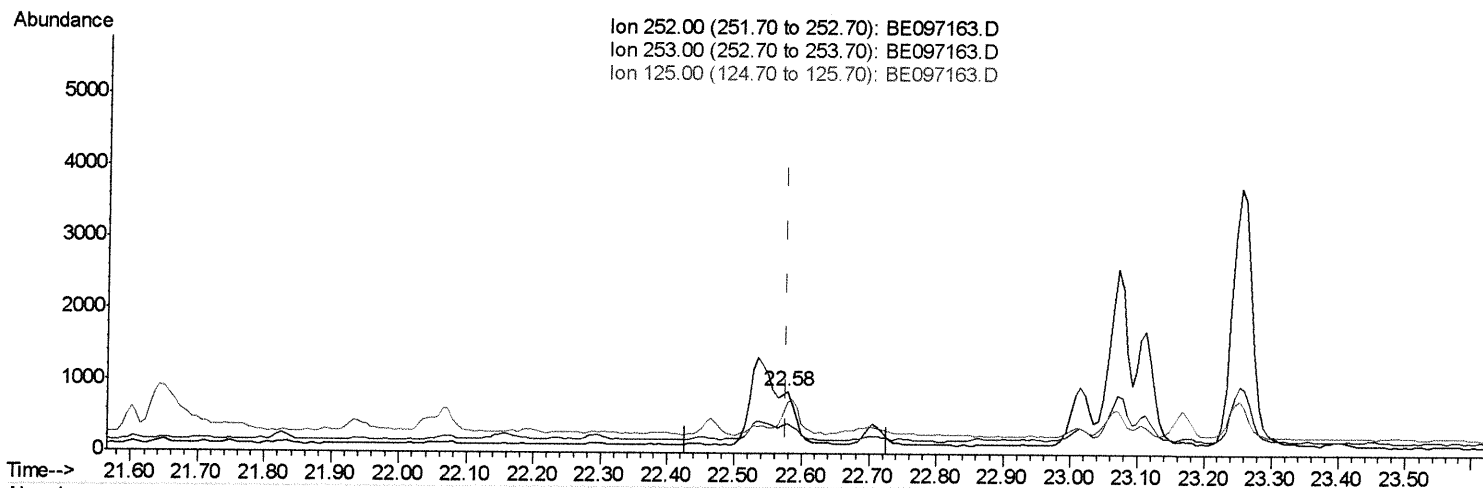

(22) Benzo(k)fluoranthene

22.578min (+0.001) 0.04ng/ul m>50 879118

response 1116

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	48.15#
125.00	17.10	83.03#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097163.D
 Acq On : 2 Aug 2018 22:36
 Operator : SJ/JU
 Sample : J4171-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J4

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:12 PM

Quant Time: Aug 03 00:23:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1340	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6933	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4642	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	11037m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	11942m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	10244m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.73	152	4926	0.44	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	15286m	0.40	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.18	128	1862	0.111	ng/ul#	93
5) 2-Methylnaphthalene	11.80	142	367	0.033	ng/ul	94
12) Phenanthrene	16.81	178	3654m	0.130	ng/ul	
15) Fluoranthene	18.84	202	4534m	0.122	ng/ul	
17) Pyrene	19.21	202	5566m	0.174	ng/ul	
18) Benzo(a)anthracene	20.96	228	2318	0.068	ng/ul#	85
19) Chrysene	21.01	228	2862	0.081	ng/ul#	88
21) Benzo(b)fluoranthene	22.54	252	2867m	0.103	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	1116m	0.037	ng/ul	
23) Benzo(a)pyrene	23.11	252	2746	0.098	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	25.50	276	1624	0.046	ng/ul#	83
26) Benzo(g,h,i)perylene	26.20	276	1780	0.059	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed