

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:10:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

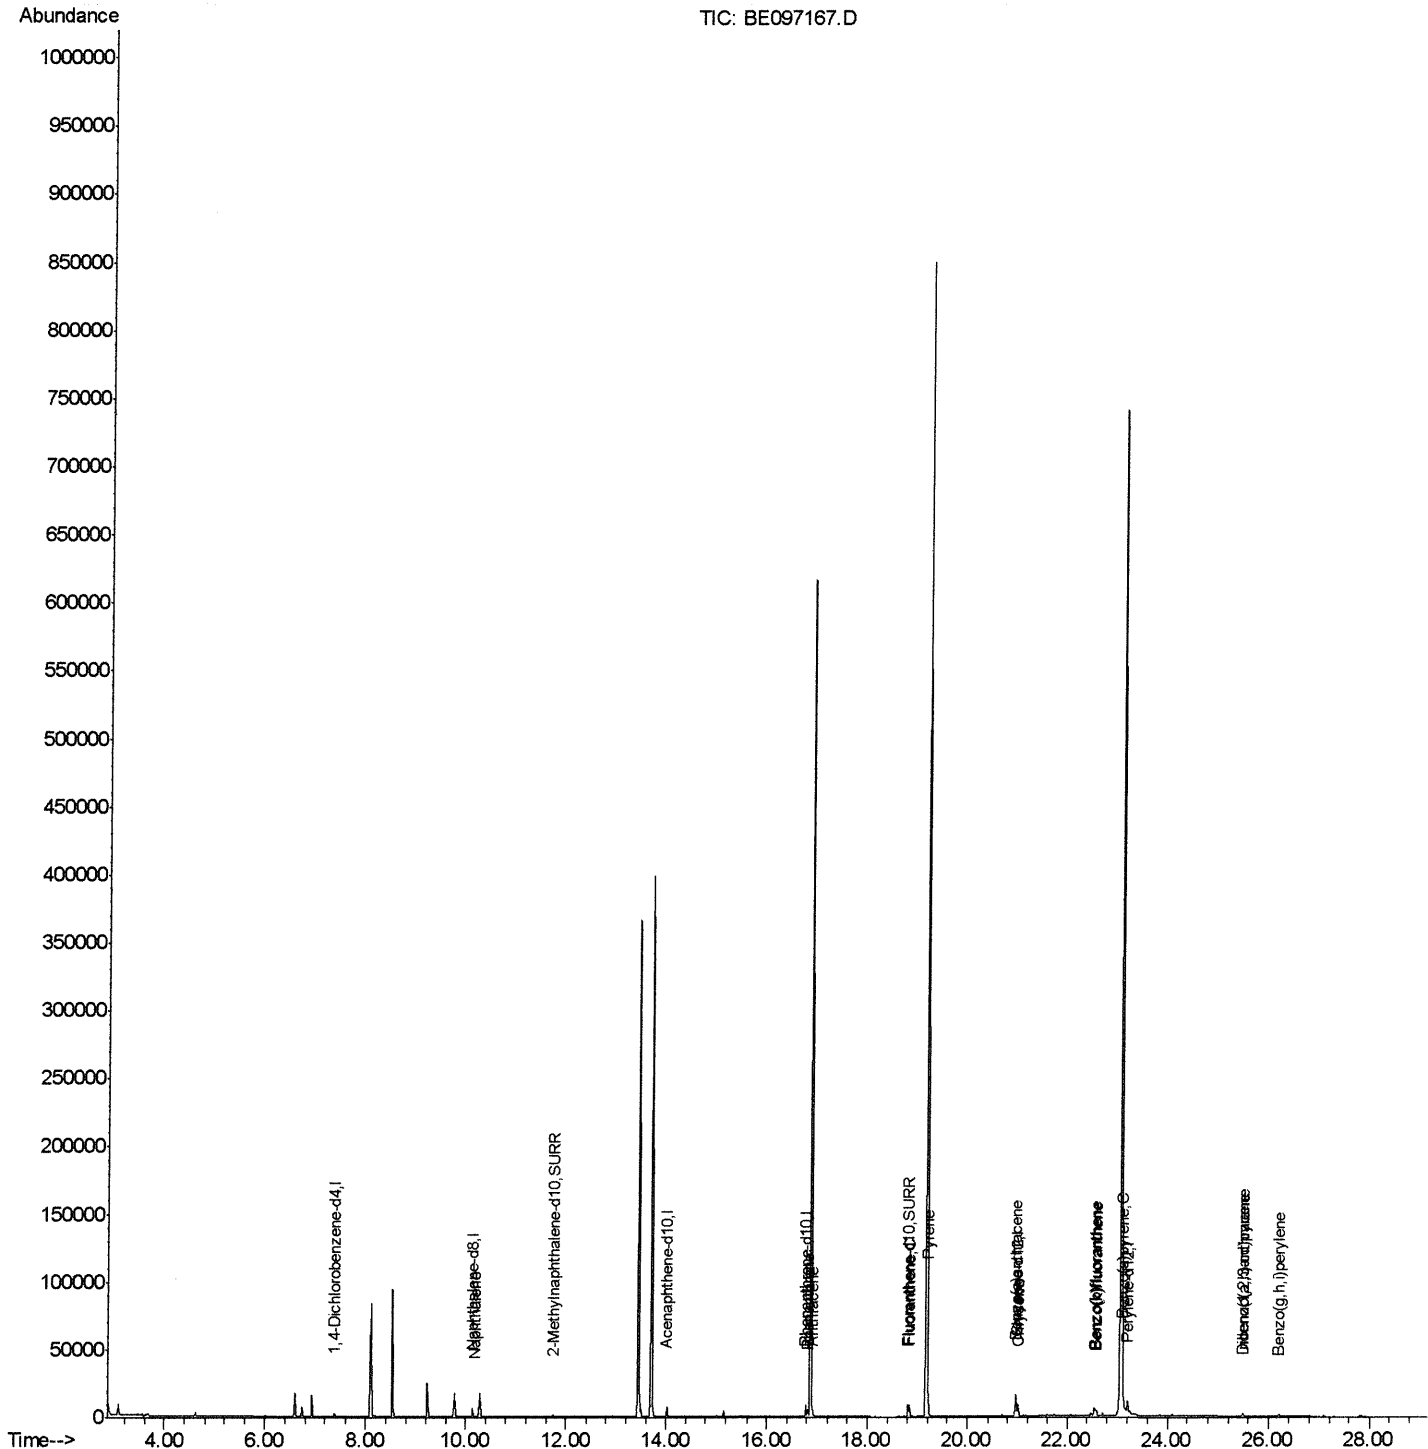

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 03:07:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

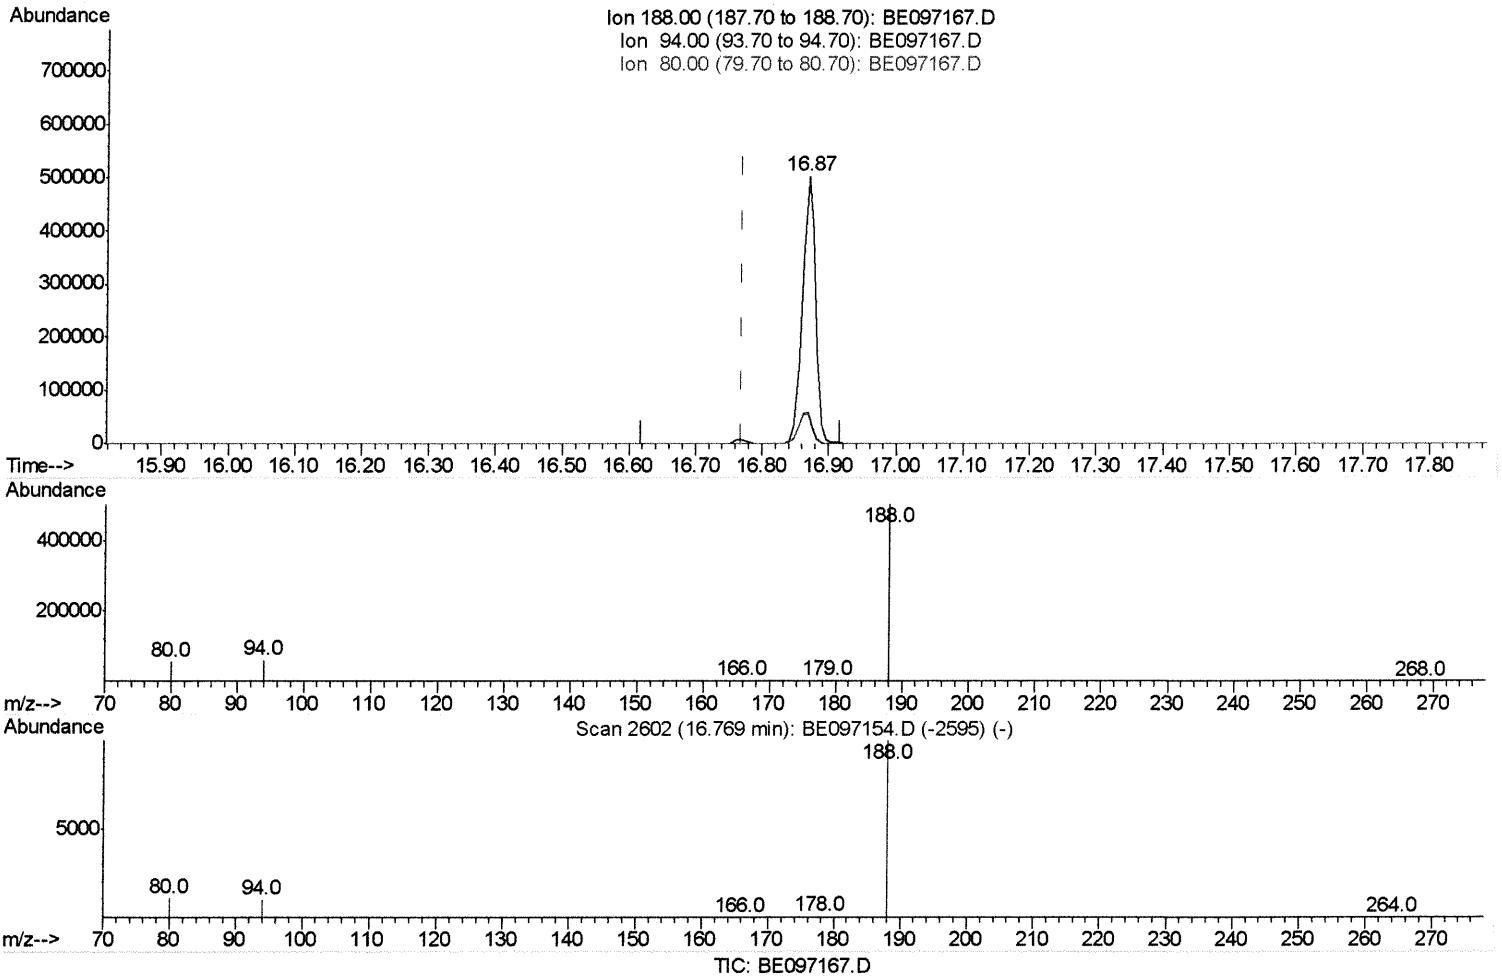

(10) Phenanthrene-d10 (I)

16.868min (+0.099) 0.40ng/ul

response 699340

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.84
80.00	11.80	10.78
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 03:07:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

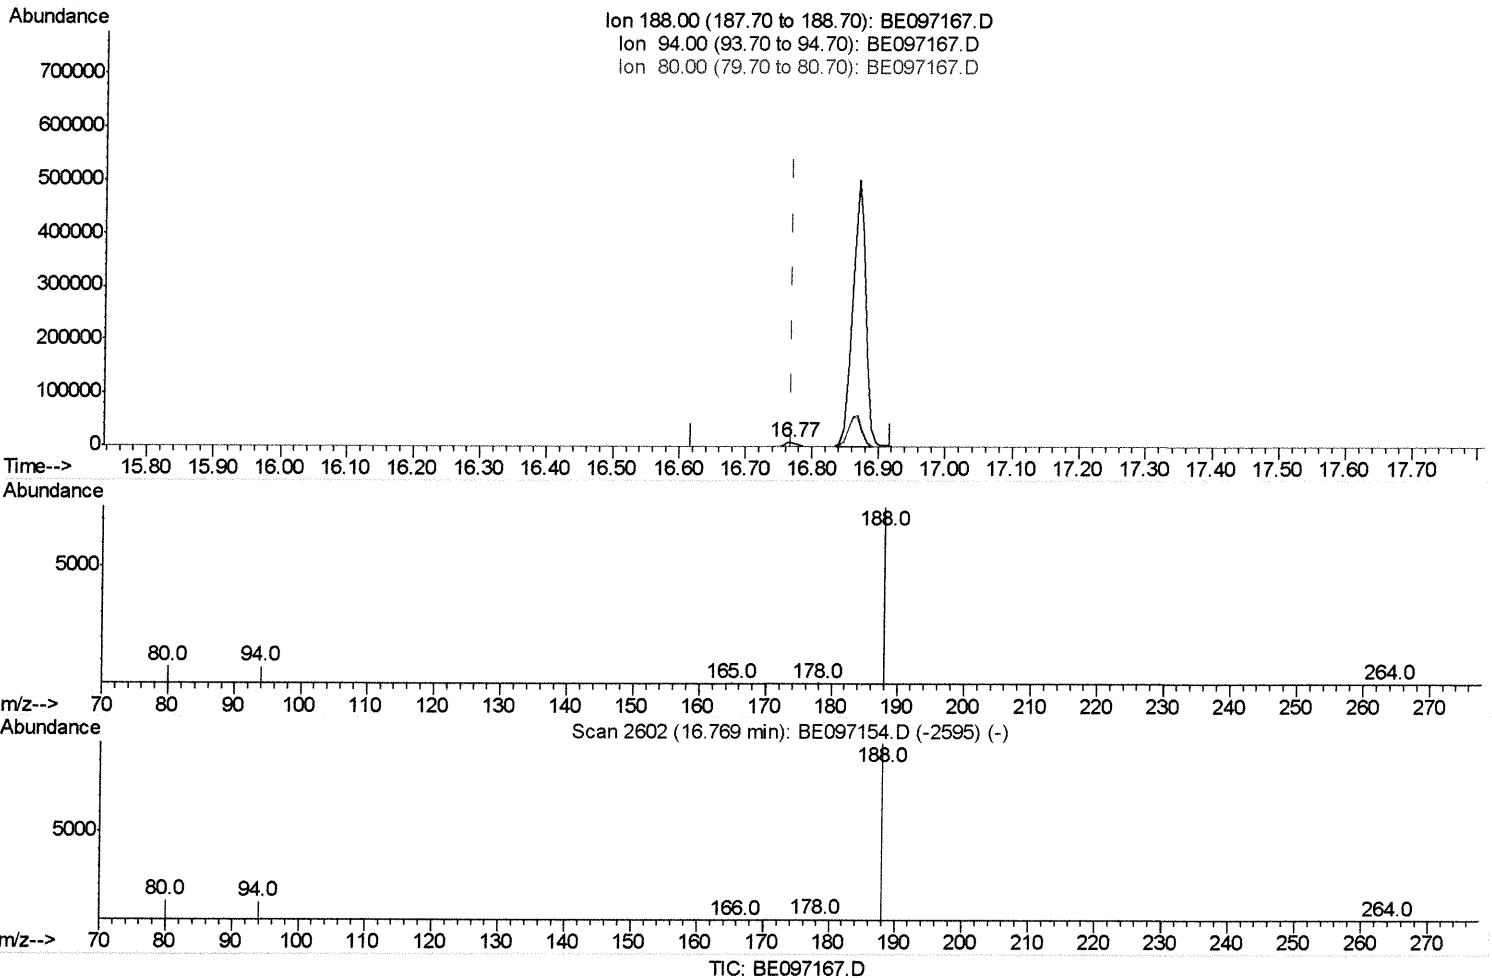

(10) Phenanthrene-d10 (I)

16.769min (+0.000) 0.40ng/ul m> SJ 8/9/18

response 10758

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.60
80.00	11.80	10.11
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

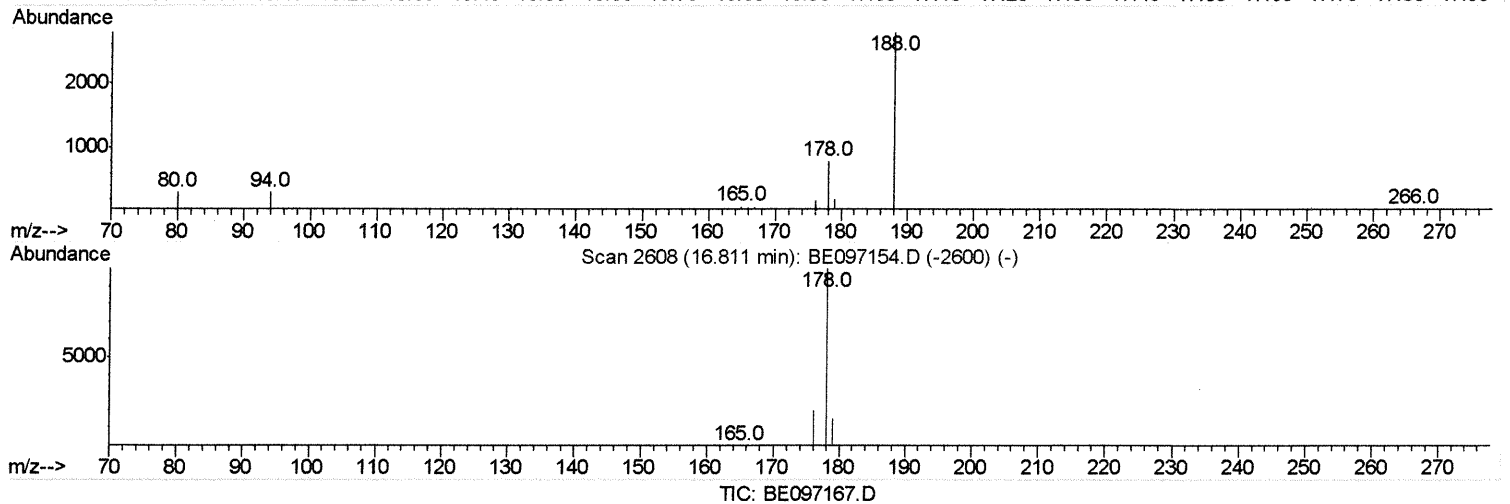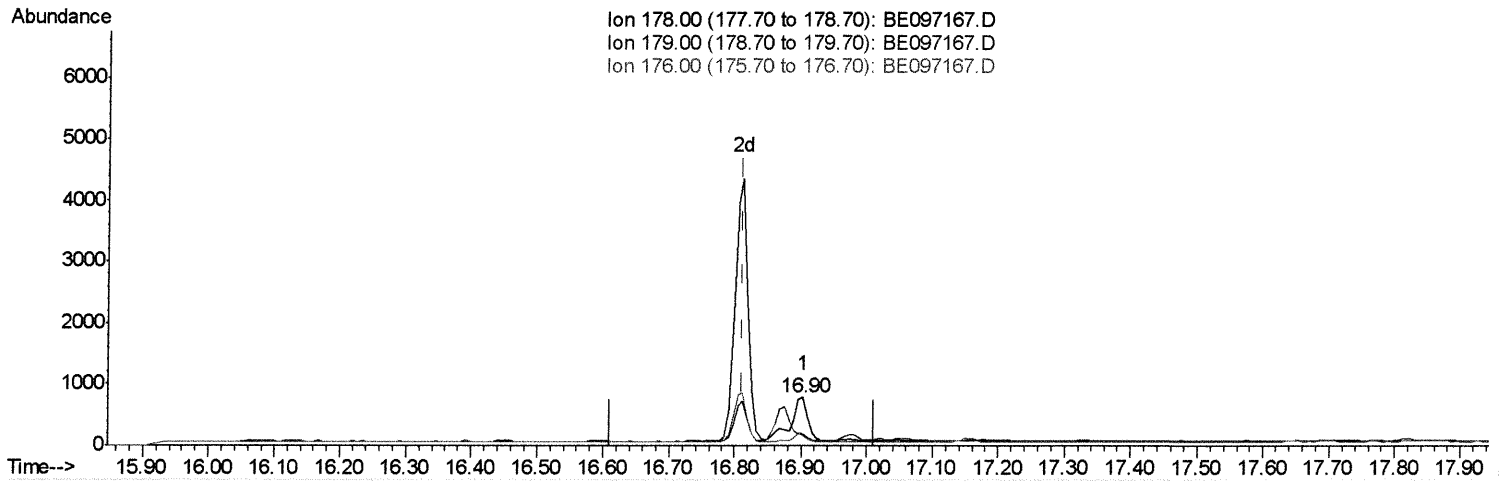

(12) Phenanthrene

16.903min (+0.092) 0.05ng/ui

response 1299

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	24.62
176.00	17.00	23.98#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

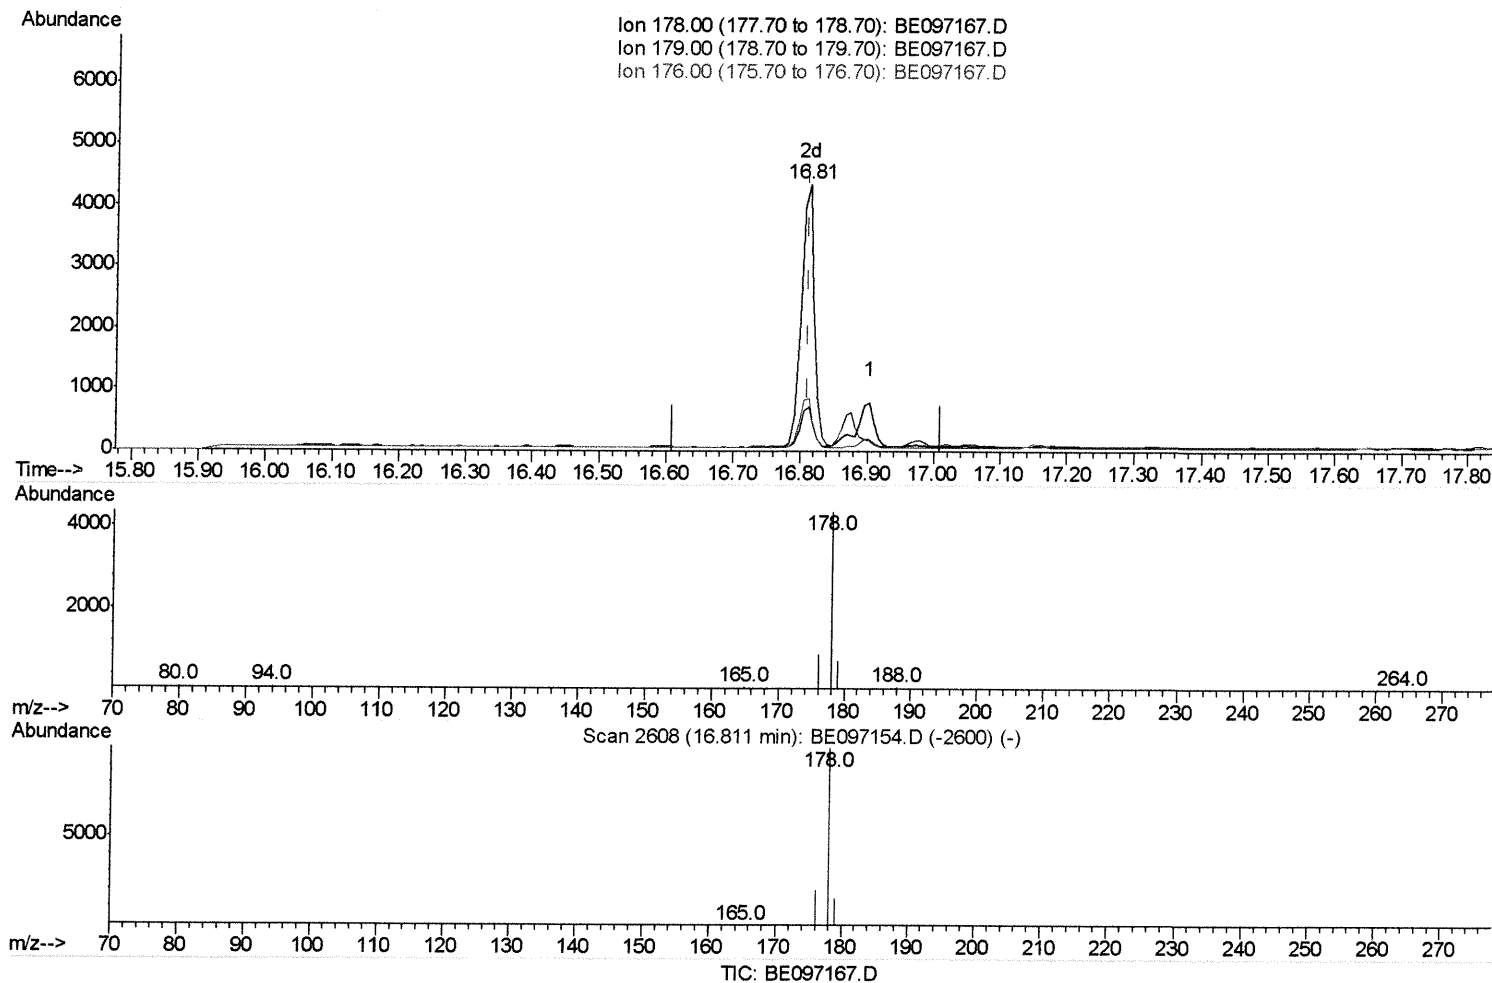

(12) Phenanthrene

16.811min (+0.000) 0.22ng/ul m

> SJ 8/9/18

response 5965

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	16.69#
176.00	17.00	19.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

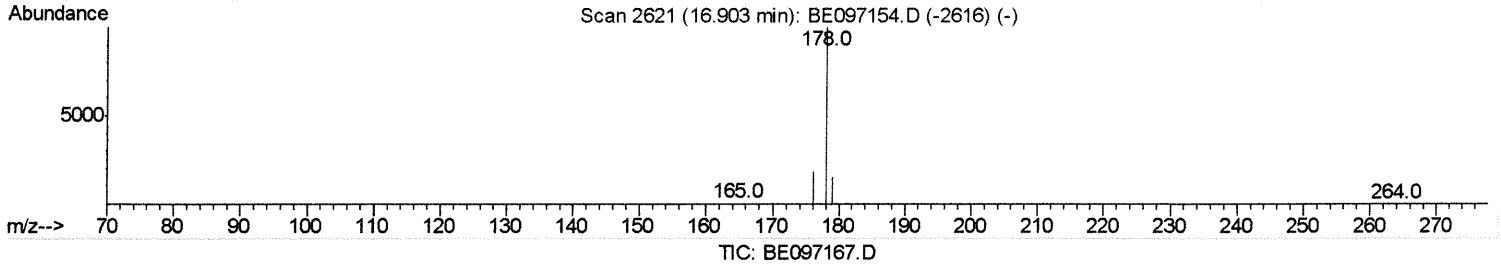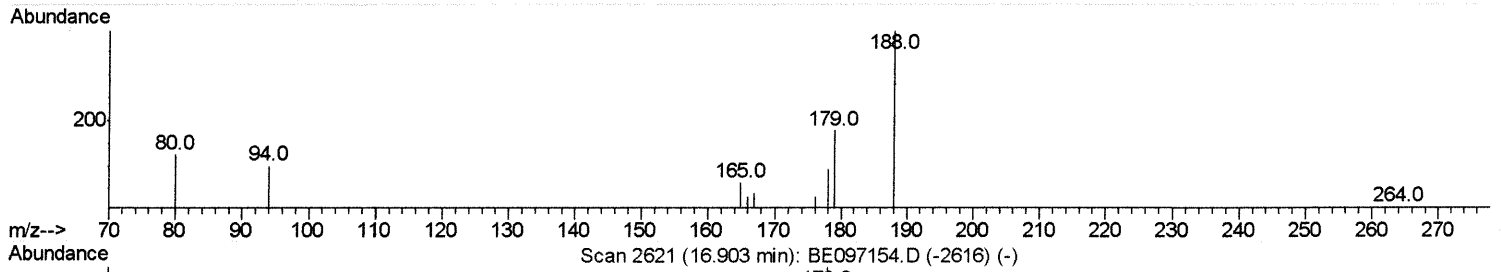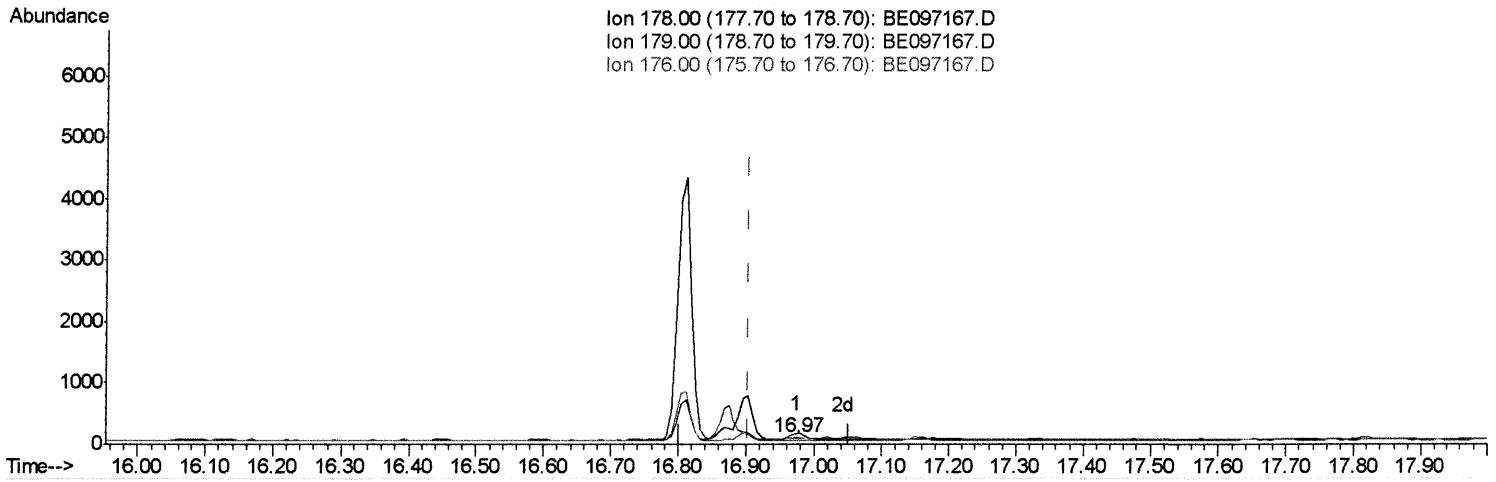

(13) Anthracene

16.973min (+0.071) 0.00ng/ul

response 50

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	158.26#
176.00	18.40	57.39#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

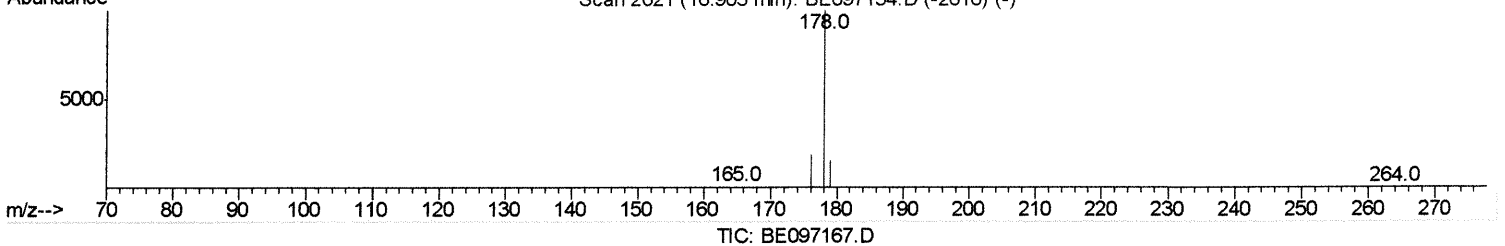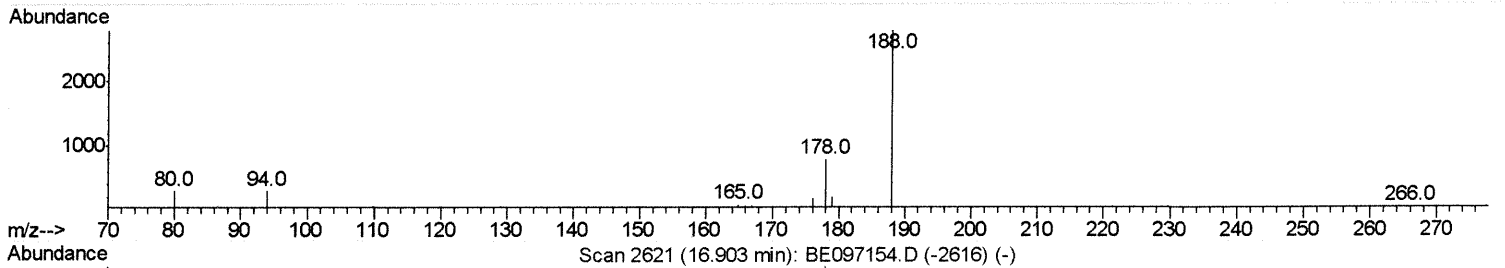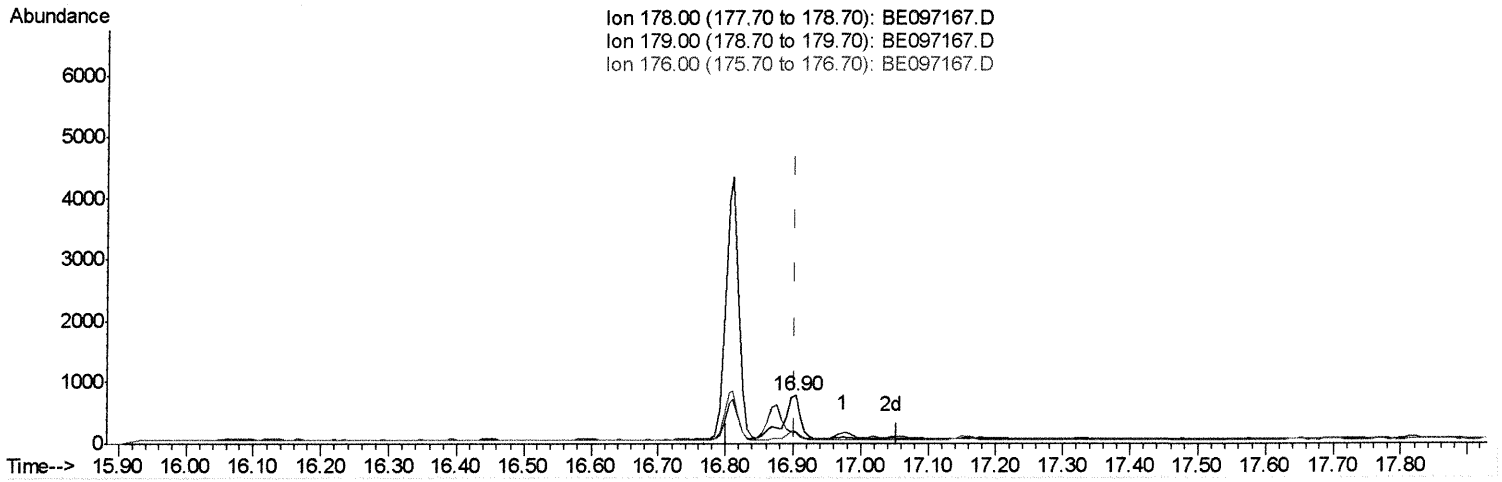

(13) Anthracene

16.903min (+0.000) 0.04ng/ul m > 50 8/9/18

response 959

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	24.62
176.00	18.40	23.98#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

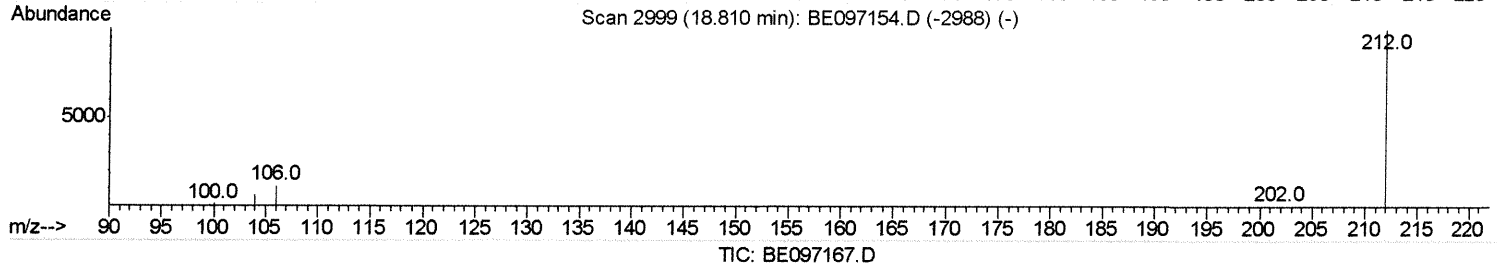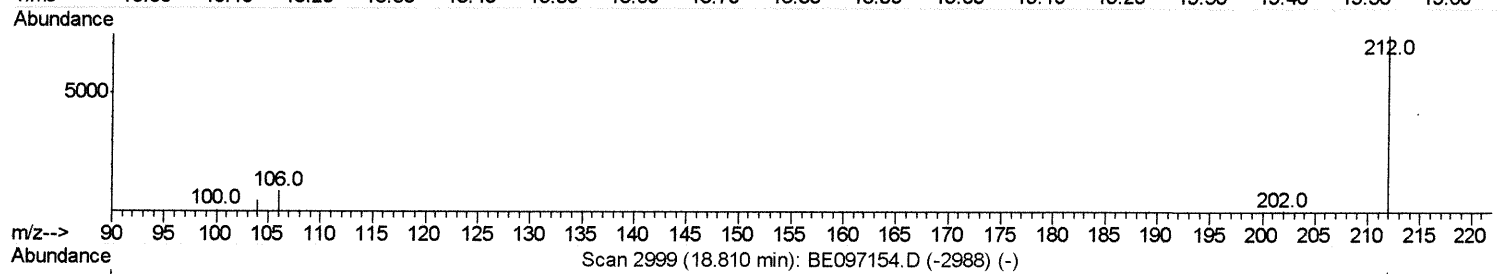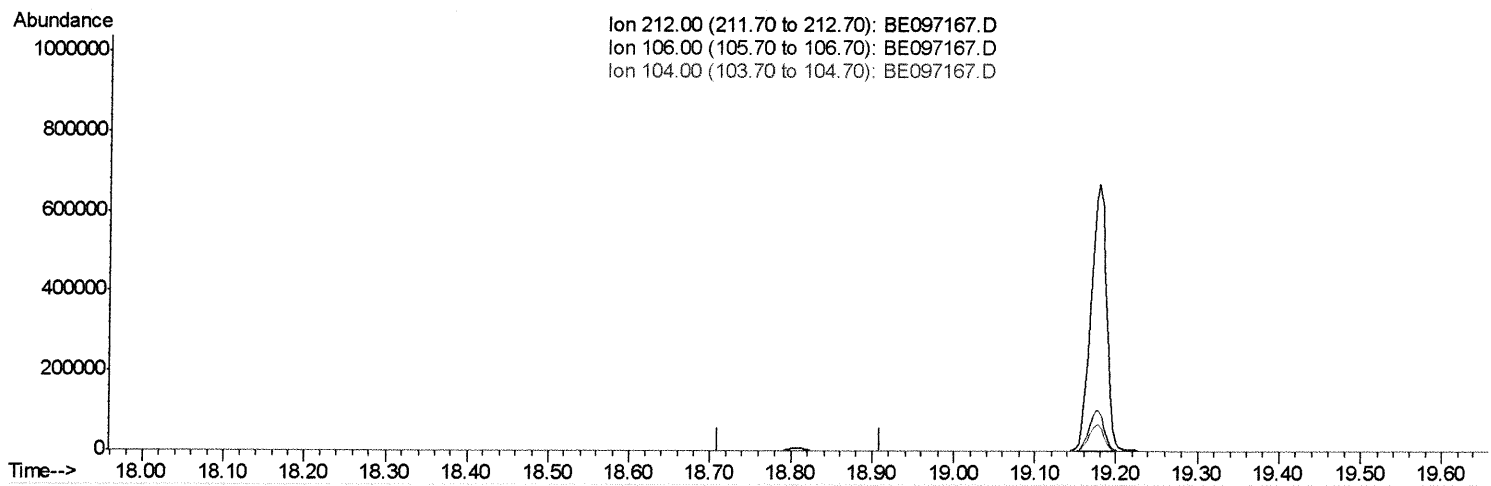

(14) Fluoranthene-d10 (SURR)

18.810min (-18.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

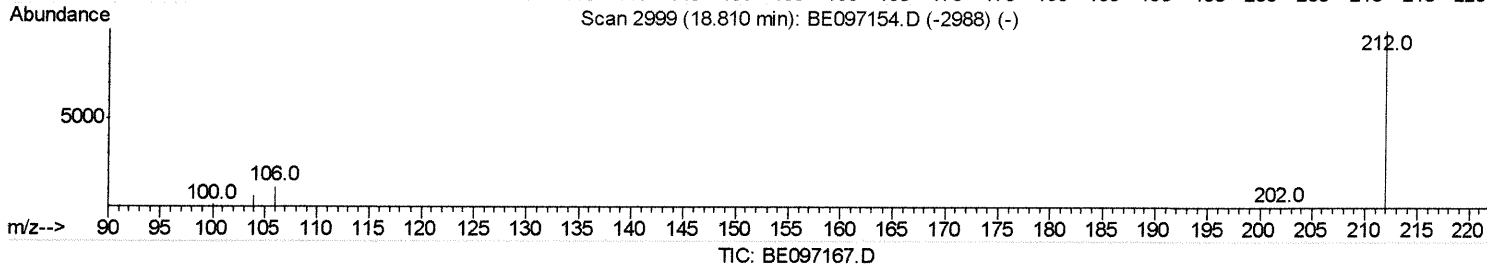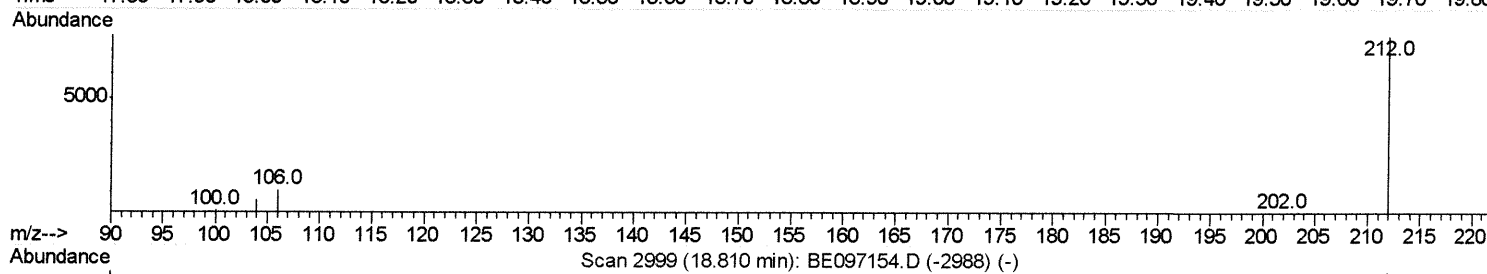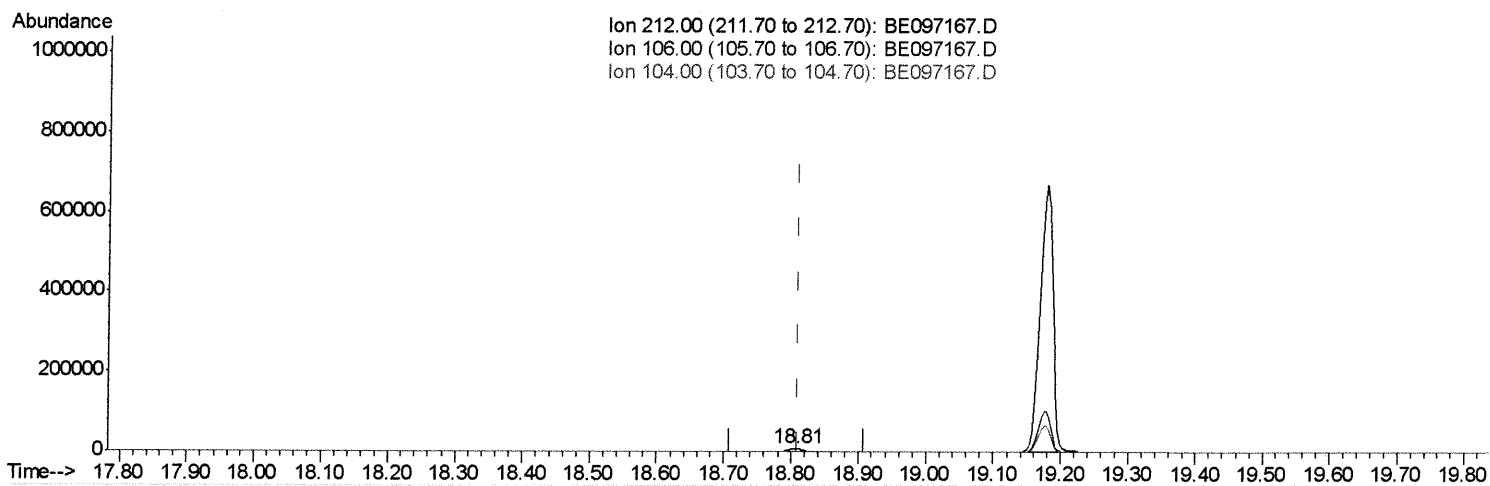

(14) Fluoranthene-d10 (SURR)

18.807min (-0.003) 0.28ng/ul m

SD 8/9/18

response 10345

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

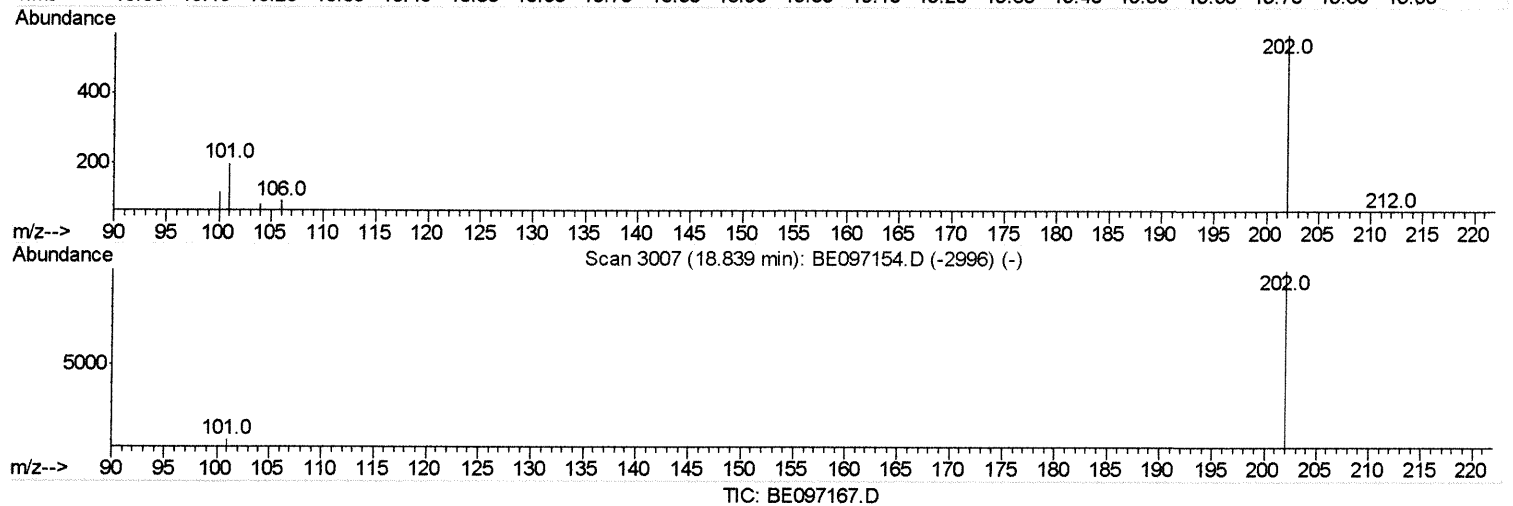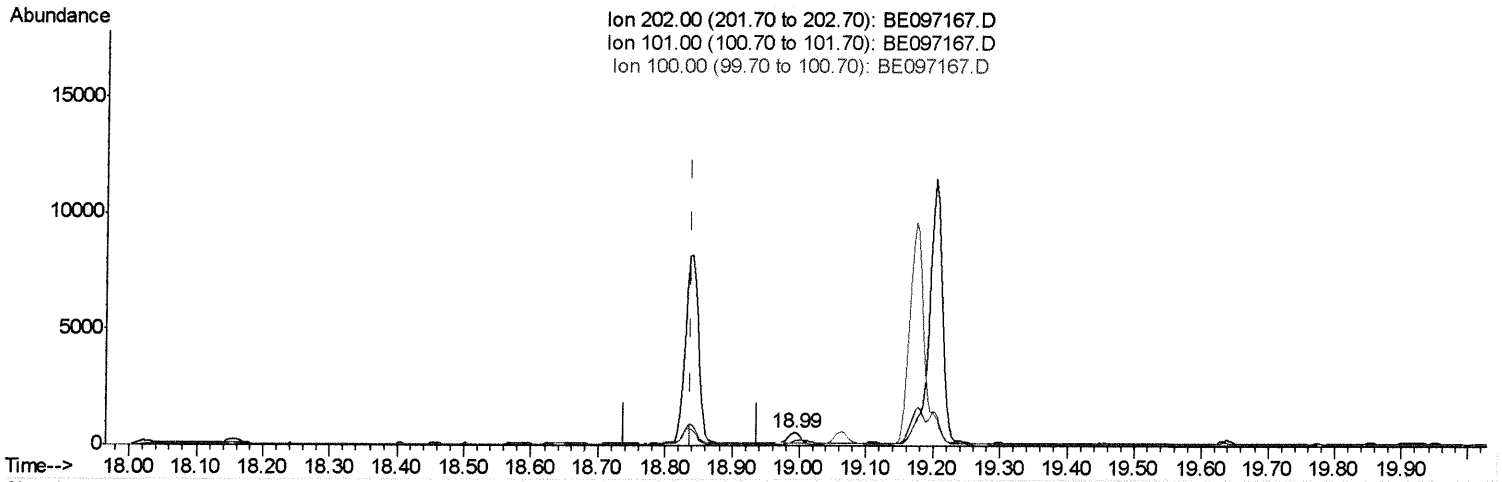

(15) Fluoranthene (C)

18.992min (+0.154) 0.02ng/ui

response 618

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	34.97#
100.00	19.50	20.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

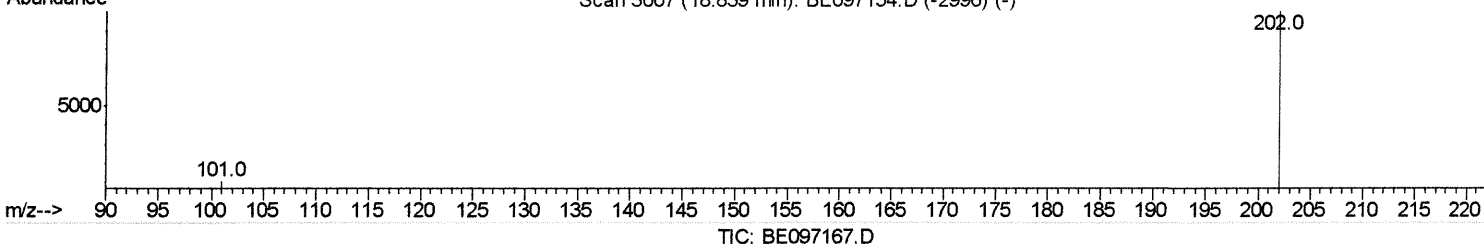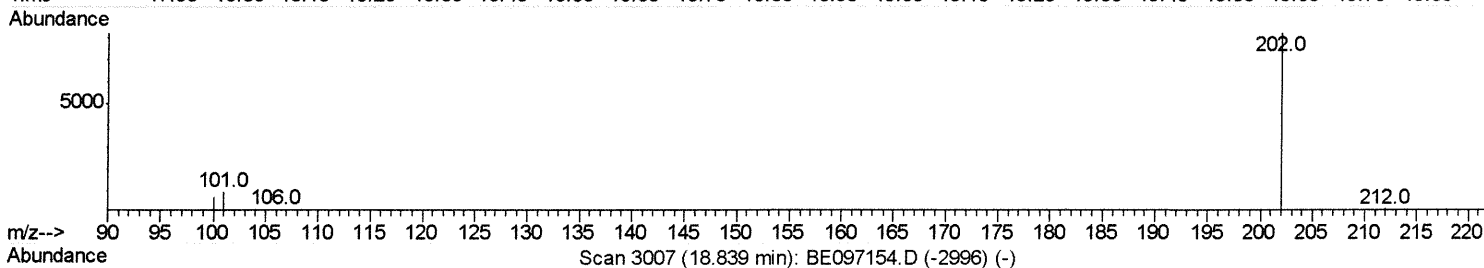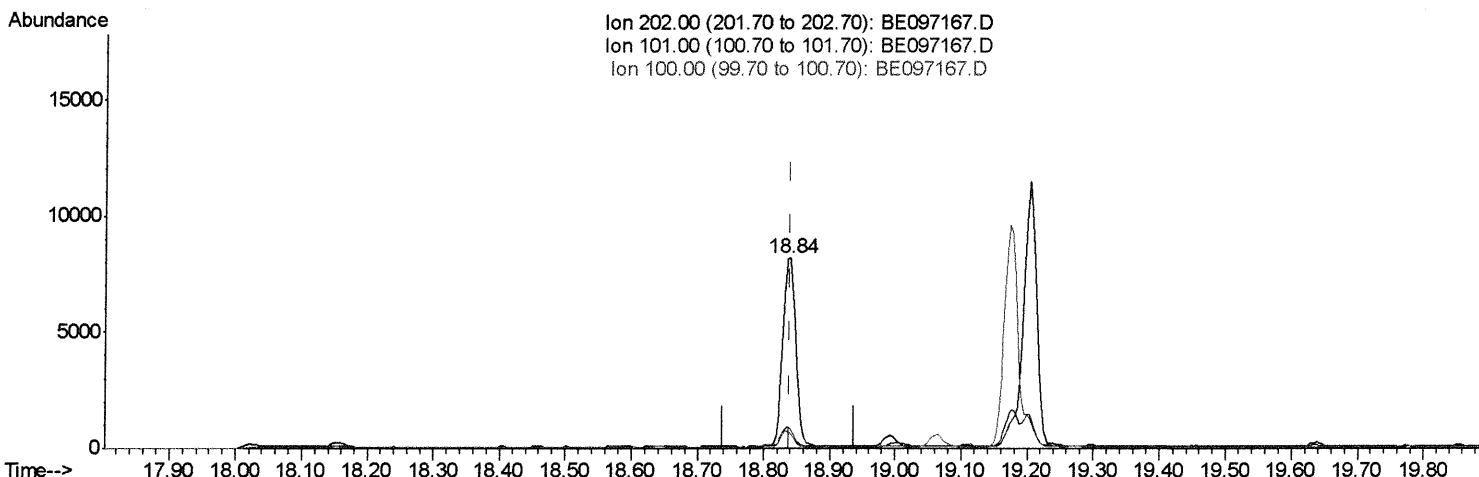

(15) Fluoranthene (C)

18.839min (+0.000) 0.31ng/ul m> SJ 8/9/18

response 11109

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.89
100.00	19.50	8.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

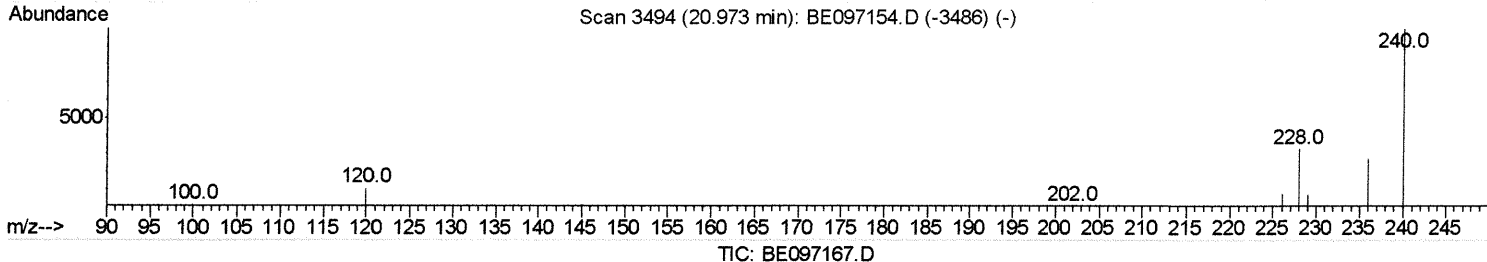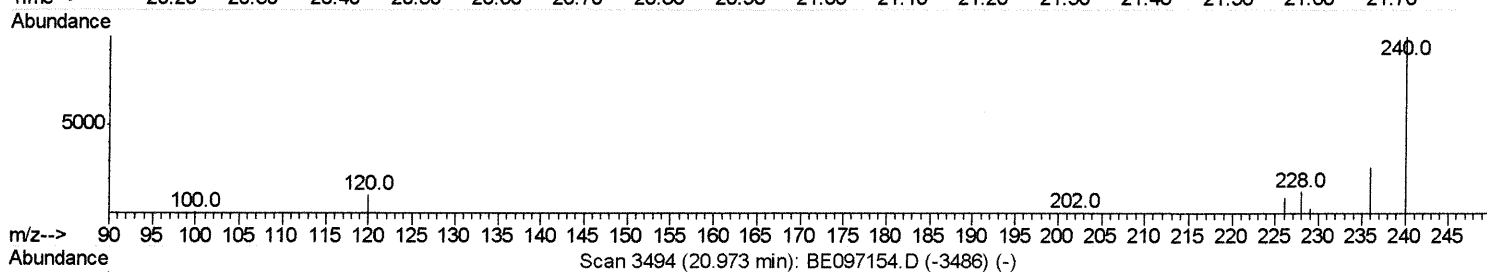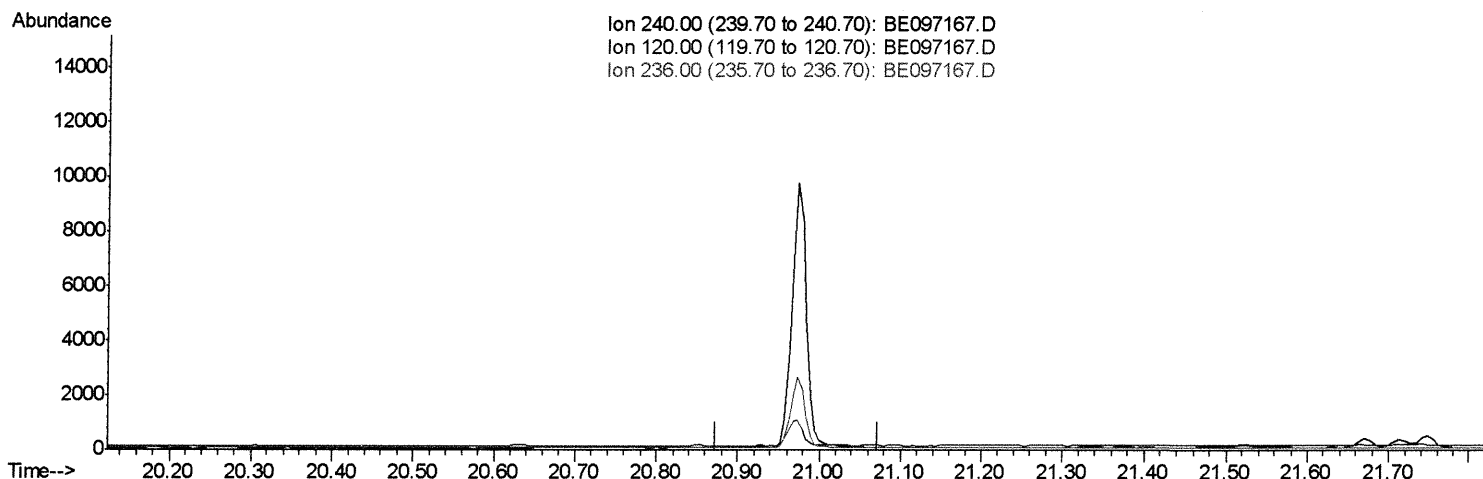

(16) Chrysene-d12 (I)

20.973min (-20.973) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:06:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

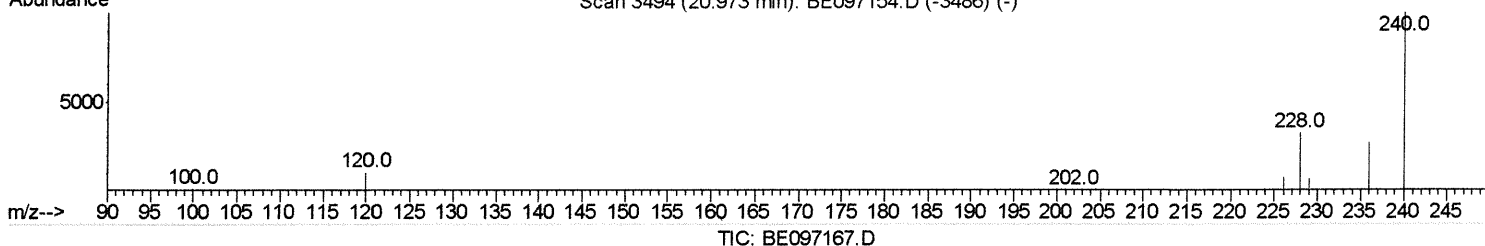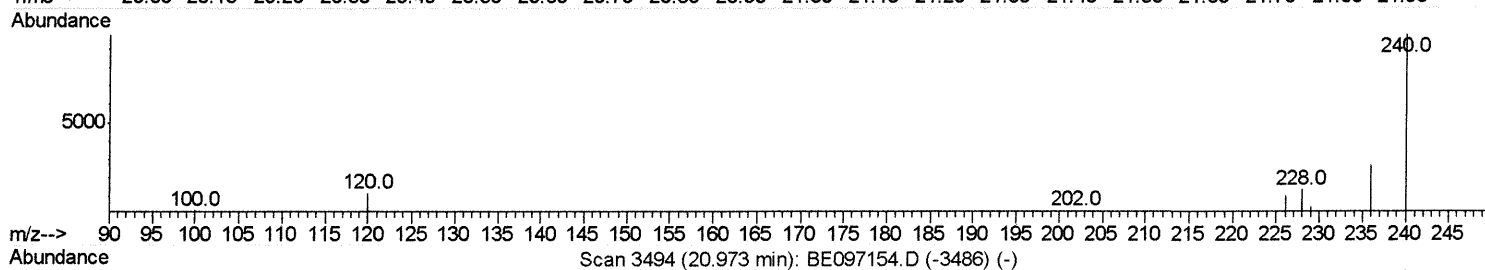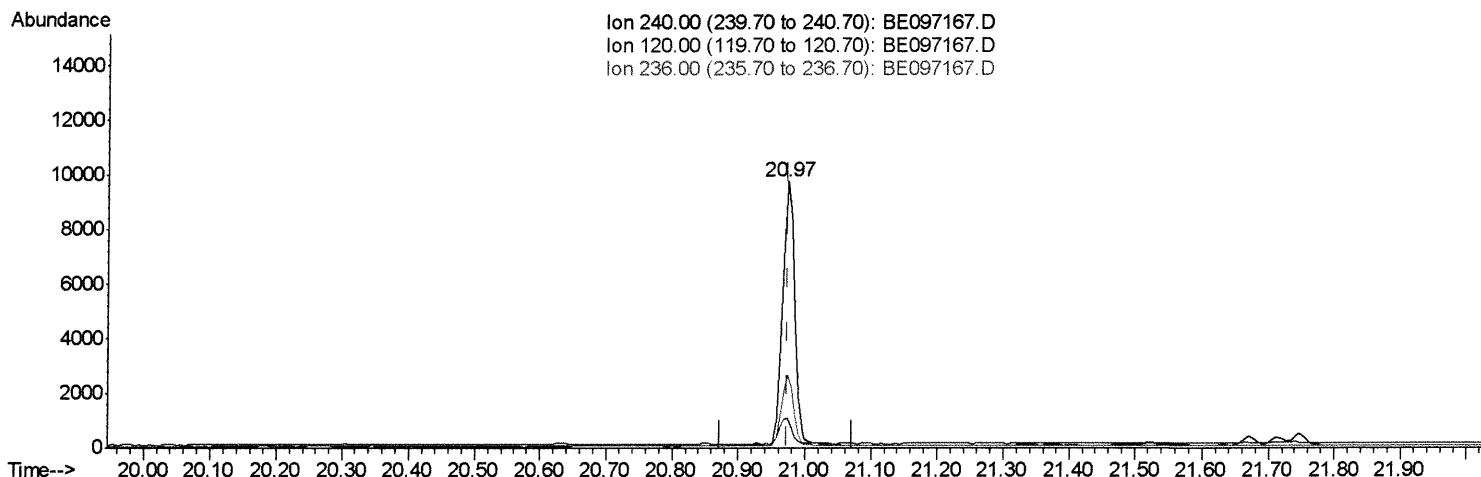

(16) Chrysene-d12 (I)

20.973min (-0.000) 0.40ng/ul m> SJ 8/9/18

response 11931

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.30#
236.00	34.90	27.40#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:08:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

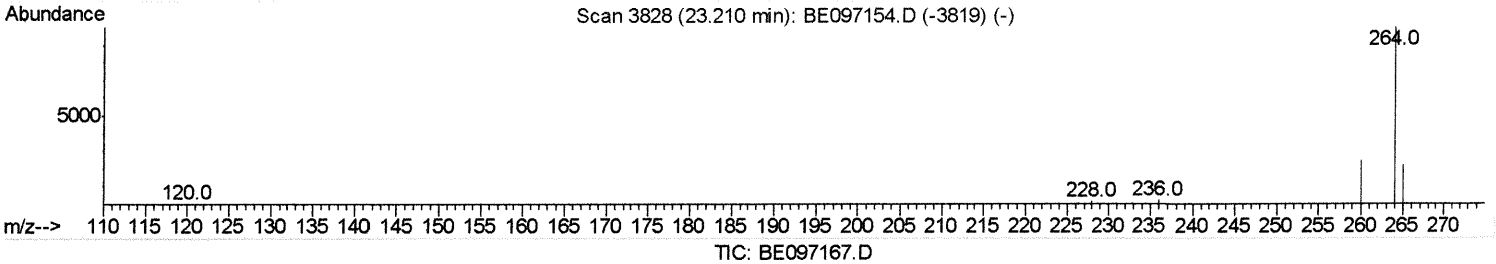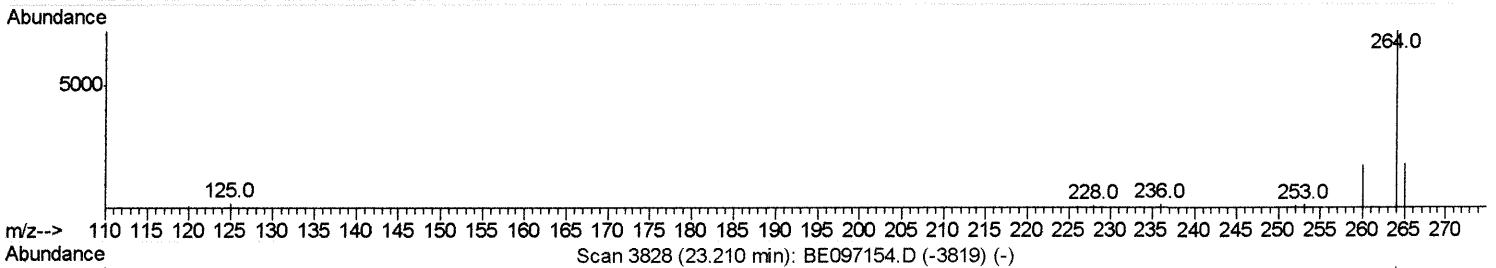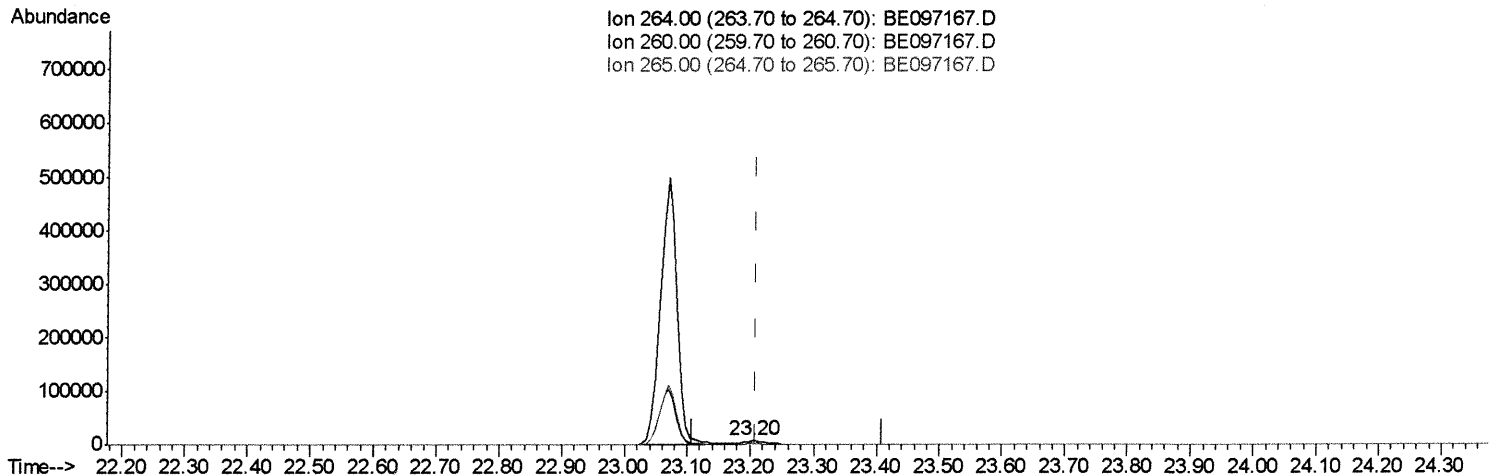

(20) Perylene-d12 (I)

23.203min (-0.007) 0.40ng/ul

response 16737

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.79
265.00	103.50	25.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:08:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

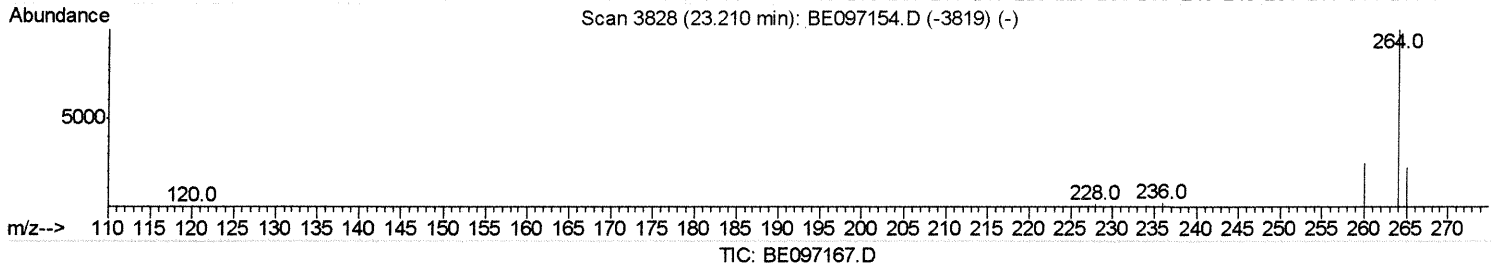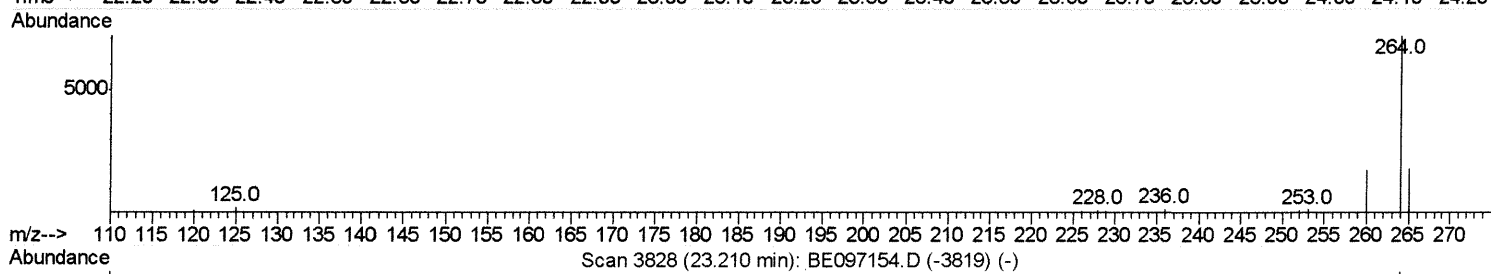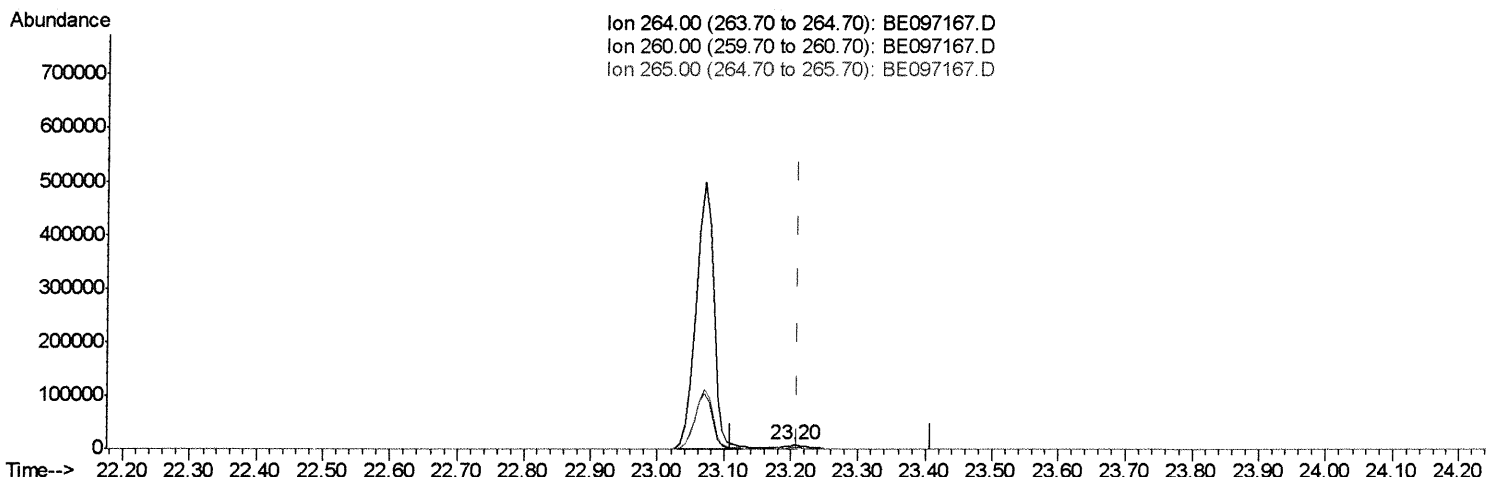

(20) Perylene-d12 (I)

23.203min (-0.007) 0.40ng/ul m> 50 8/9/18

response 10921

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.79
265.00	103.50	25.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:08:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

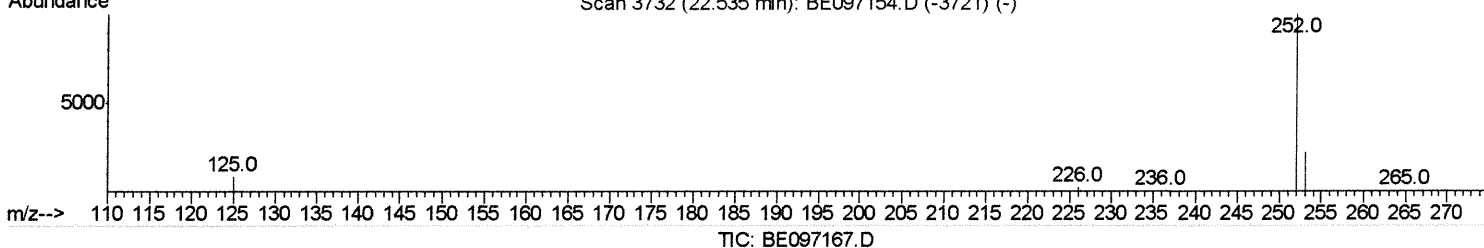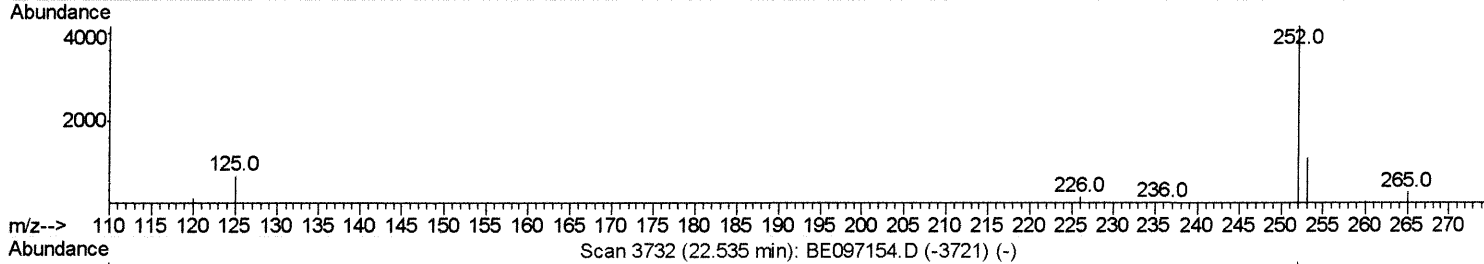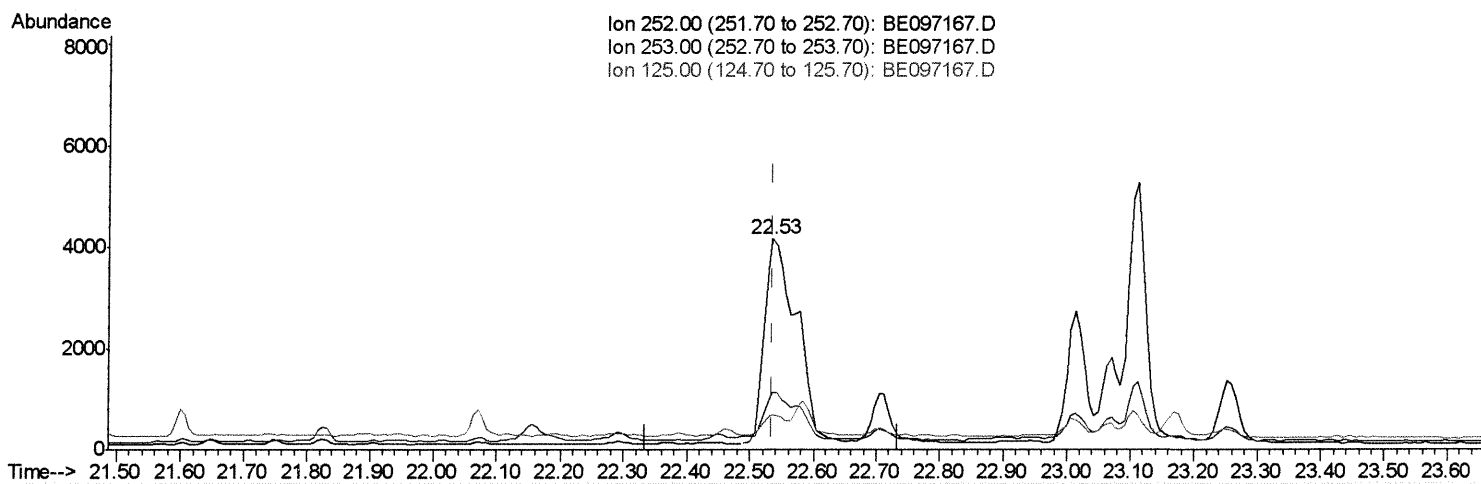

(21) Benzo(b)fluoranthene
 22.535min (+0.000) 0.48ng/ui
 response 14305

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.04
125.00	17.50	16.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:08:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

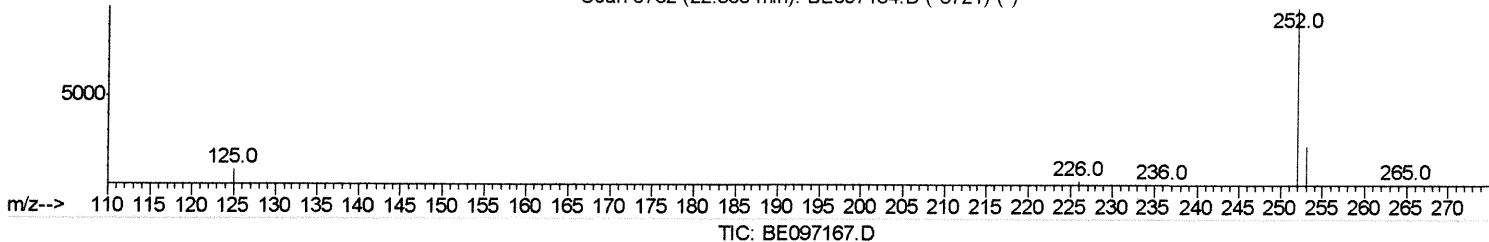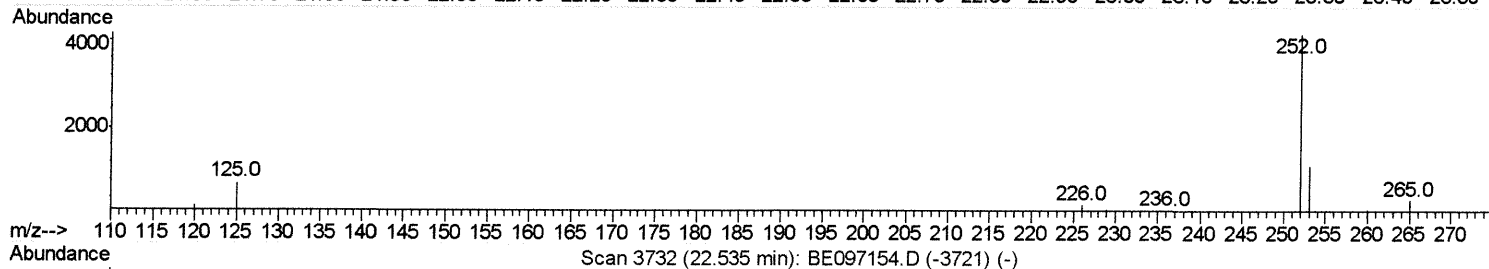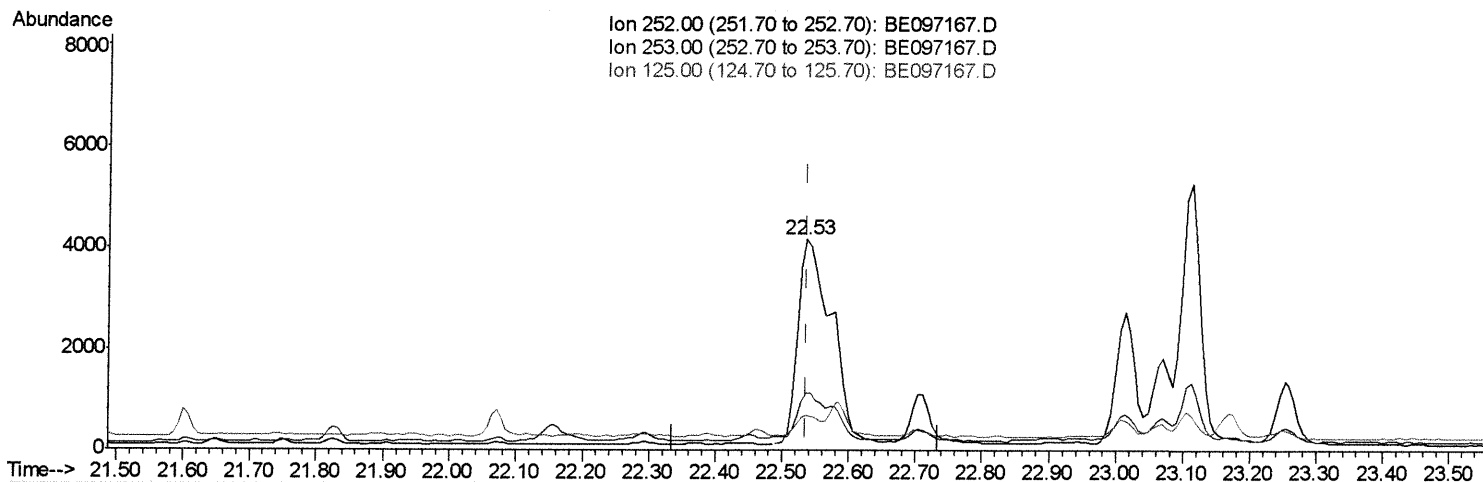

(21) Benzo(b)fluoranthene

22.535min (+0.000) 0.34ng/ul m *SD 8/9/18*

response 10106

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.04
125.00	17.50	16.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:08:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

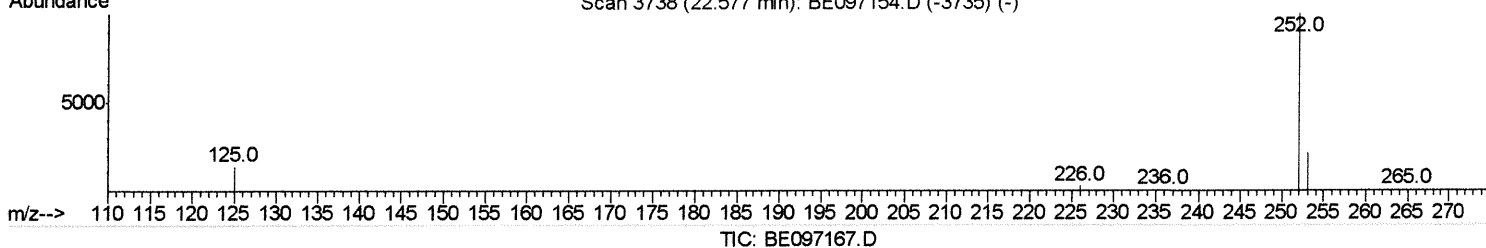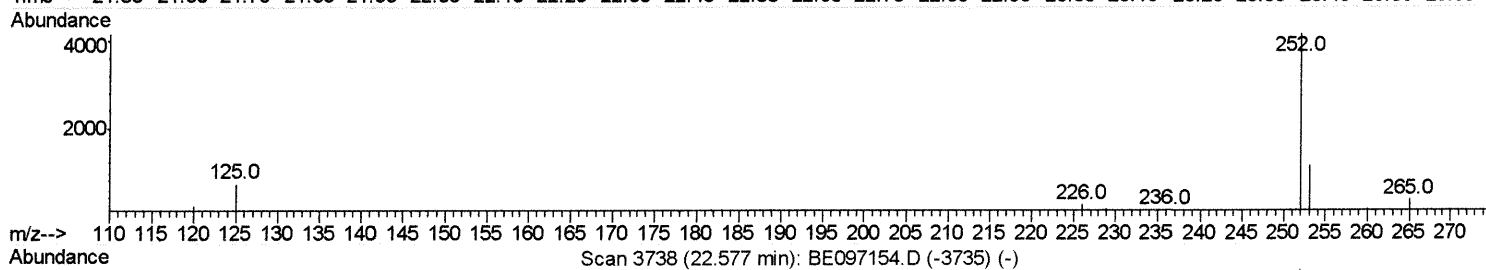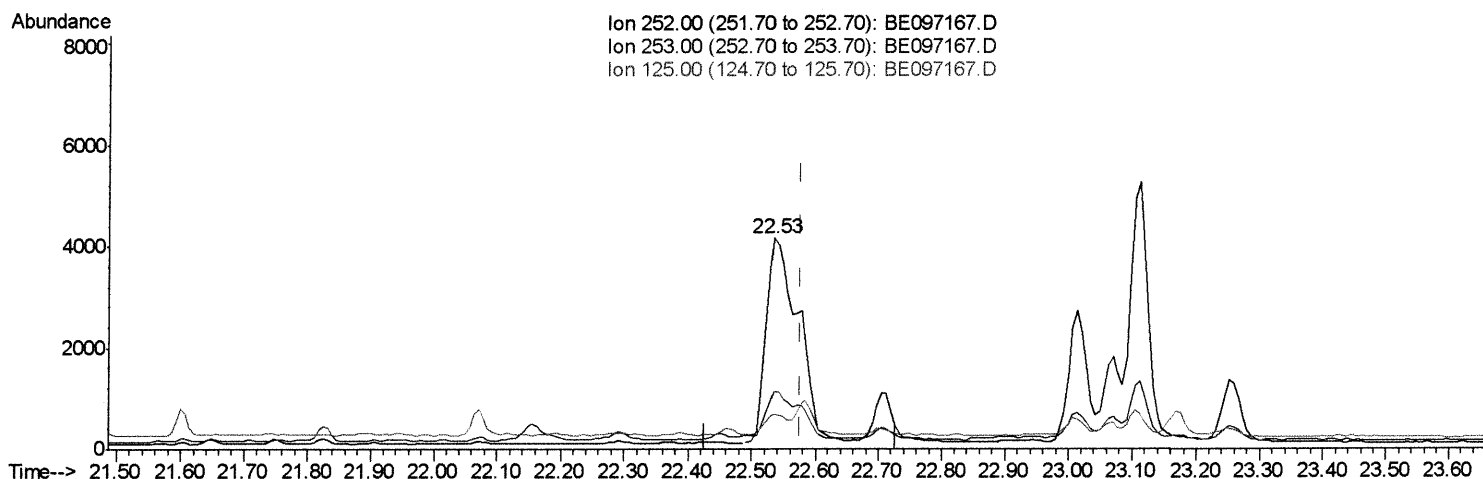

(22) Benzo(k)fluoranthene
 22.535min (-0.042) 0.45ng/ul
 response 14305

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	27.04
125.00	17.10	16.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:08:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

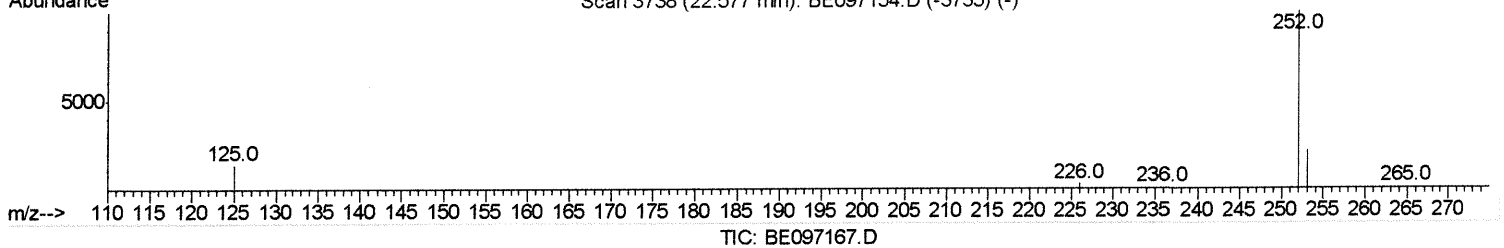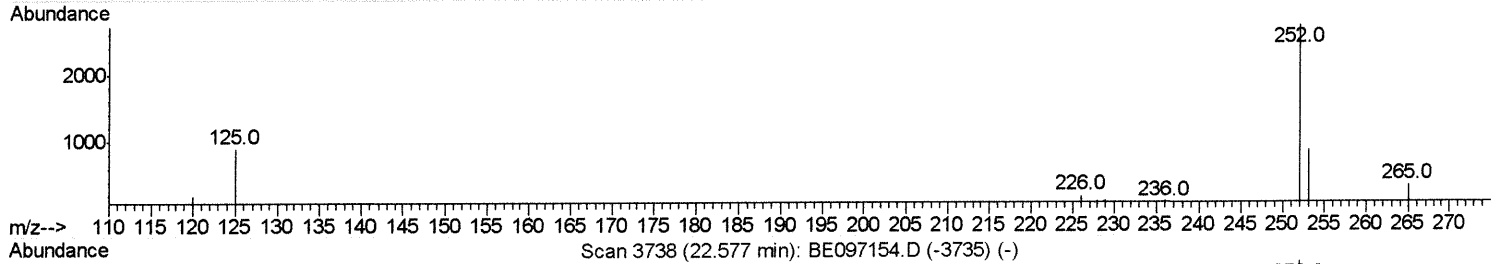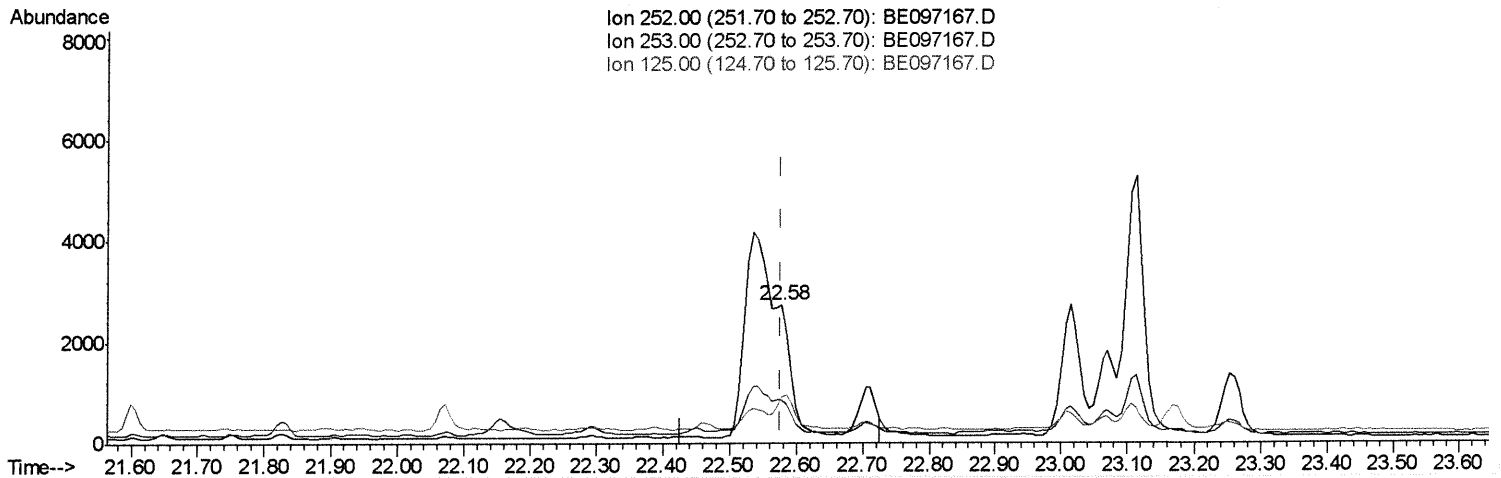

(22) Benzo(k)fluoranthene

22.577min (+0.000) 0.13ng/ul m

> 50 8/9/18

response 4182

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	31.64
125.00	17.10	33.17#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097167.D
 Acq On : 3 Aug 2018 1:08
 Operator : SJ/JU
 Sample : J4171-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K6

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:18 PM

Quant Time: Aug 03 04:10:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1284	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6577	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4216	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	10758m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	11931m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	10921m	0.40	ng/ul	0.00

SJ 8/9/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.73	152	2817	0.27	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	10345m	0.28	ng/ul	0.00

SJ 8/9/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.18	128	373	0.023	ng/ul#	64
12) Phenanthrene	16.81	178	5965m	0.218	ng/ul	
13) Anthracene	16.90	178	959m	0.037	ng/ul	
15) Fluoranthene	18.84	202	11109m	0.306	ng/ul	
17) Pyrene	19.20	202	15863	0.496	ng/ul#	81
18) Benzo(a)anthracene	20.96	228	7026	0.206	ng/ul#	81
19) Chrysene	21.01	228	7829	0.223	ng/ul	96
21) Benzo(b)fluoranthene	22.53	252	10106m	0.340	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	4182m	0.130	ng/ul	
23) Benzo(a)pyrene	23.11	252	9600	0.322	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	25.50	276	6270	0.168	ng/ul#	72
25) Dibenzo(a,h)anthracene	25.51	278	1189	0.039	ng/ul#	75
26) Benzo(g,h,i)perylene	26.19	276	5066	0.157	ng/ul	94

SJ 8/9/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed