

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:06:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

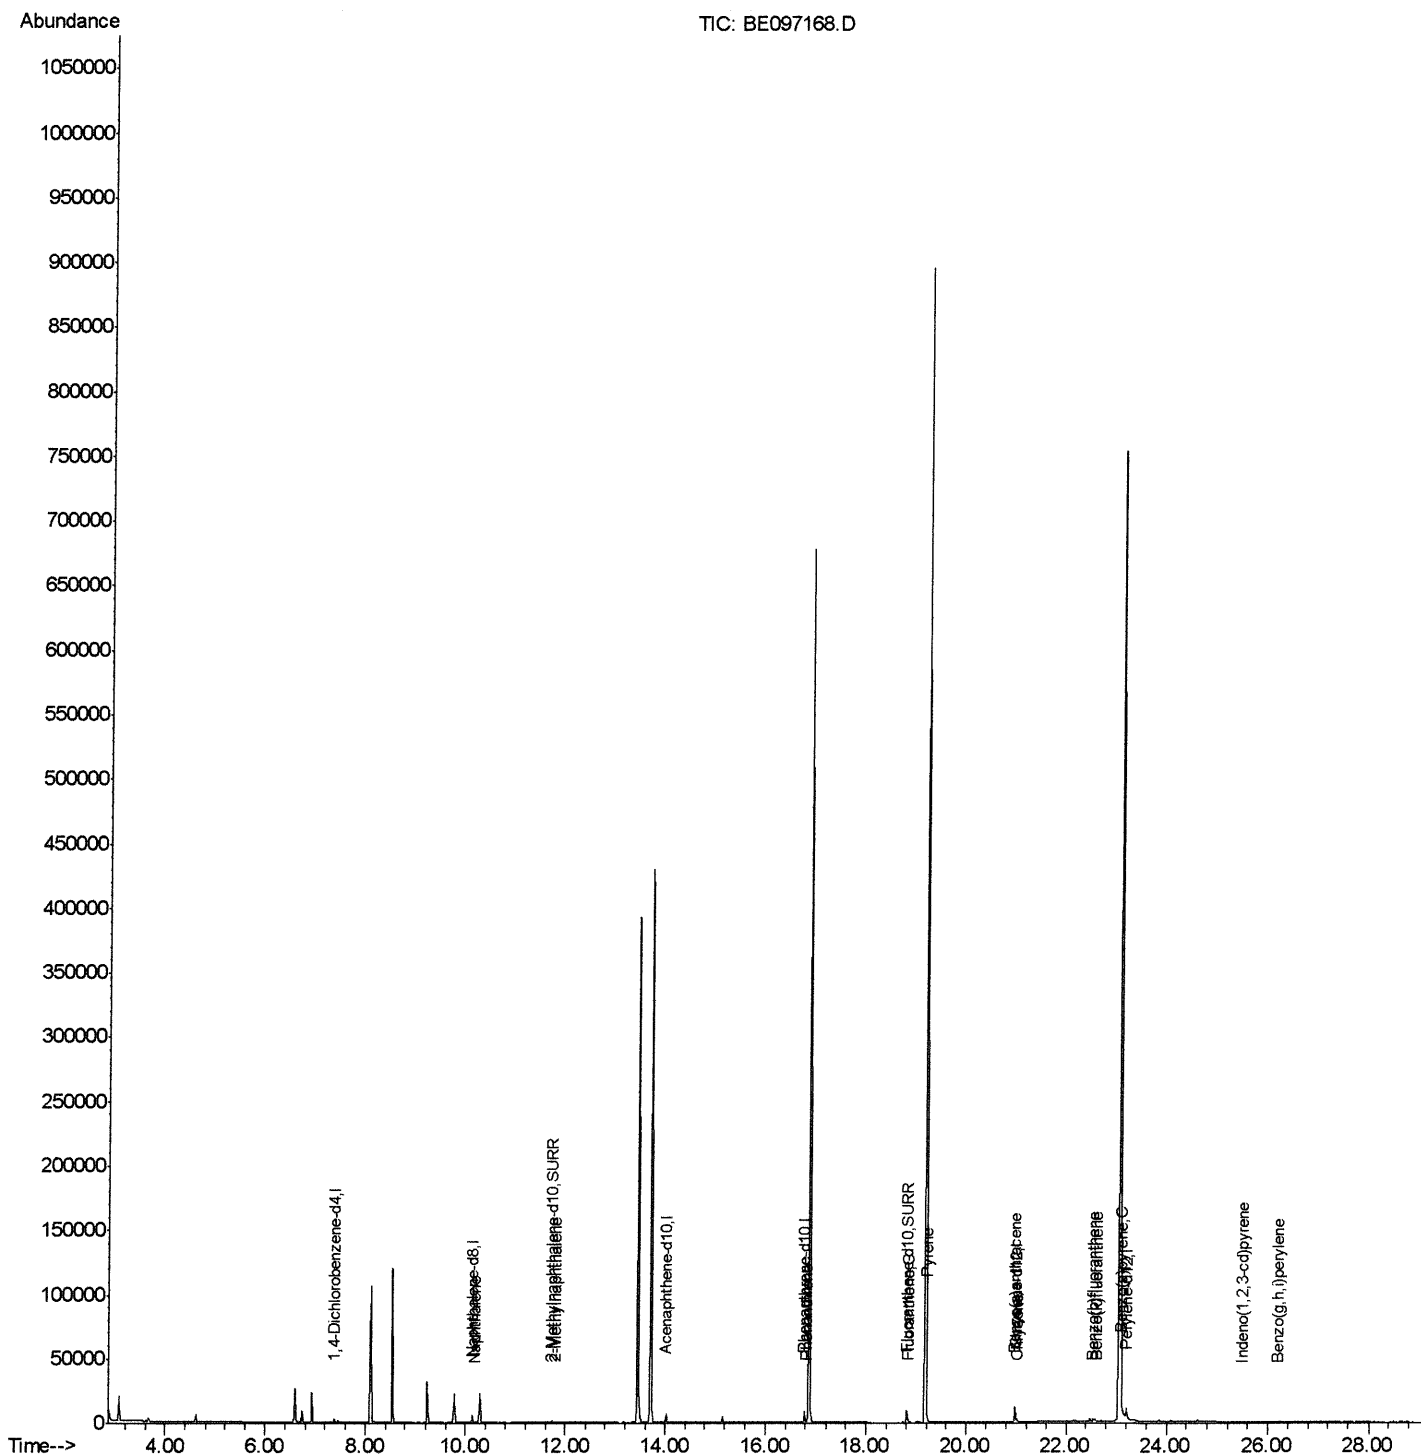

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:47:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

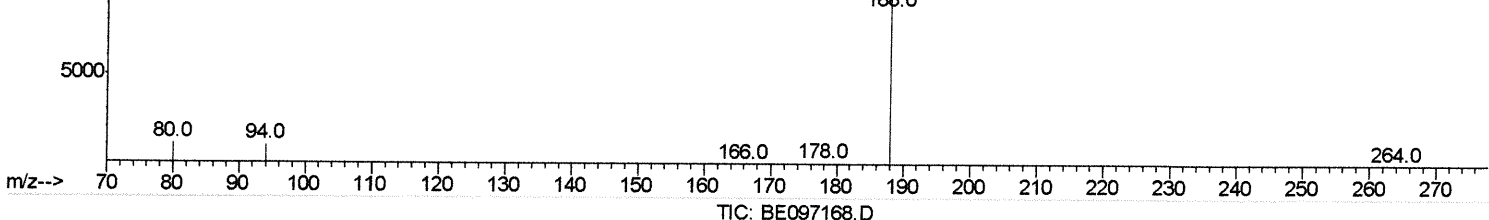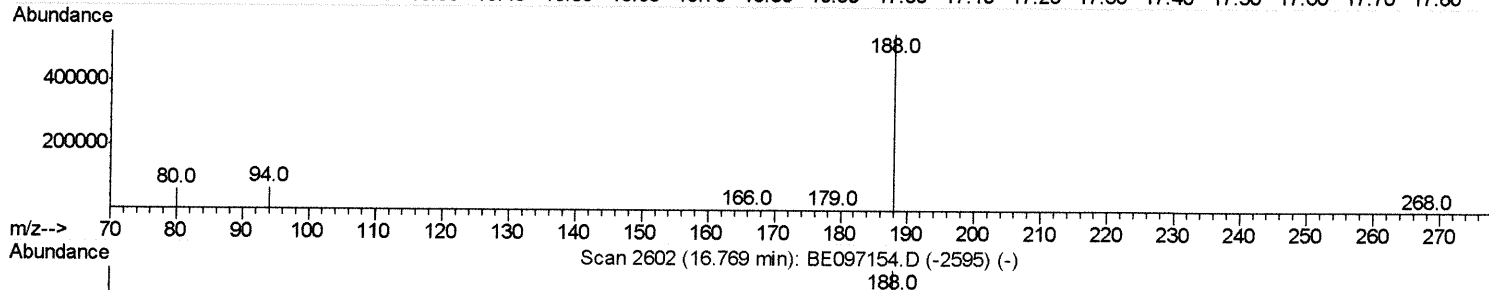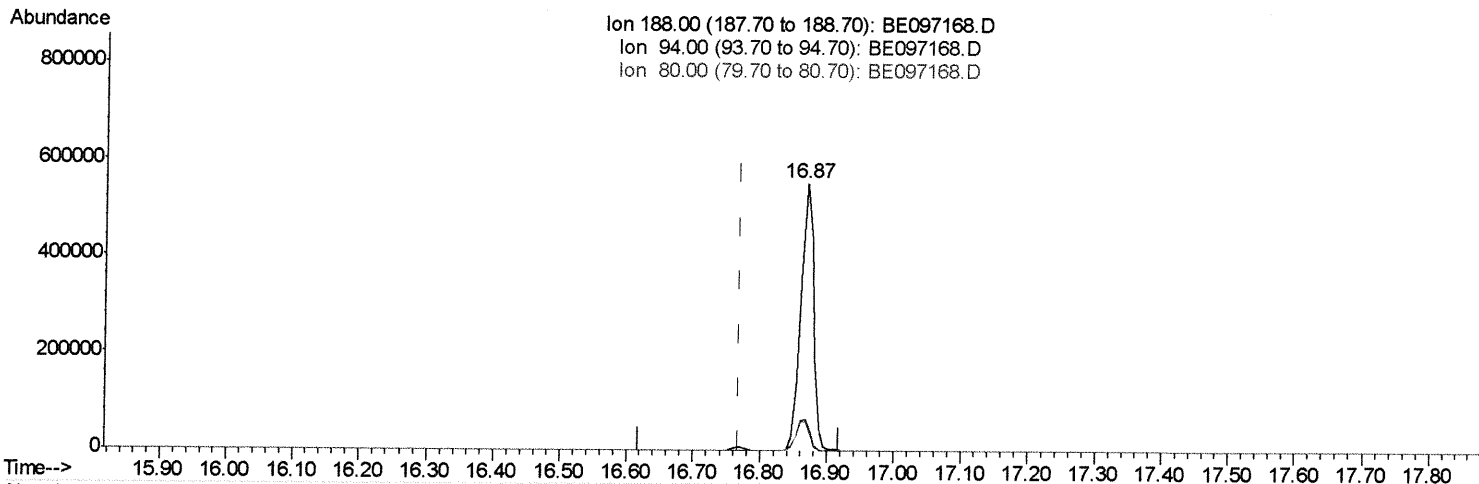

(10) Phenanthrene-d10 (I)
 16.867min (+0.098) 0.40ng/ul
 response 738914

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.91
80.00	11.80	10.83
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:47:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

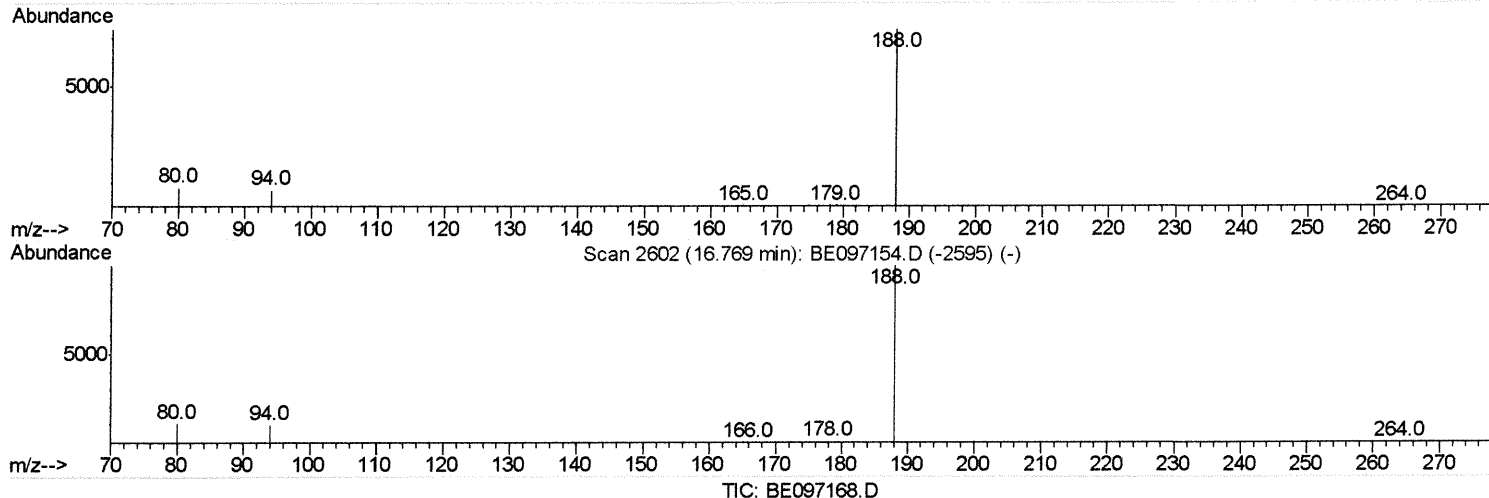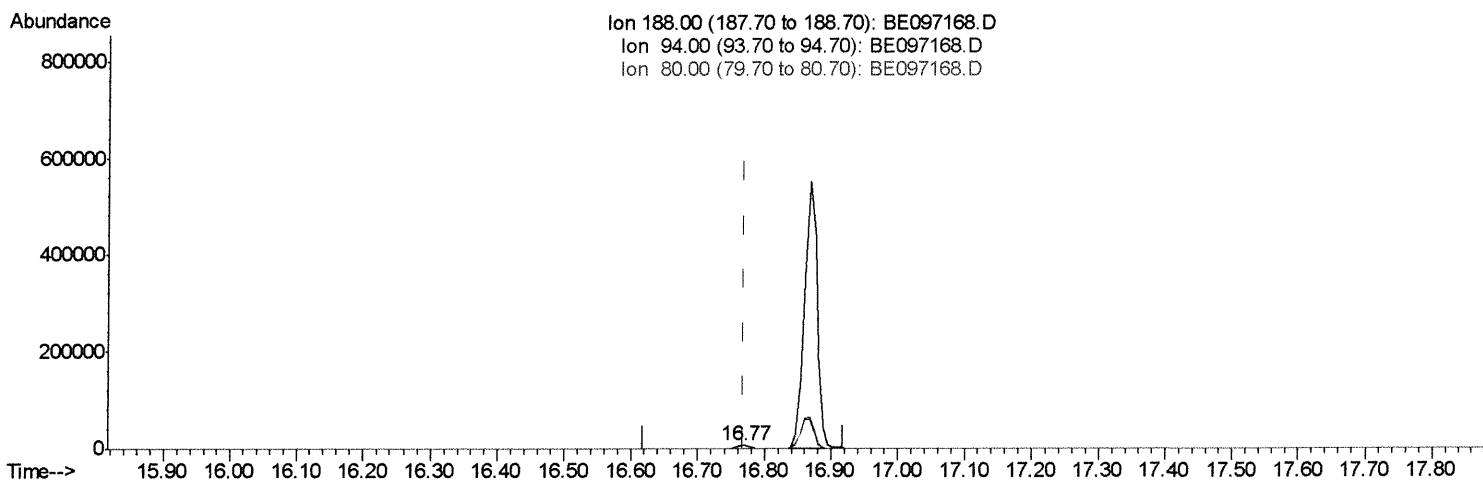

(10) Phenanthrene-d10 (I)

16.769min (-0.000) 0.40ng/ul m

> SJ 8/9/18

response 10349

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.78
80.00	11.80	10.90
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:48:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

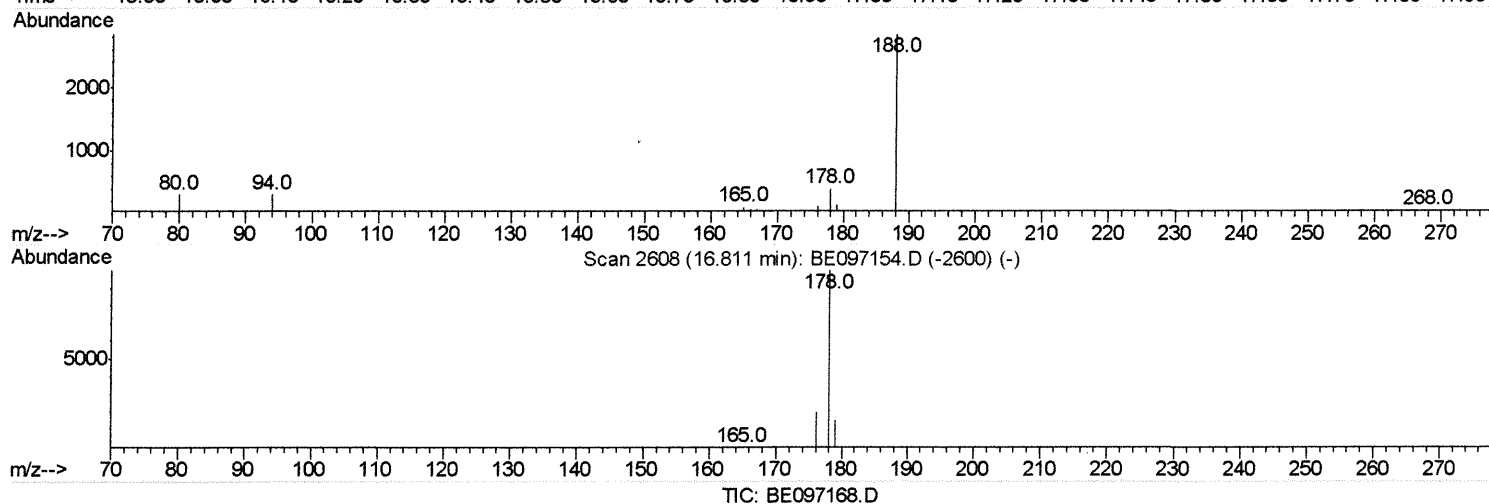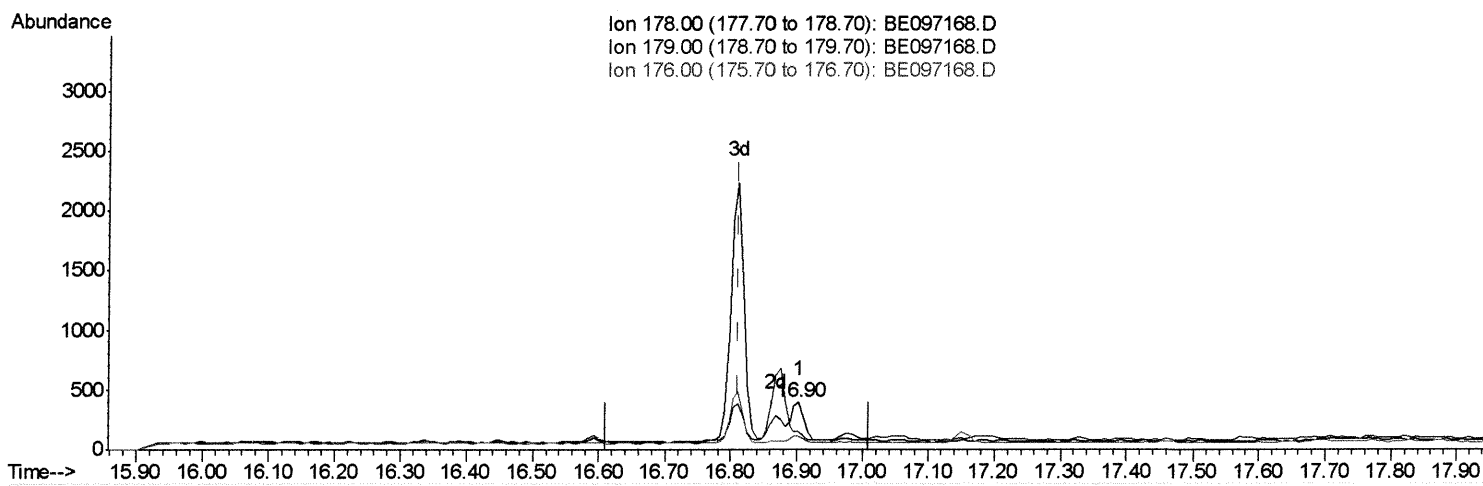

(12) Phenanthrene

16.902min (+0.091) 0.02ng/ul

response 448

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	37.47#
176.00	17.00	29.62#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:48:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

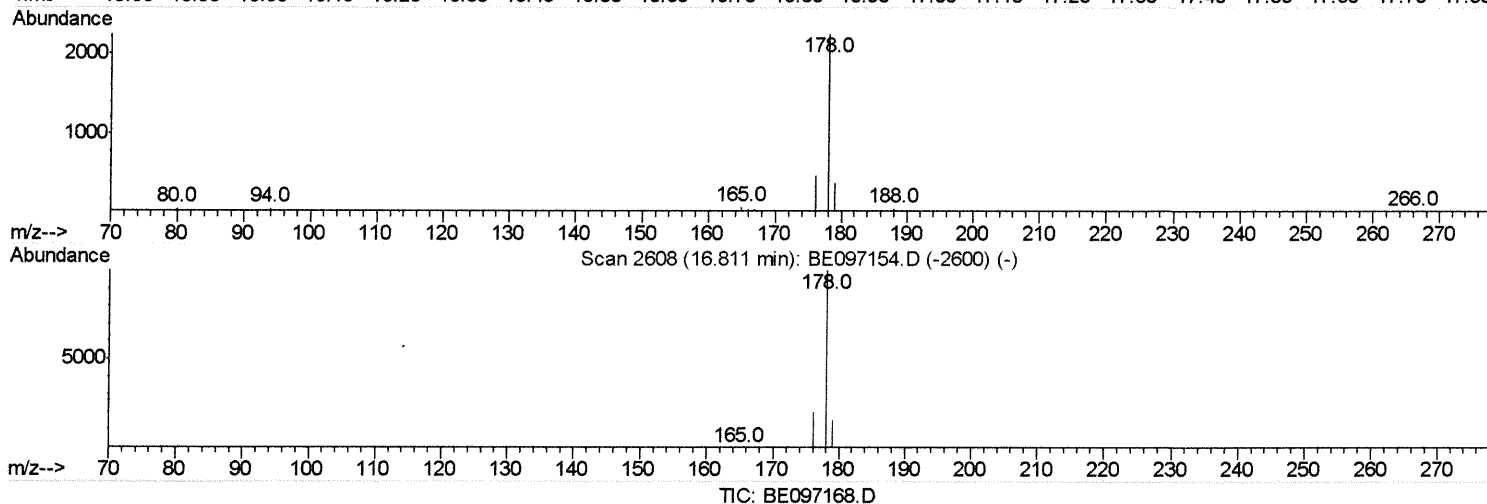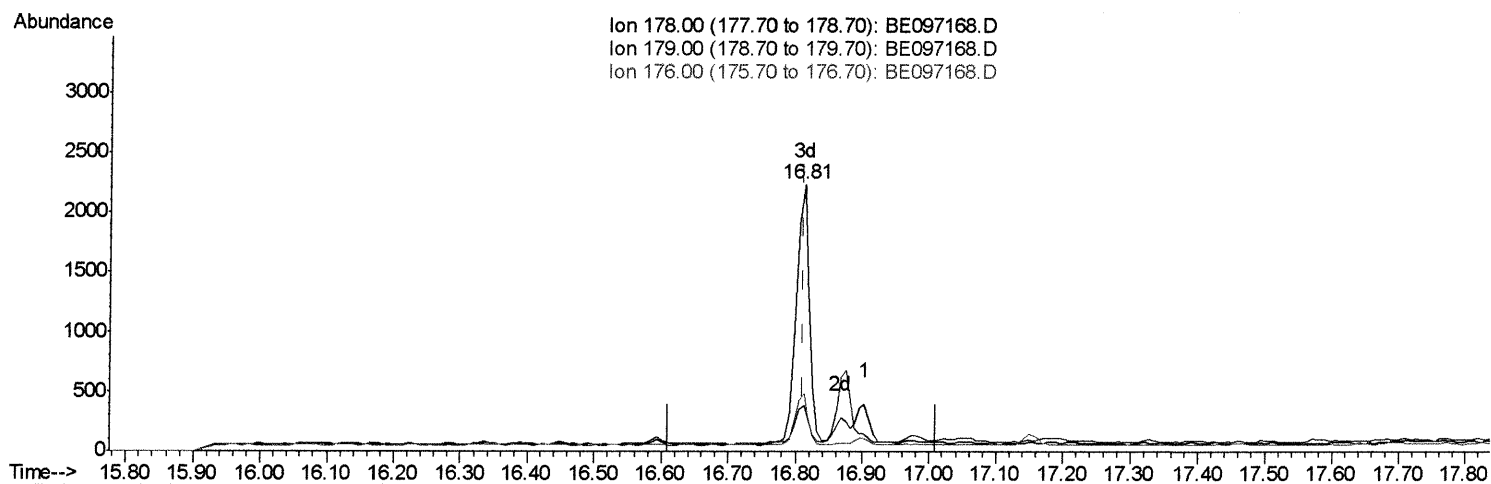

(12) Phenanthrene

16.811min (-0.000) 0.11ng/ul m > SJ 8/9/18

response 2951

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	17.45#
176.00	17.00	21.61#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

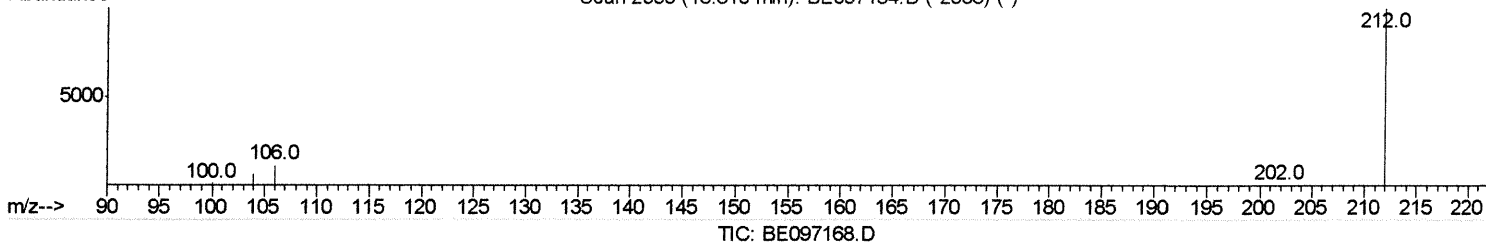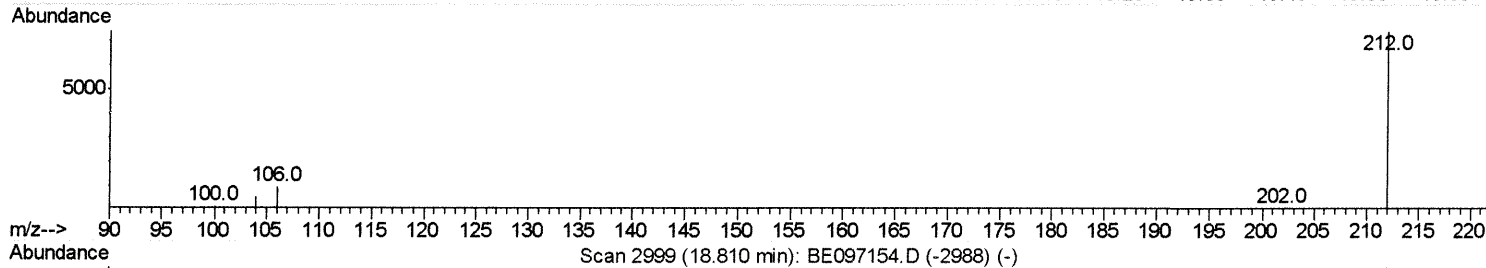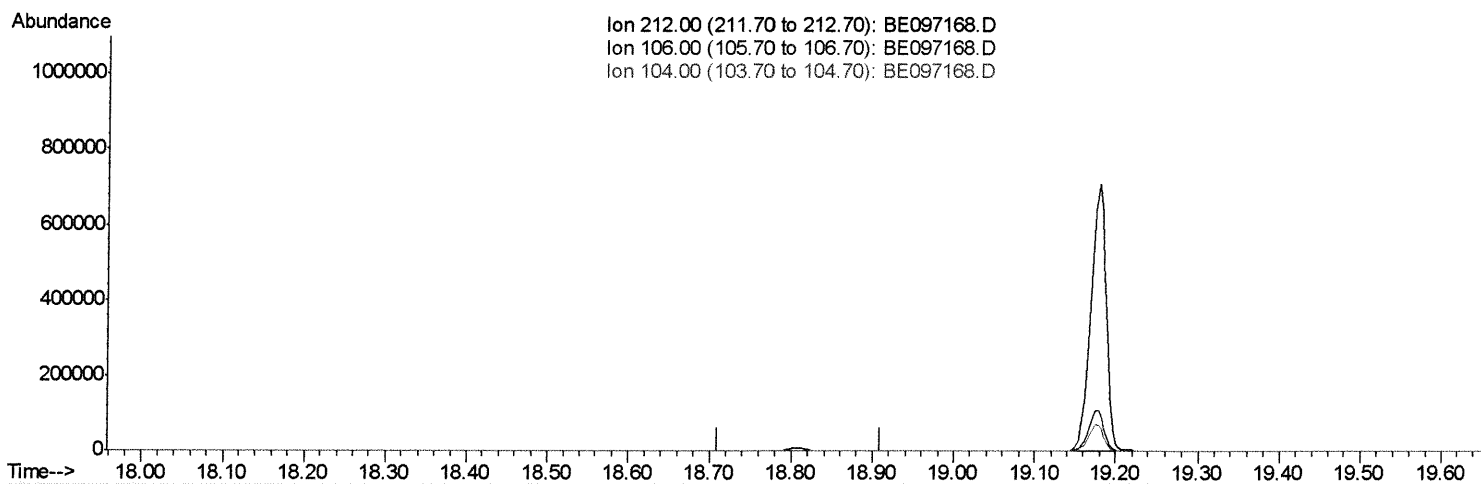

(14) Fluoranthene-d10 (SURR)

18.810min (-18.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

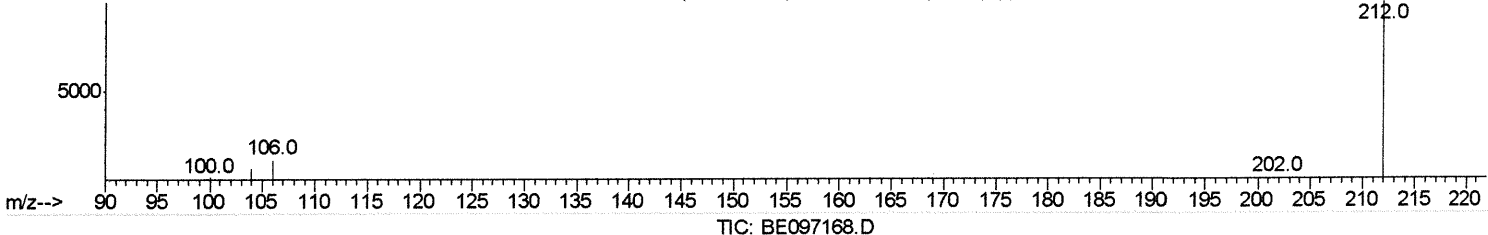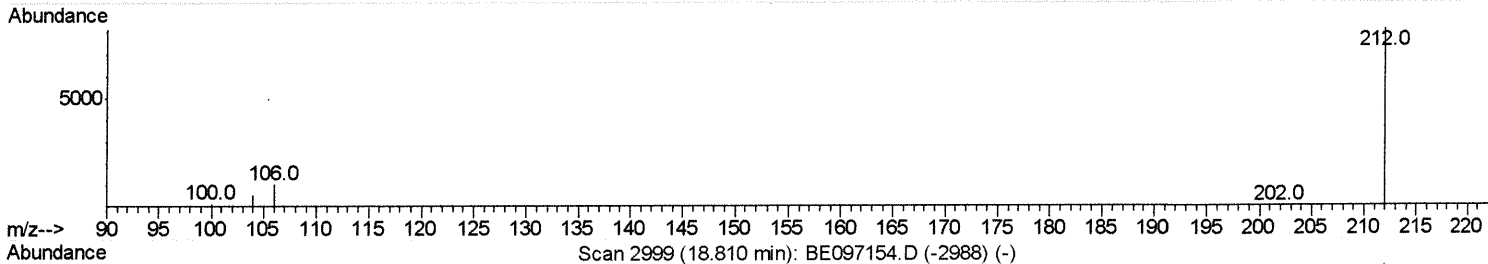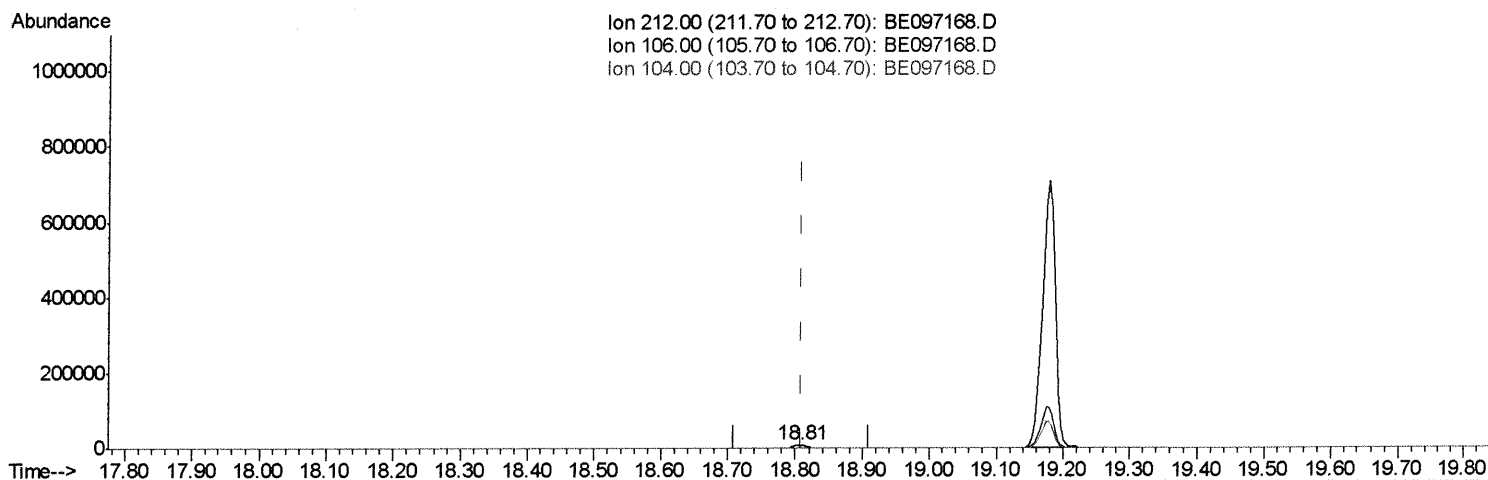

(14) Fluoranthene-d10 (SURR)

18.807min (-0.003) 0.31ng/ul m > SJ 8/9/18

response 10907

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

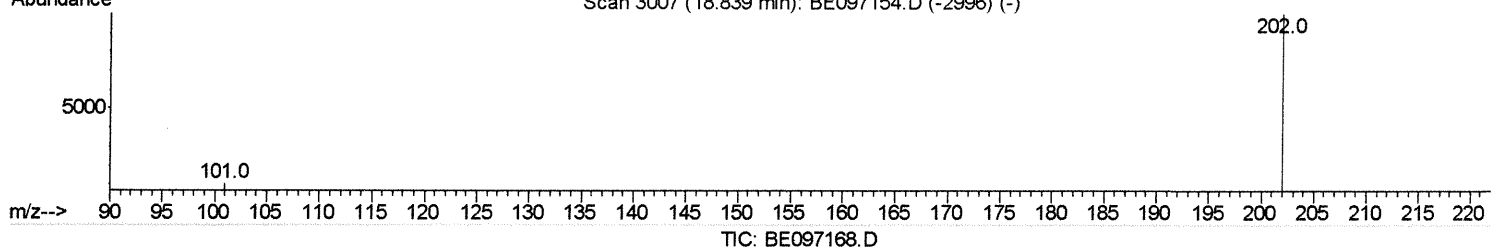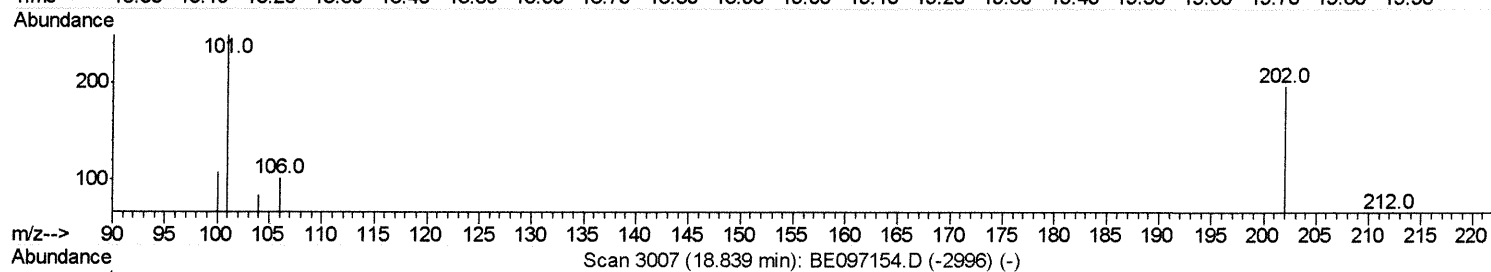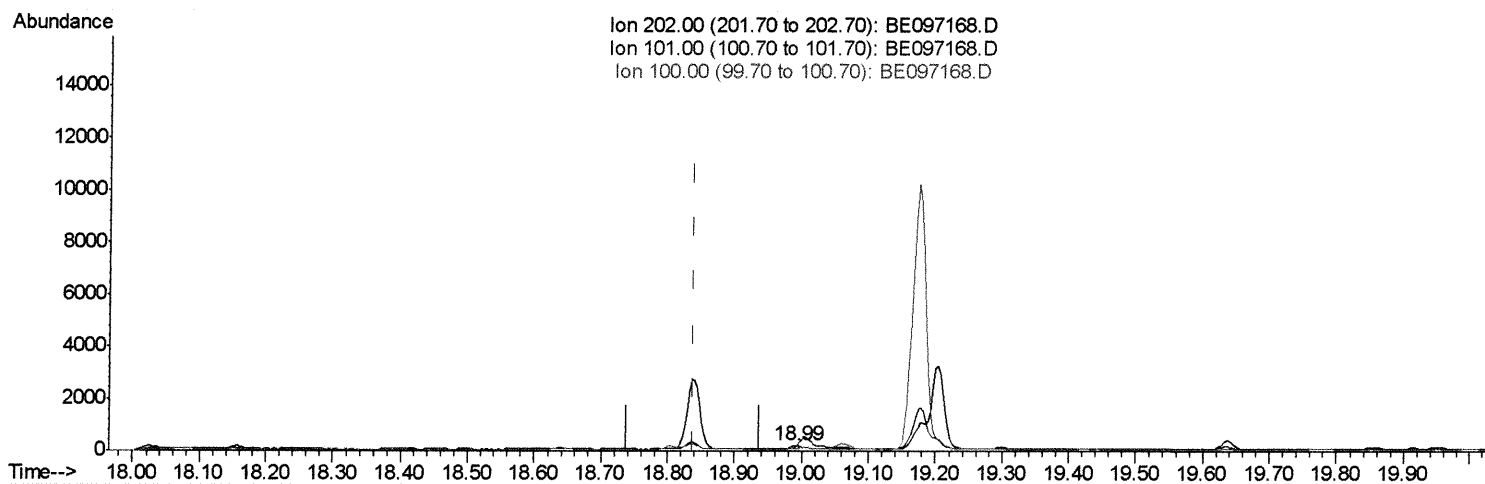

(15) Fluoranthene (C)

18.993min (+0.154) 0.00ng/ul

response 147

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	127.04#
100.00	19.50	55.10#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

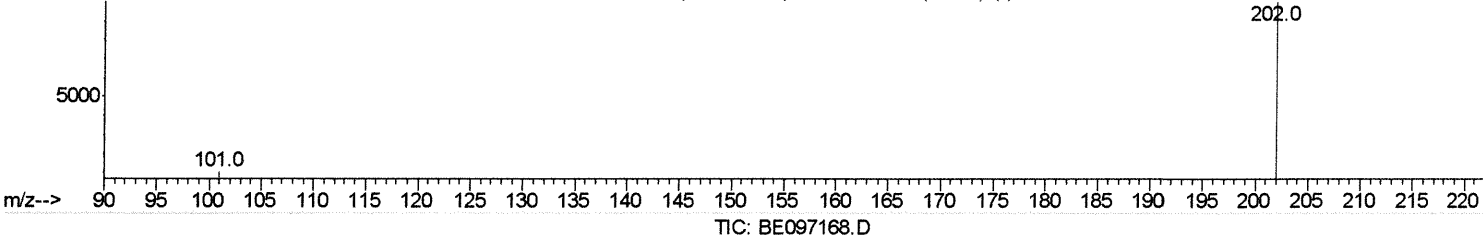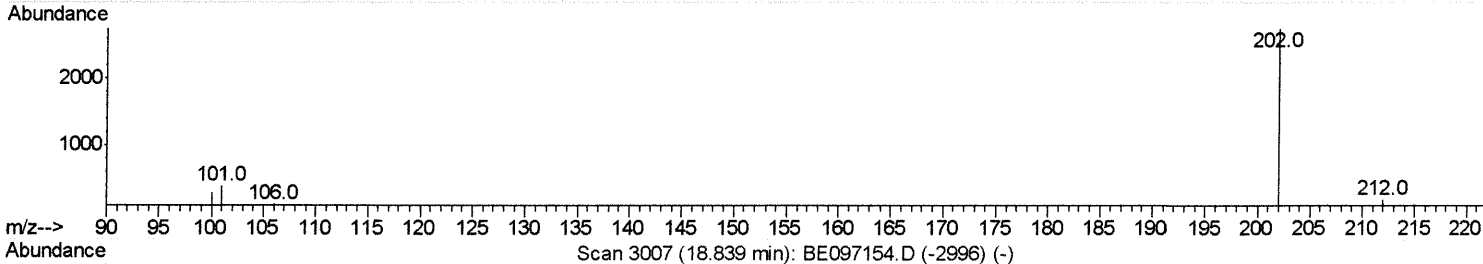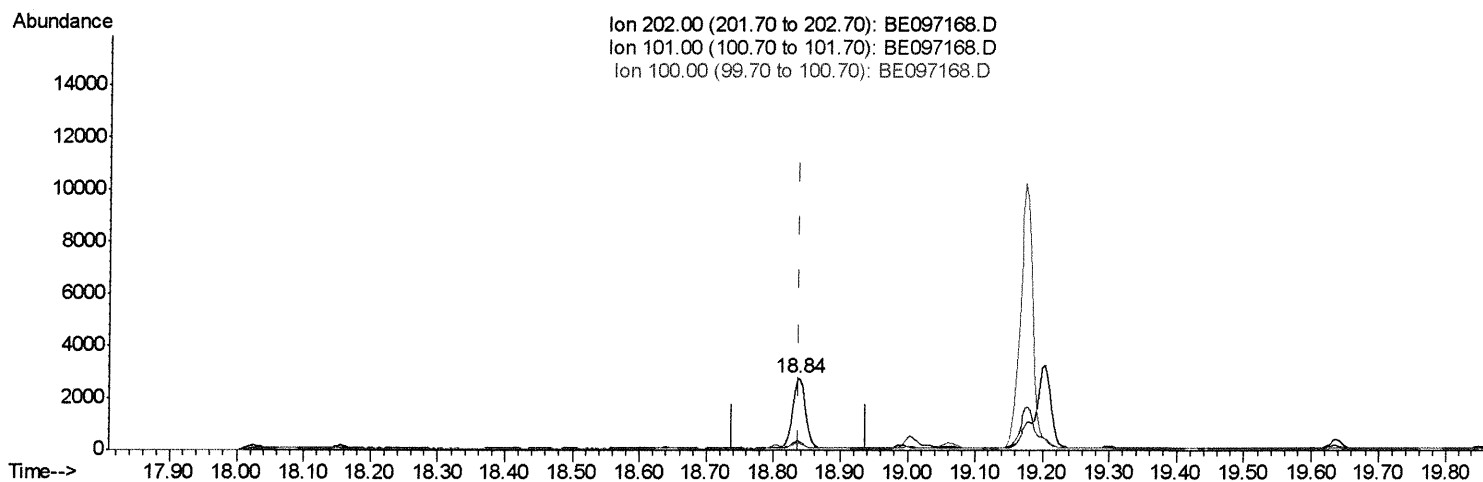

(15) Fluoranthene (C)

18.836min (-0.003) 0.10ng/ul m > 50 8/9/18

response 3581

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	13.33
100.00	19.50	10.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

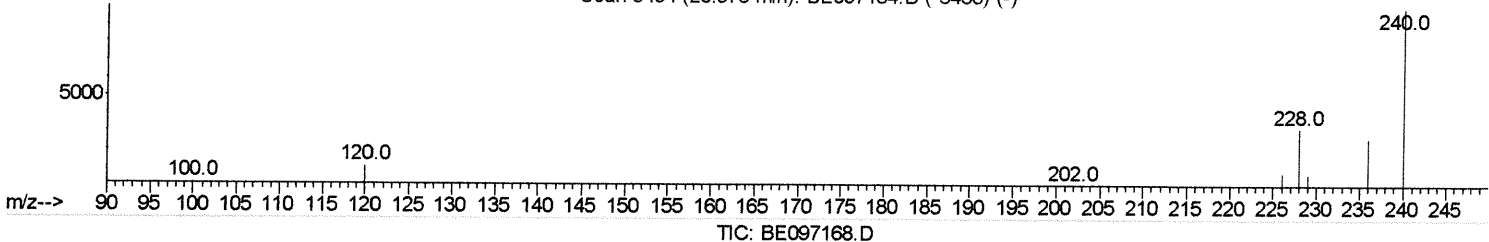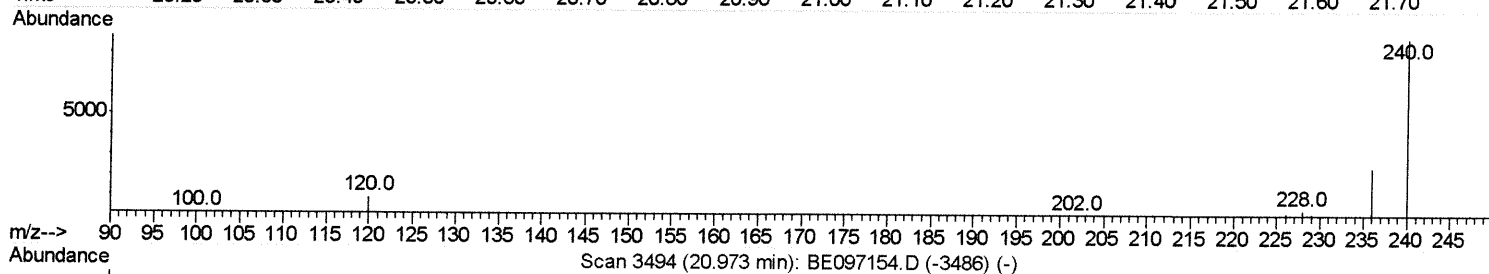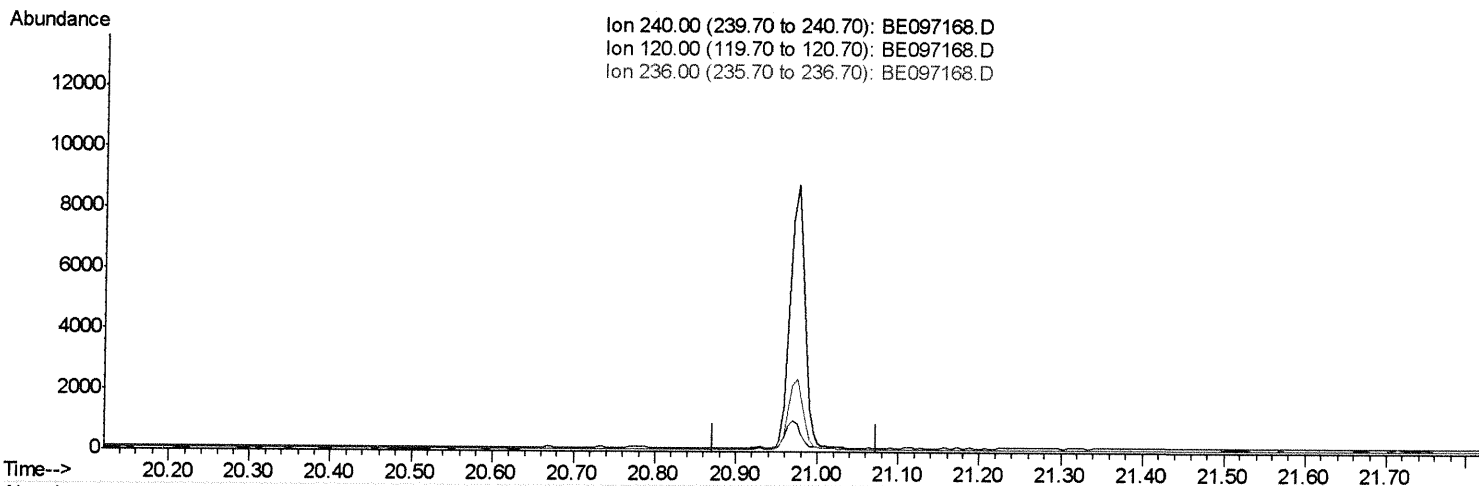

(16) Chrysene-d12 (I)

20.973min (-20.973) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

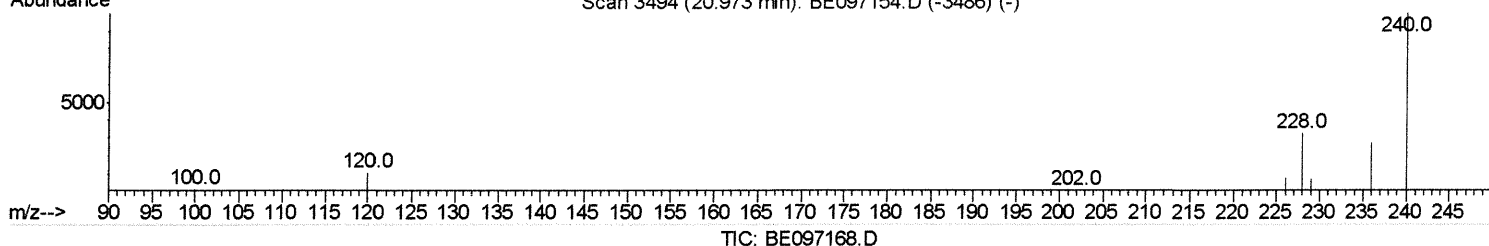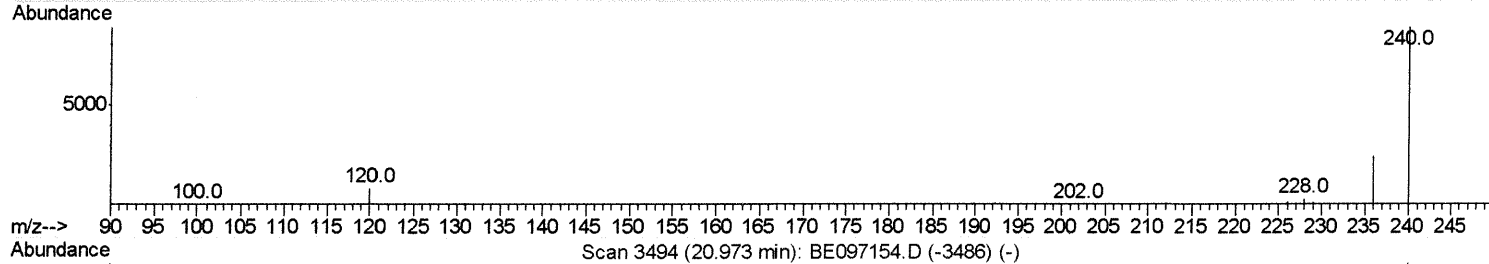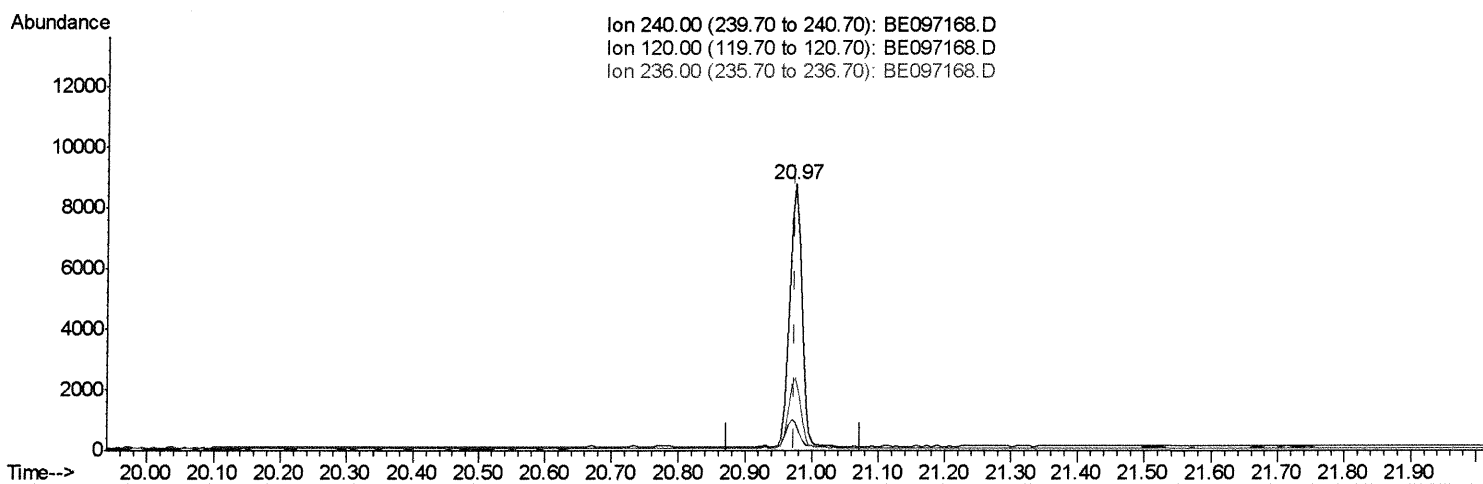

(16) Chrysene-d12 (I)

20.974min (+0.001) 0.40ng/ul m > 50 8/9/18

response 11141

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	10.43#
236.00	34.90	27.40#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

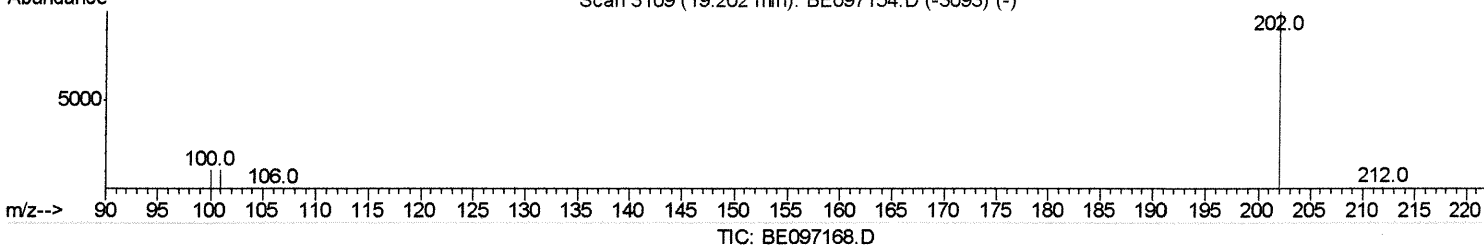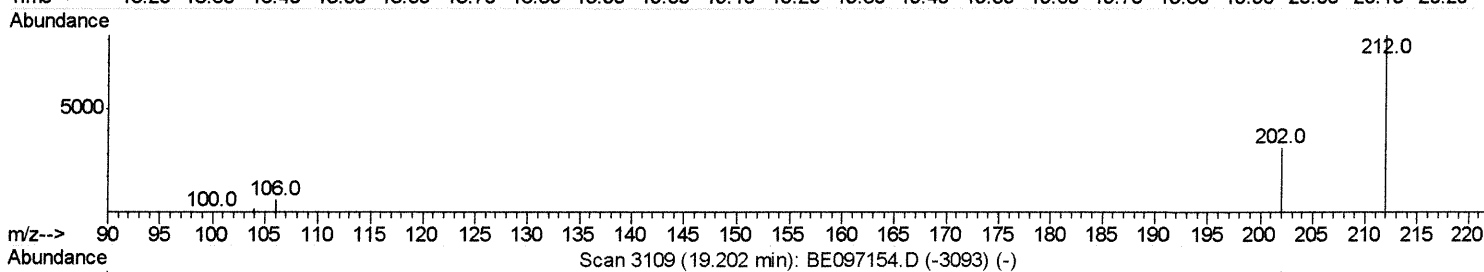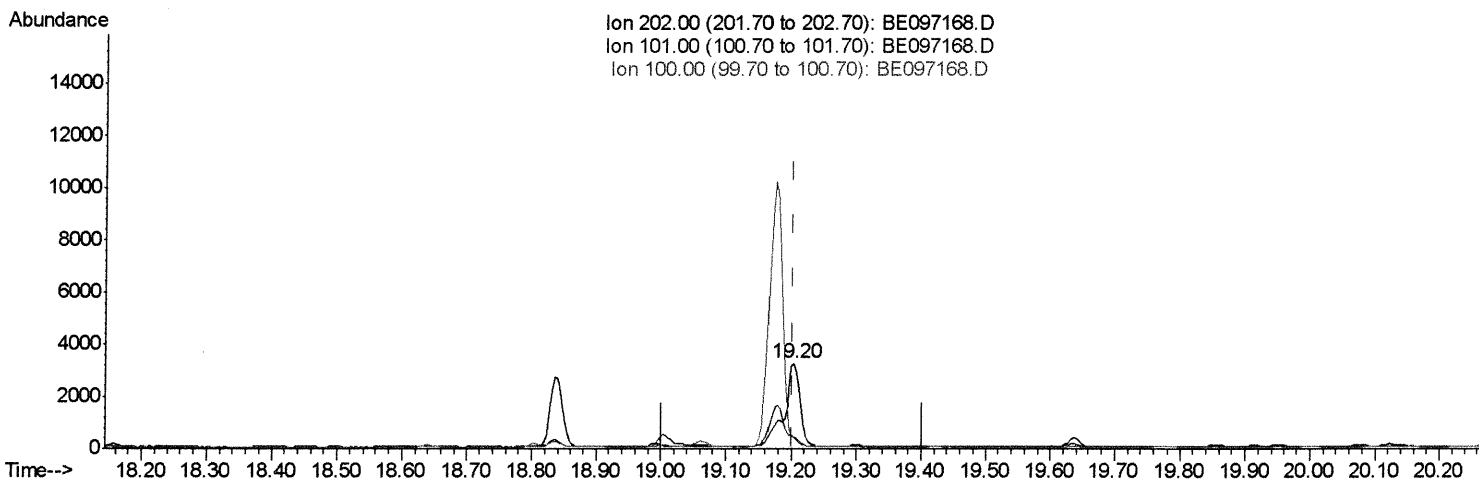

(17) Pyrene

19.203min (+0.001) 0.18ng/ul

response 5401

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	14.64#
100.00	19.50	14.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 07:49:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

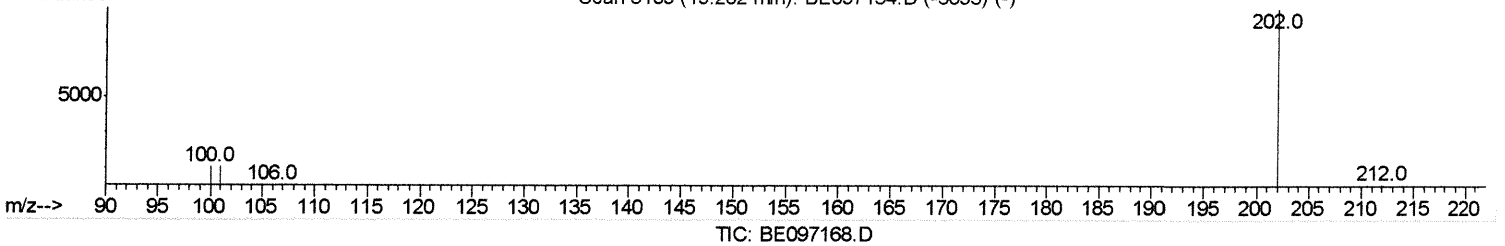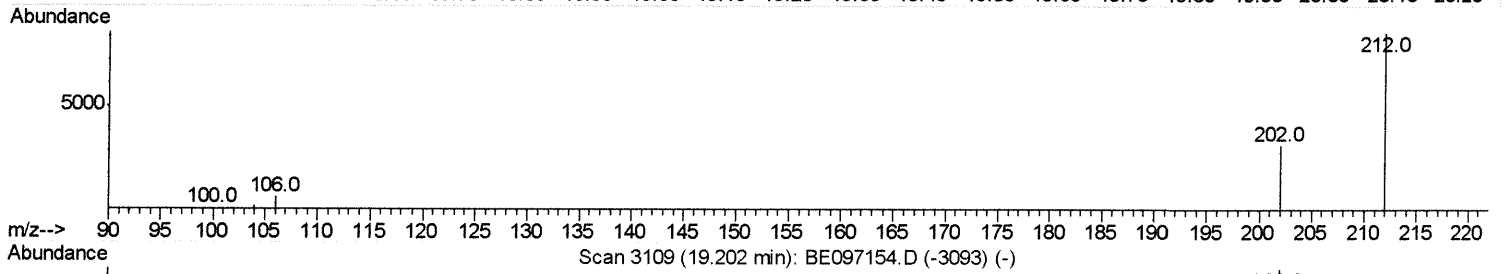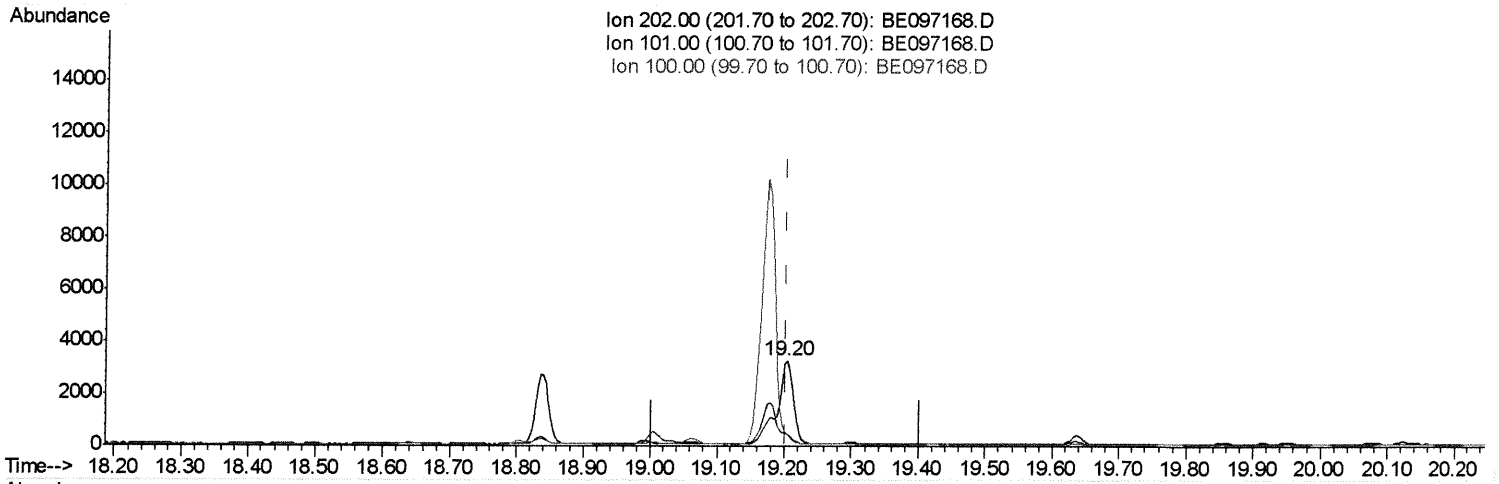

(17) Pyrene

19.203min (+0.001) 0.14ng/ul m > 50 8/9/18

response 4186

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	14.64#
100.00	19.50	14.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:05:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

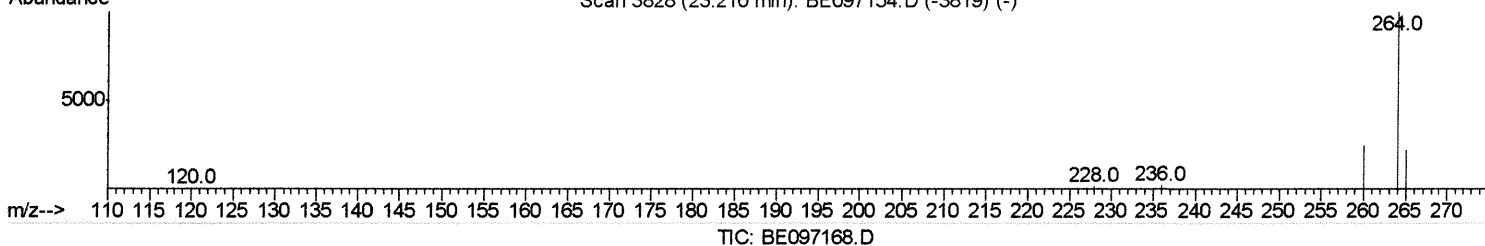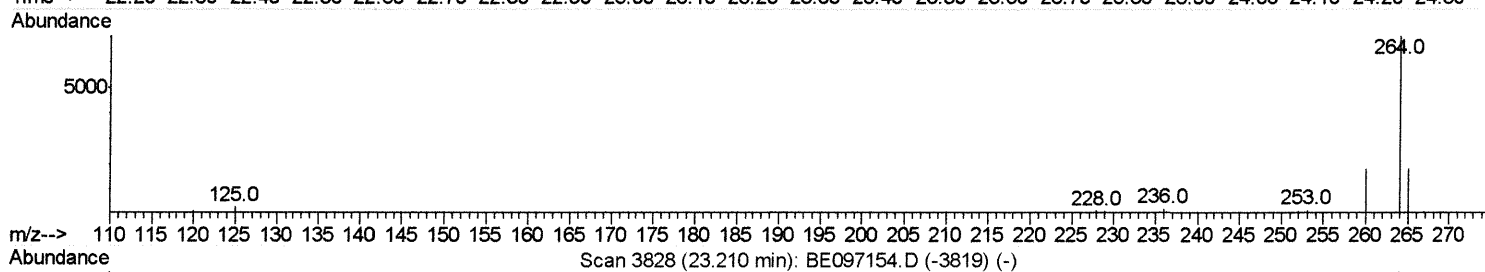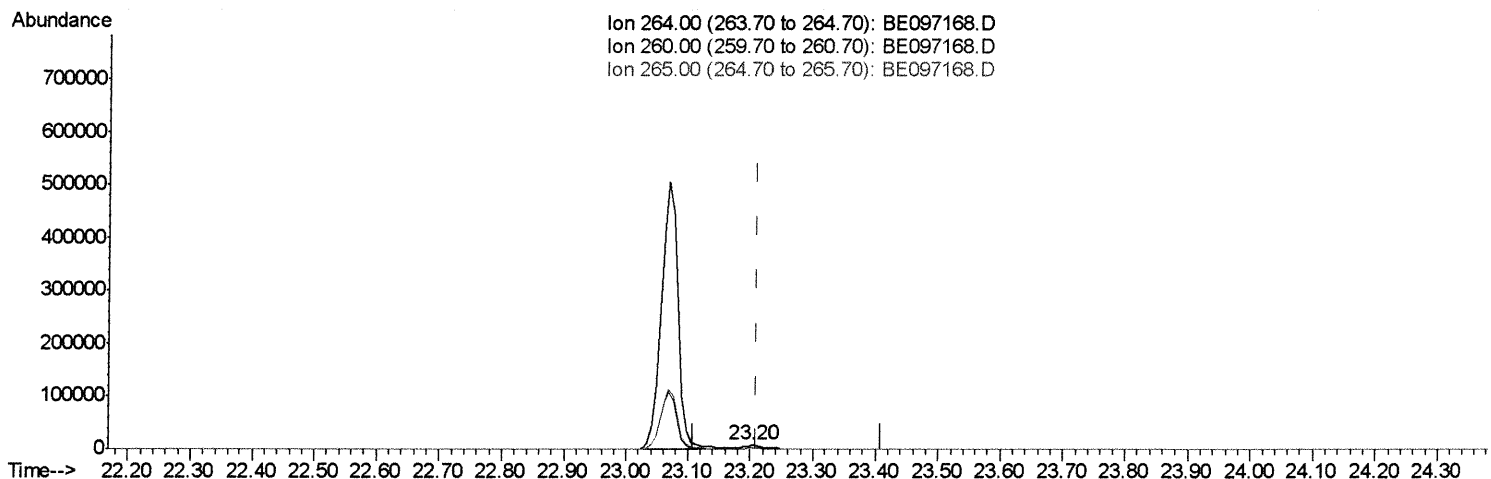

(20) Perylene-d12 (I)

23.202min (-0.008) 0.40ng/ul

response 17458

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.52
265.00	103.50	25.47#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:05:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

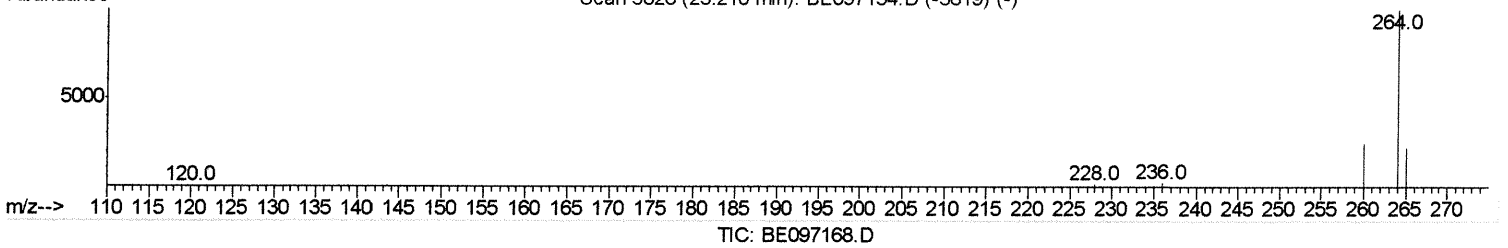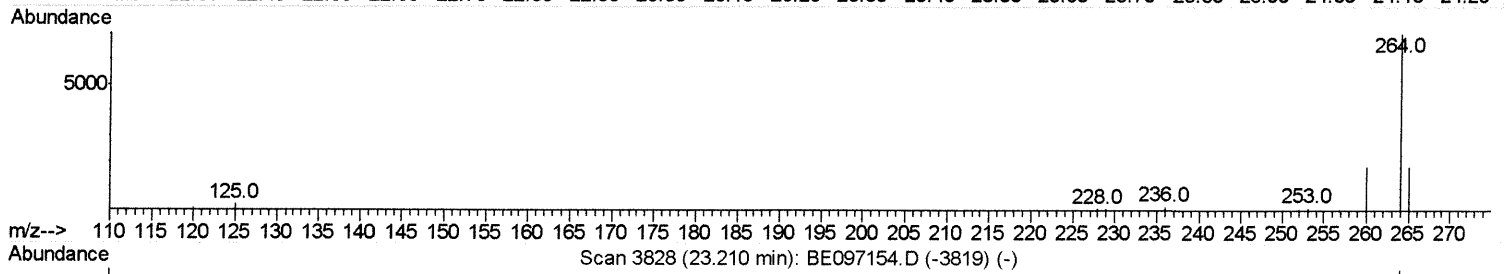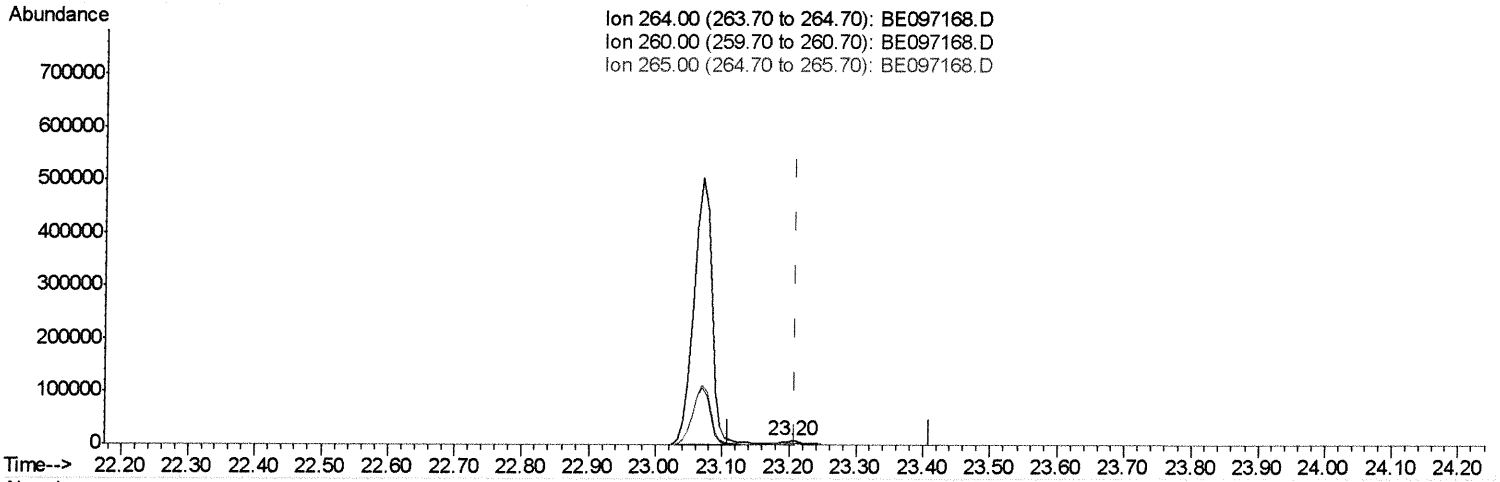

(20) Perylene-d12 (I)

23.202min (-0.008) 0.40ng/ul m > SJ 8/9/18

response 9482

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.52
265.00	103.50	25.47#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:05:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

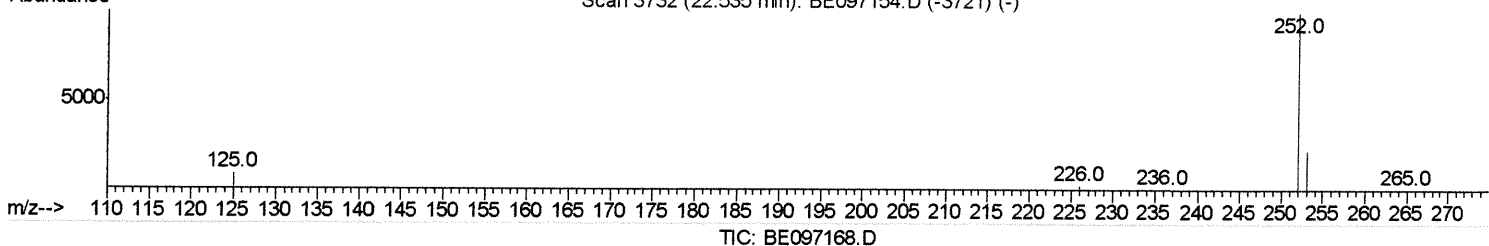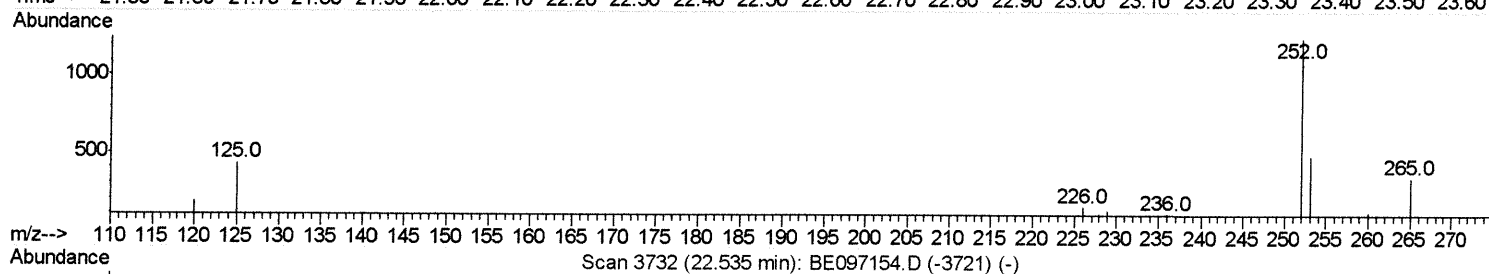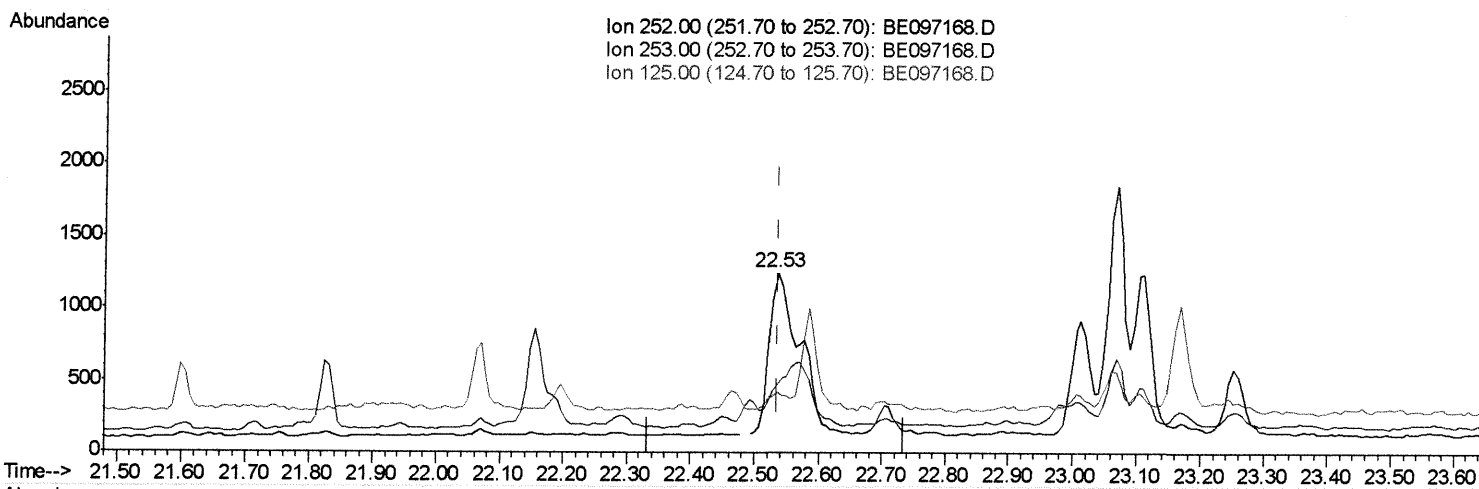

(21) Benzo(b)fluoranthene
 22.534min (-0.001) 0.14ng/ul
 response 3696

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	38.38
125.00	17.50	33.97
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:05:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

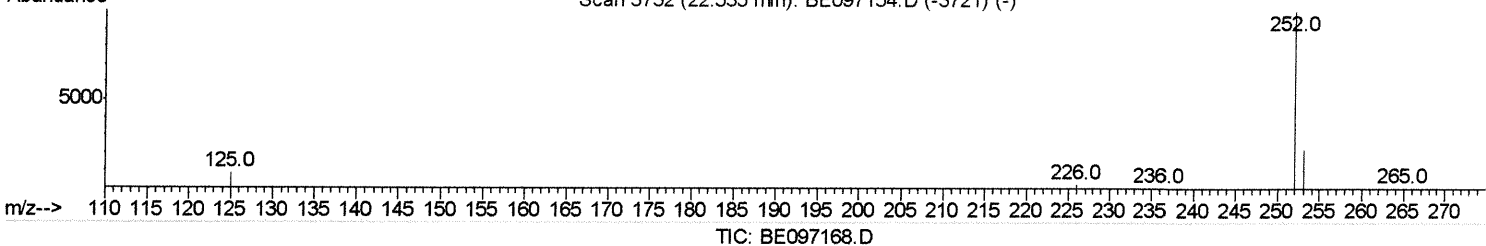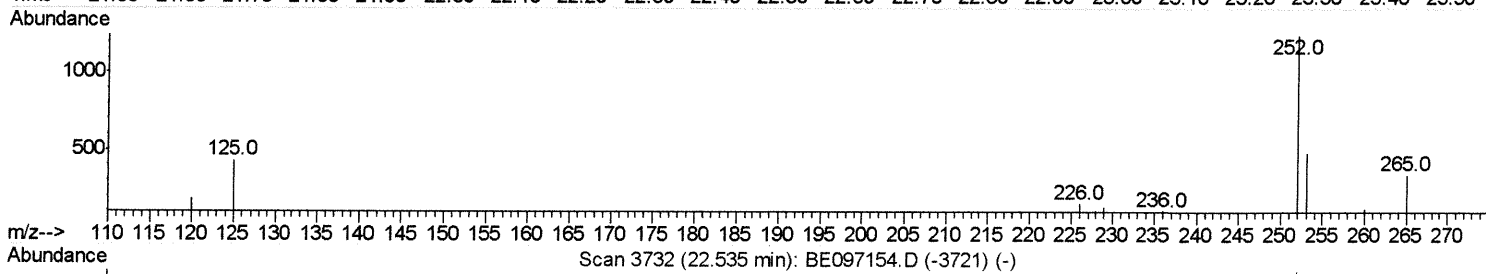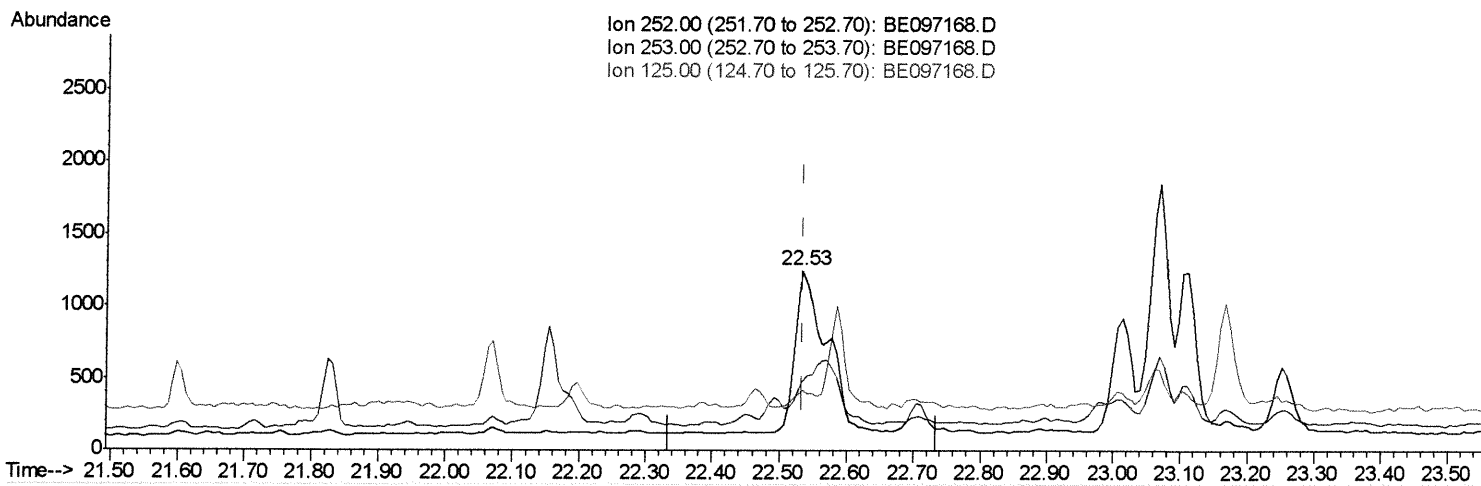

(21) Benzo(b)fluoranthene

22.534min (-0.001) 0.10ng/ul m > SJ 8/9/18

response 2599

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	38.38
125.00	17.50	33.97
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097168.D
Acq On : 3 Aug 2018 1:44
Operator : SJ/JU
Sample : J4171-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1K5

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:05:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 23:40:30 2018
Response via : Initial Calibration

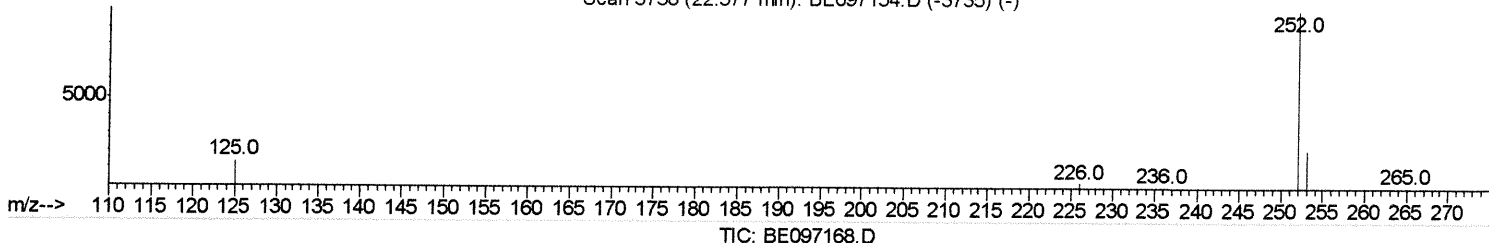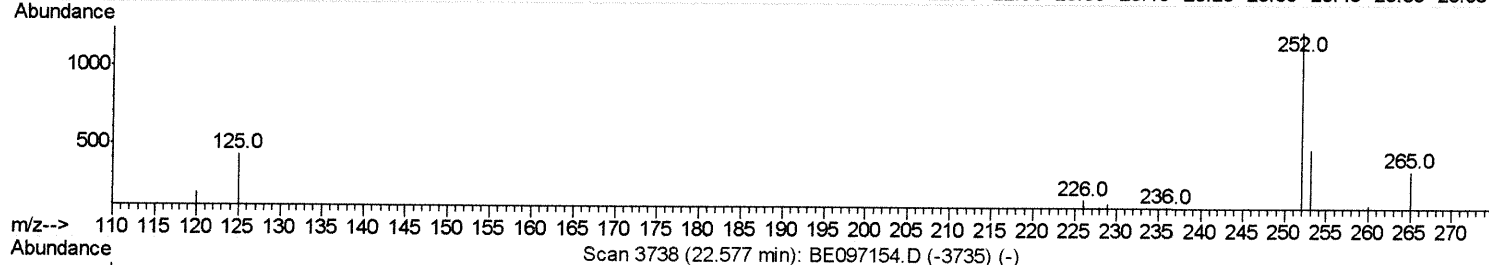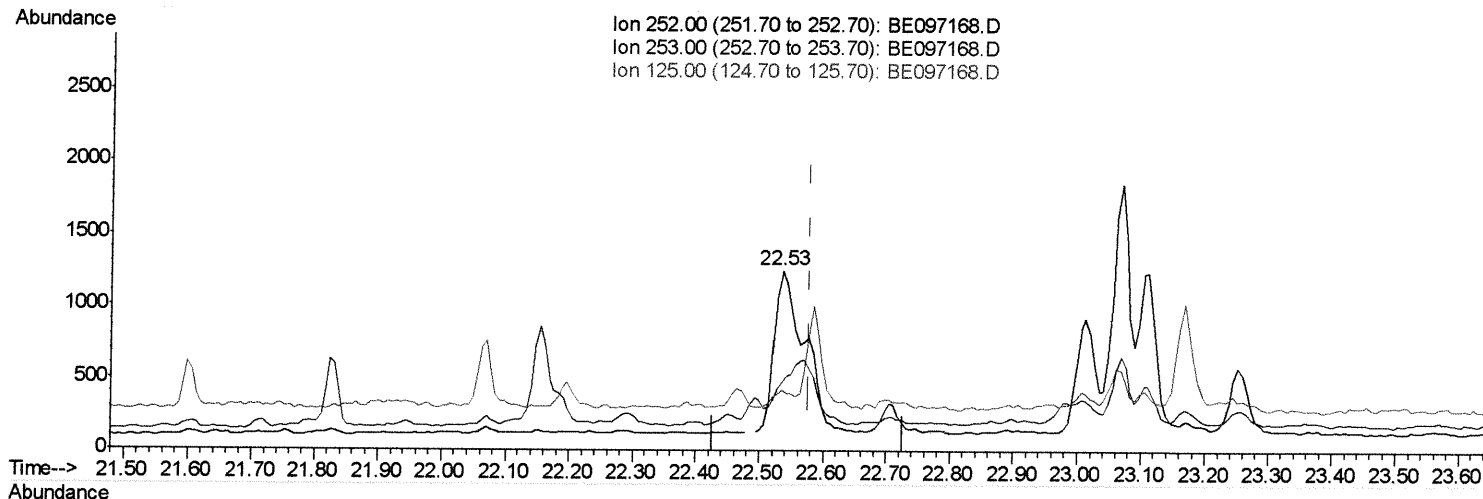

(22) Benzo(k)fluoranthene

22.534min (-0.043) 0.13ng/ul

response 3696

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	38.38#
125.00	17.10	33.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:05:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

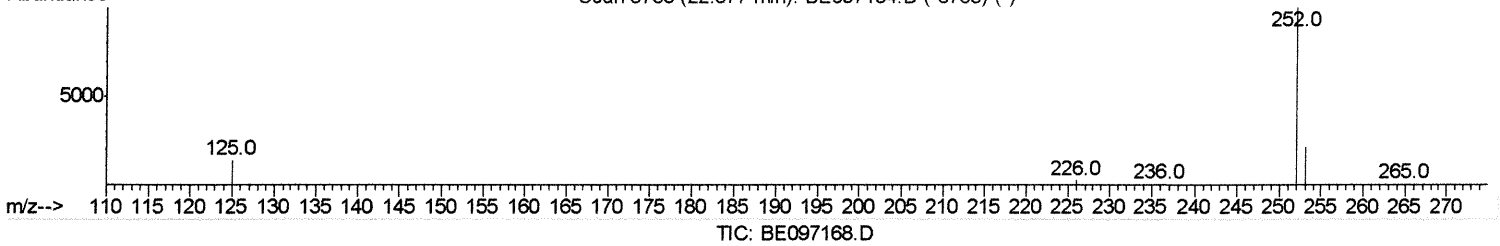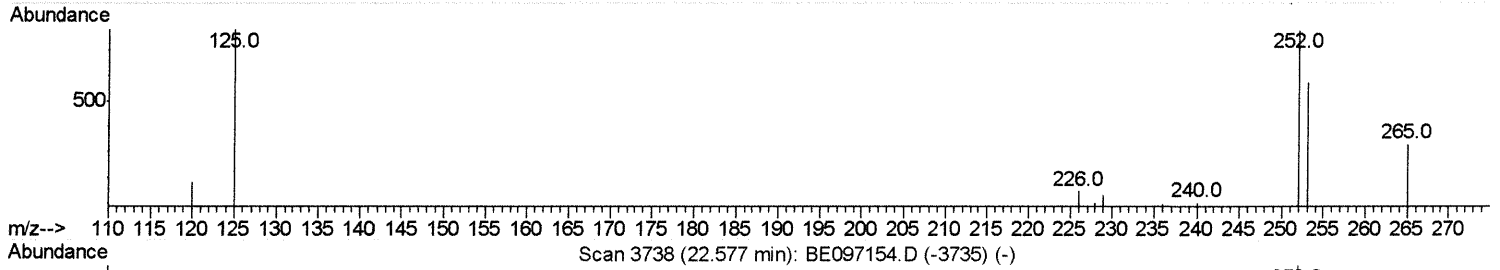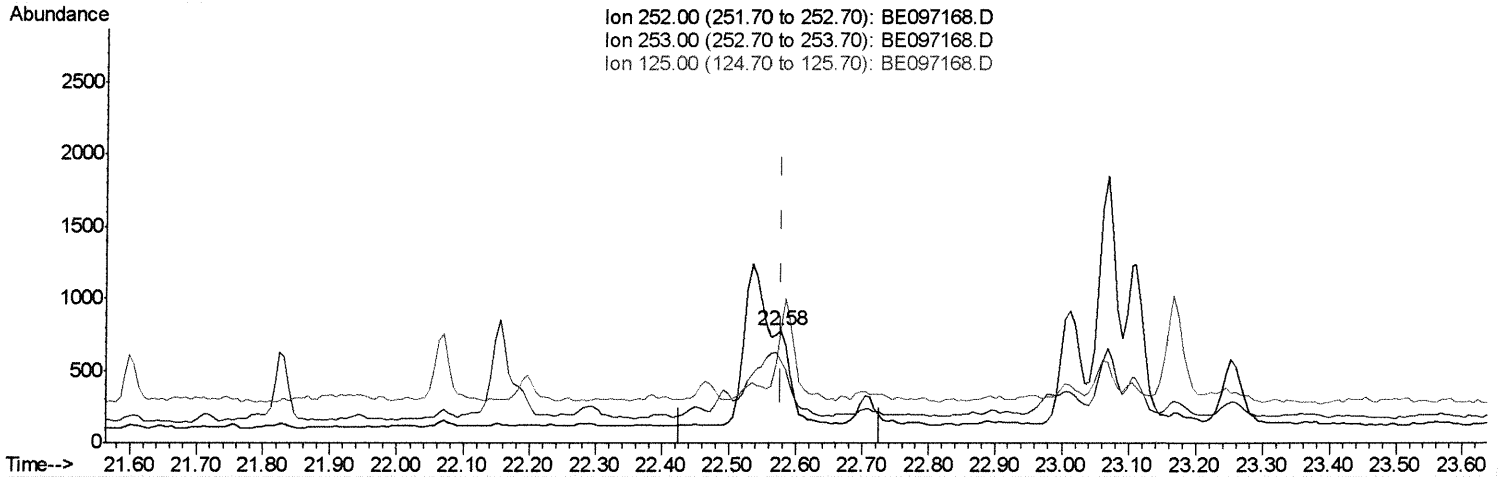

(22) Benzo(k)fluoranthene

22.576min (-0.001) 0.04ng/ul m> 50 819118

response 1088

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	73.81#
125.00	17.10	100.51#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097168.D
 Acq On : 3 Aug 2018 1:44
 Operator : SJ/JU
 Sample : J4171-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1K5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:19 PM

Quant Time: Aug 03 08:06:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 23:40:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1189	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6202	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4046	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	10349m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	11141m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	9482m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.73	152	3298	0.33	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	10907m	0.31	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)	Ovalue
3) Naphthalene	10.18	128	1735	0.116	ng/ul#	94	
5) 2-Methylnaphthalene	11.80	142	1474	0.149	ng/ul	98	
12) Phenanthrene	16.81	178	2951m	0.112	ng/ul		
15) Fluoranthene	18.84	202	3581m	0.103	ng/ul		
17) Pyrene	19.20	202	4186m	0.140	ng/ul		
18) Benzo(a)anthracene	20.96	228	1815	0.057	ng/ul#	89	
19) Chrysene	21.01	228	2192	0.067	ng/ul#	89	
21) Benzo(b)fluoranthene	22.53	252	2599m	0.101	ng/ul		
22) Benzo(k)fluoranthene	22.58	252	1088m	0.039	ng/ul		
23) Benzo(a)pyrene	23.11	252	1793	0.069	ng/ul#	91	
24) Indeno(1,2,3-cd)pyrene	25.49	276	1432	0.044	ng/ul#	86	
26) Benzo(a,h,i)perylene	26.19	276	1488	0.053	ng/ul#	79	

(#) = qualifier out of range (m) = manual integration (+) = signals summed