

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
 Data File : BE097161.D
 Acq On : 2 Aug 2018 21:21
 Operator : SJ/JU
 Sample : J4171-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J0

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:09 PM

Quant Time: Aug 03 00:09:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 02 14:49:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1287	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6615	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4285	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	10475m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	11373m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	10379m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	4605	0.43	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	14204m	0.39	ng/ul	0.00
Target Compounds						
15) Fluoranthene	18.84	202	1199m	0.034	ng/ul	Ovalue
17) Pyrene	19.20	202	1069	0.035	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080218\
Data File : BE097161.D
Acq On : 2 Aug 2018 21:21
Operator : SJ/JU
Sample : J4171-02
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
JJ1J0

Manual Integrations
APPROVED

Sohil
8/3/2018 5:55:09 PM

Quant Time: Aug 03 00:09:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 02 14:49:13 2018
Response via : Initial Calibration

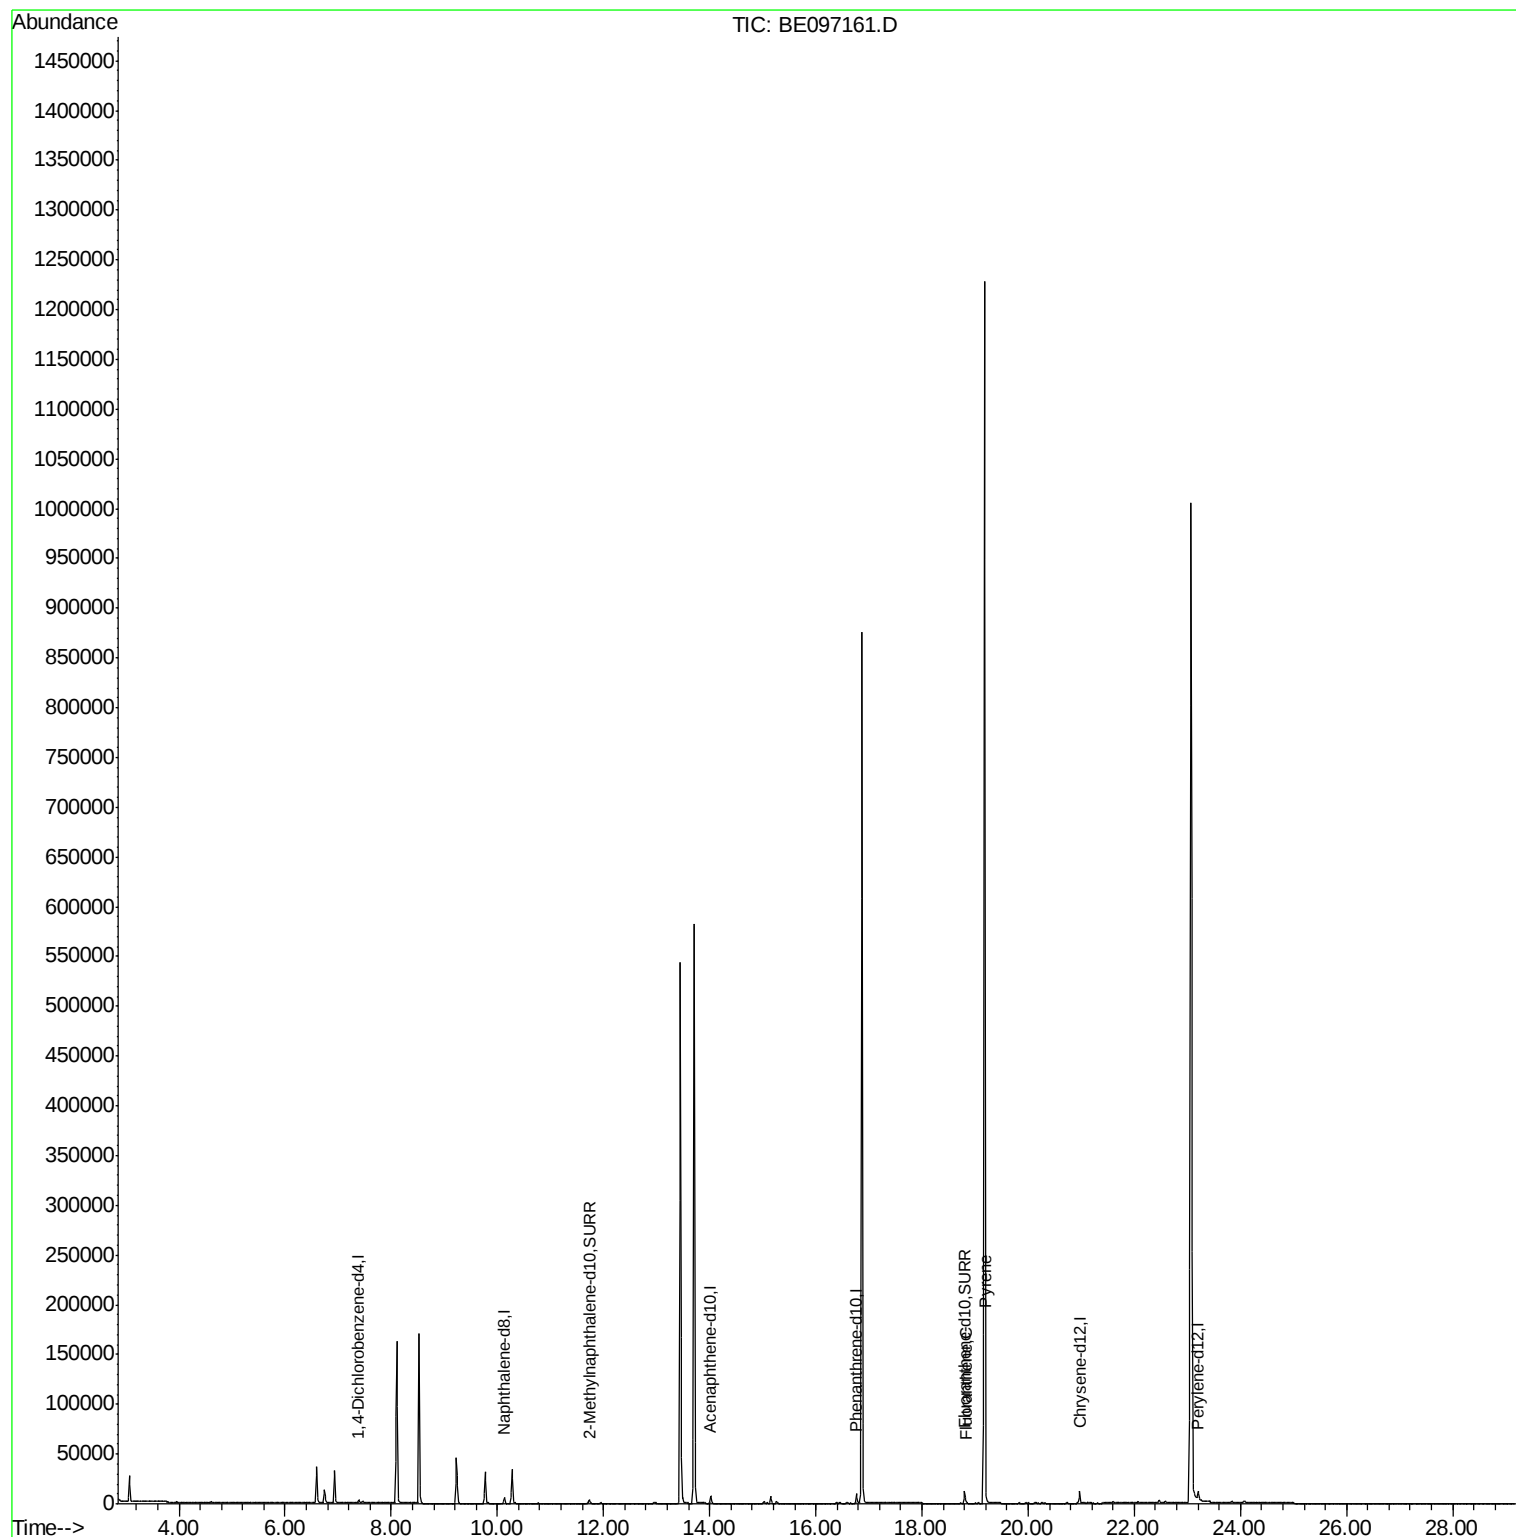

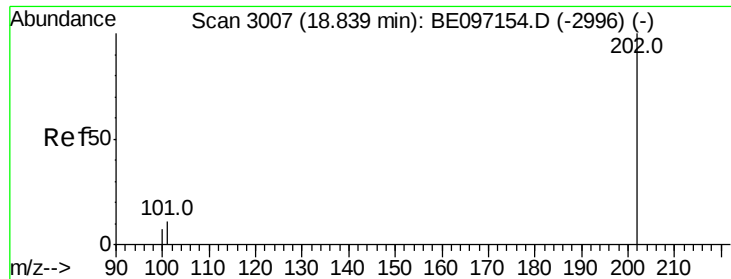





#15
Fluoranthene
 Concen: 0.034 ng/ul m
 RT: 18.84 min Scan# 3008
 Delta R.T. -0.00 min
 Lab File: BE097161.D
 Acq: 2 Aug 2018 21:21

Instrument :
 BNA_E
 ClientSampleId :
 JJ1J0

Tot Ion:	202	Resp:	1199
Ion Ratio	Lower	Upper	
202	100		
101	17.1	0.0	30.3
100	14.0	0.0	39.5

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:55:09 PM

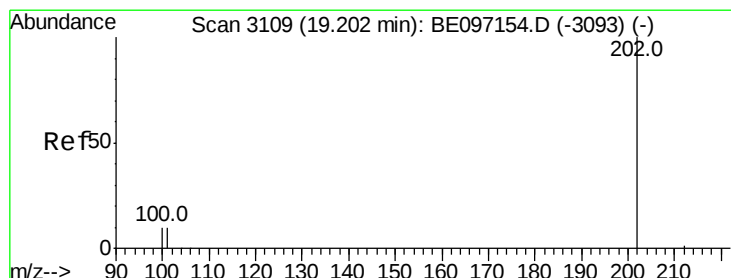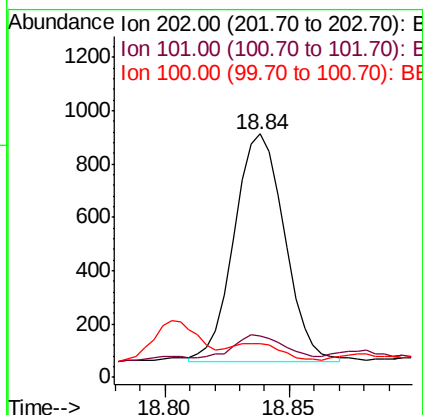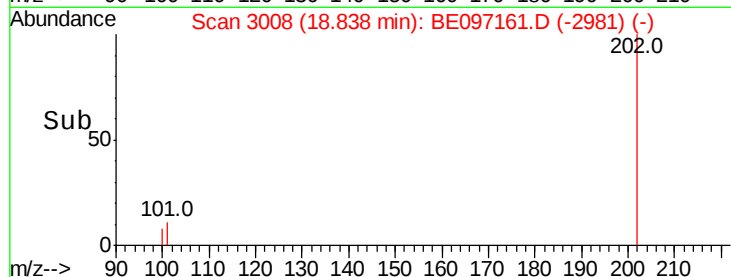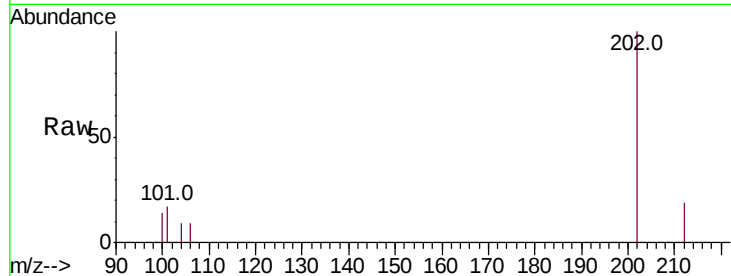

#17
Pyrene
 Concen: 0.035 ng/ul
 RT: 19.20 min Scan# 3110
 Delta R.T. -0.00 min
 Lab File: BE097161.D
 Acq: 2 Aug 2018 21:21

Tgt Ion:	202	Resp:	1069
Ion Ratio	Lower	Upper	
202	100		
101	22.2	18.2	27.4
100	30.1	15.6	23.4#

