
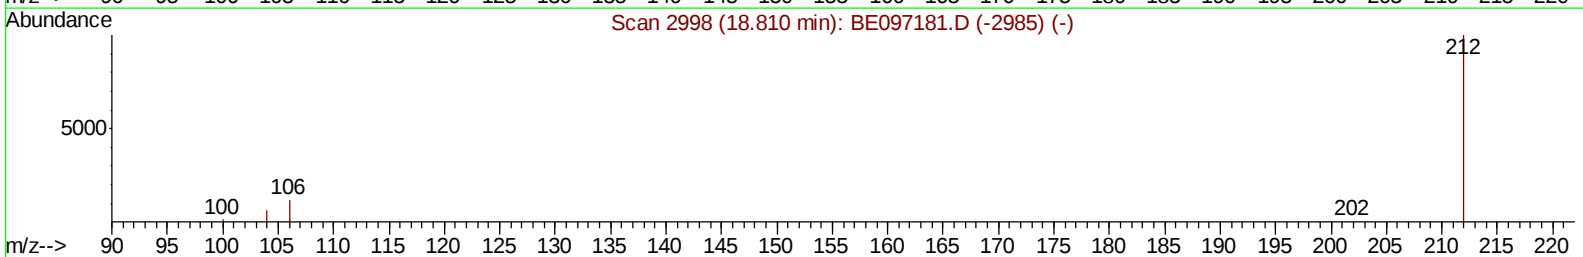
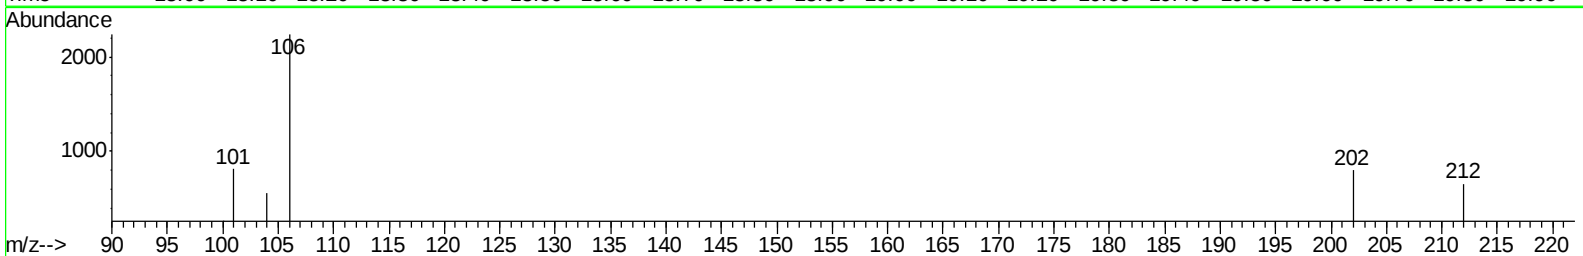


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097182.D
Acq On : 3 Aug 2018 16:42
Operator : SJ/JU
Sample : J4171-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 03 23:42:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

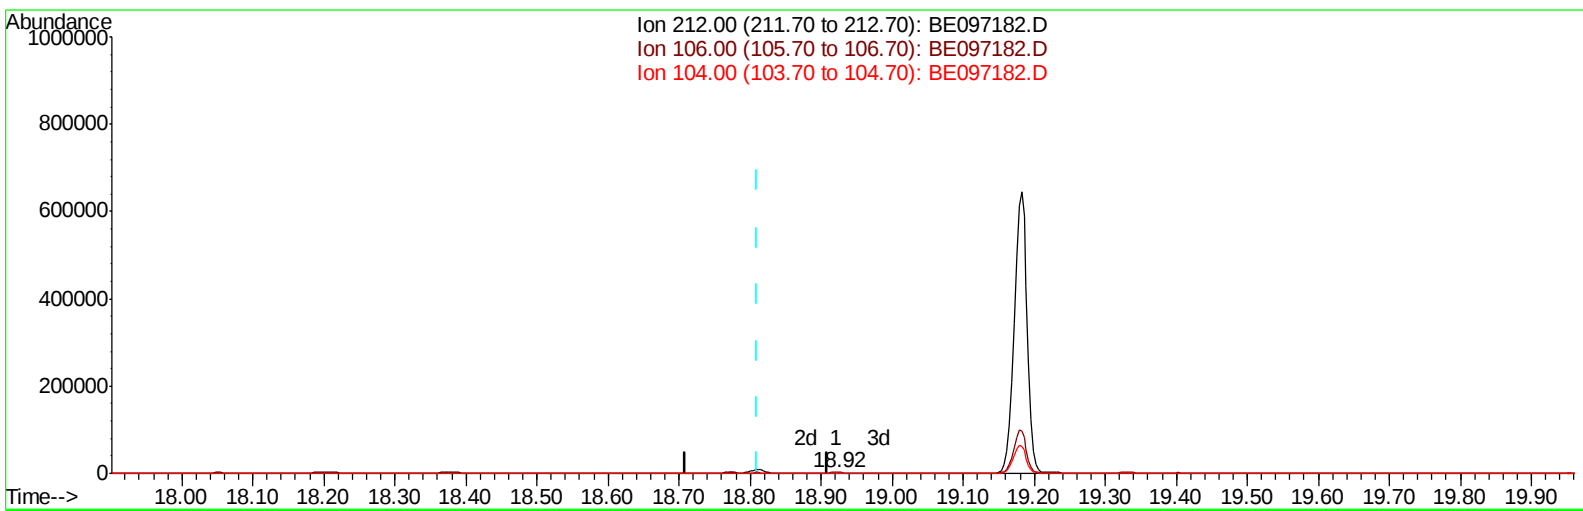

TIC: BE097182.D

(14) Fluoranthene-d10 (SURR)

18.921min (+0.111) 0.01ng/ul

response 447

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	516.78#
104.00	15.60	93.96#
0.00	0.00	0.00