
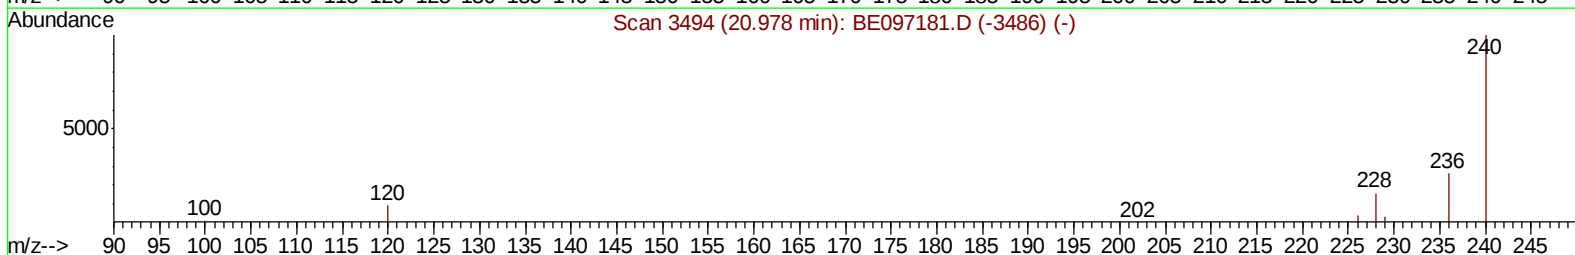
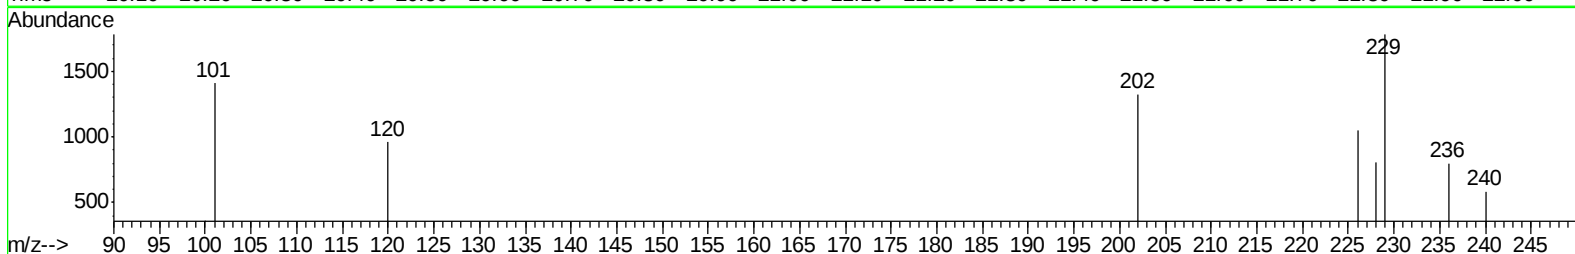


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097182.D
 Acq On : 3 Aug 2018 16:42
 Operator : SJ/JU
 Sample : J4171-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Aug 03 23:42:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration

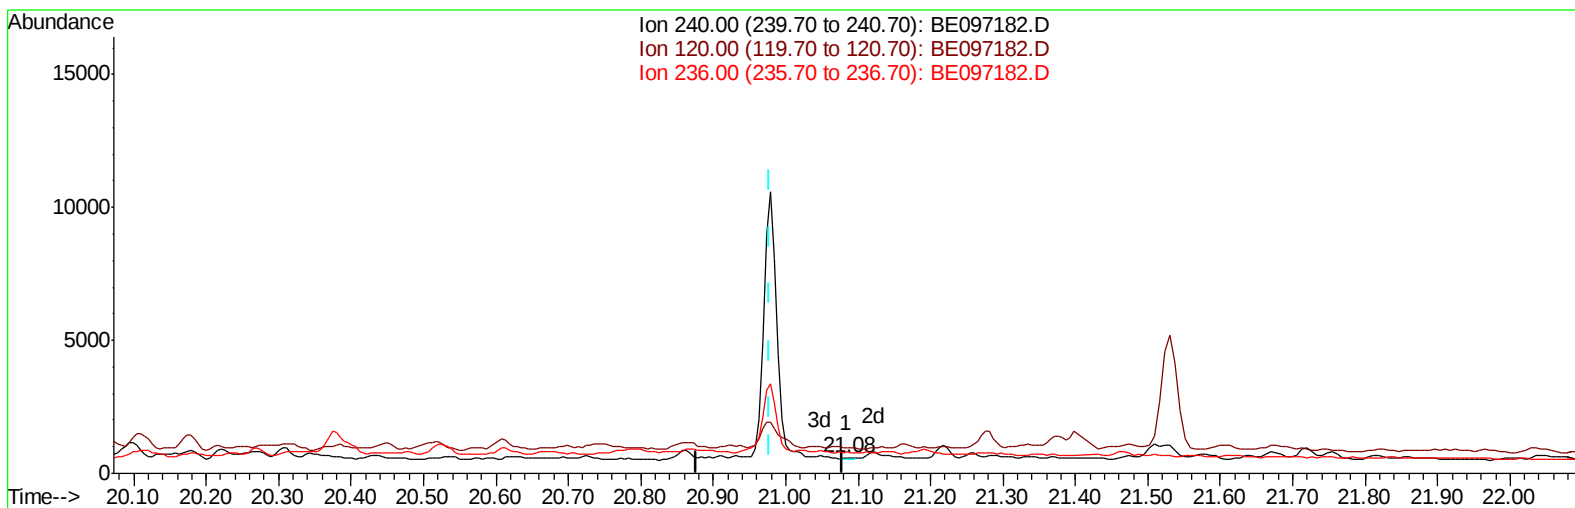

TIC: BE097182.D

(16) Chrysene-d12 (I)

21.085min (+0.107) 0.40ng/ul

response 31

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	165.13#
236.00	34.90	136.24#
0.00	0.00	0.00