
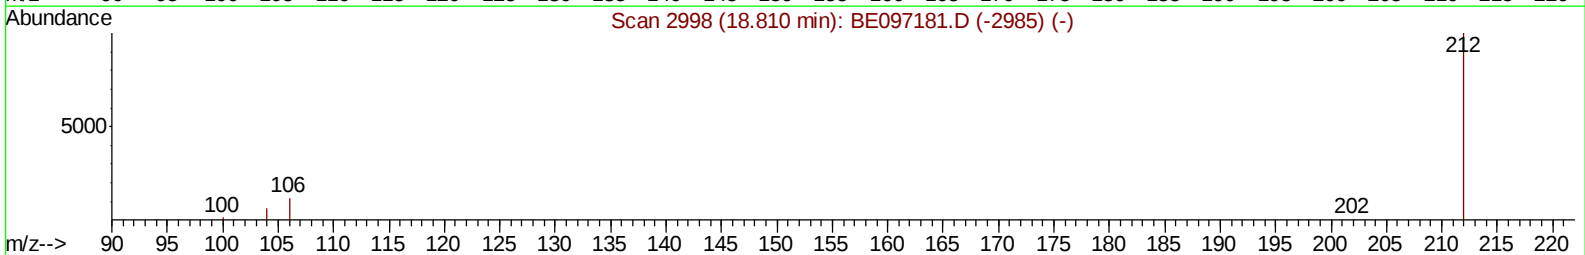
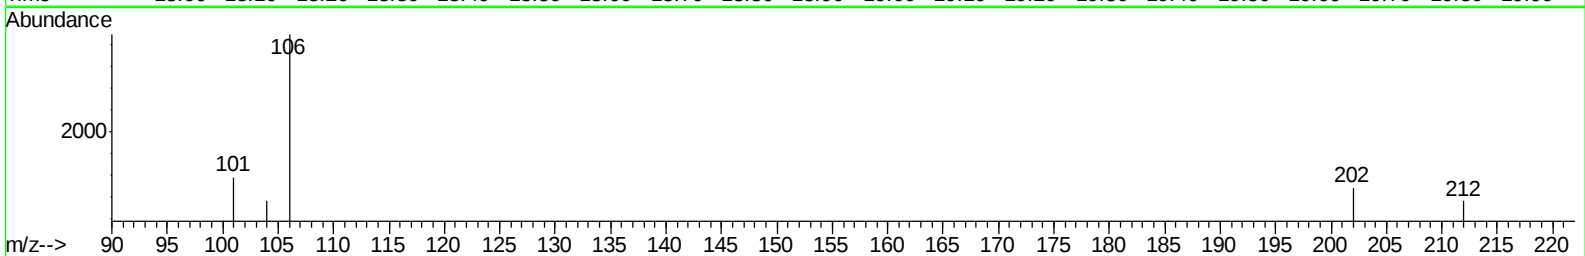


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
Data File : BE097183.D  
Acq On : 3 Aug 2018 17:18  
Operator : SJ/JU  
Sample : J4171-05  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 03 23:50:26 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 03 23:39:09 2018  
Response via : Initial Calibration

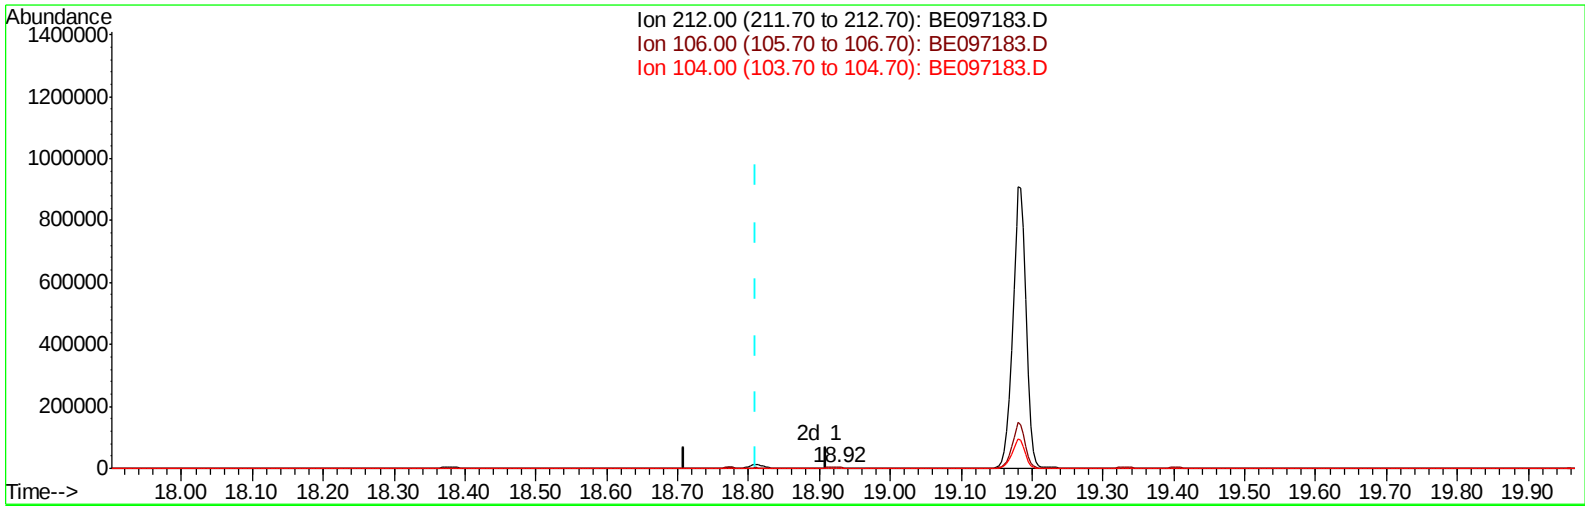

TIC: BE097183.D

(14) Fluoranthene-d10 (SURR)

18.924min (+0.114) 0.01ng/ul

response 432

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 212.00 | 100   | 100     |
| 106.00 | 18.30 | 937.96# |
| 104.00 | 15.60 | 138.89# |
| 0.00   | 0.00  | 0.00    |