
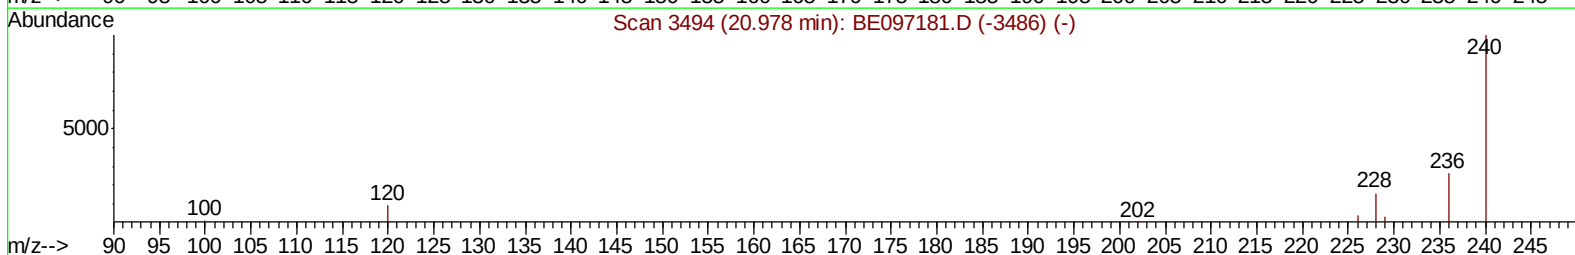
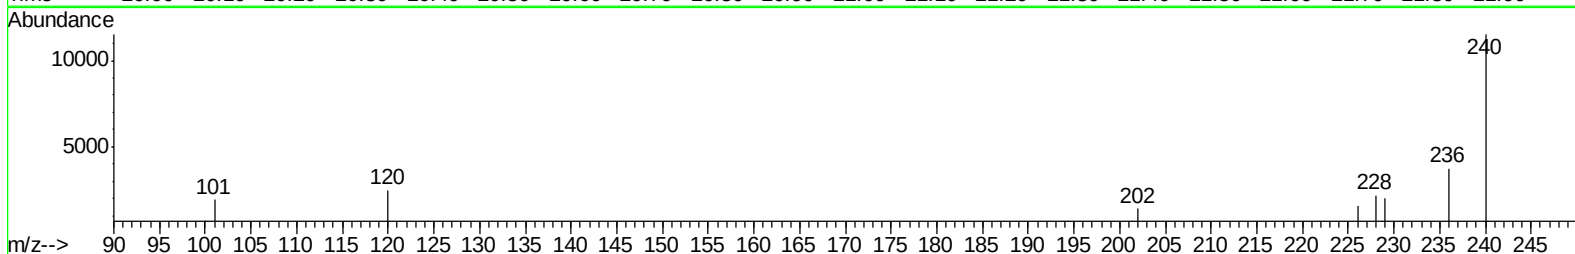


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
Data File : BE097183.D  
Acq On : 3 Aug 2018 17:18  
Operator : SJ/JU  
Sample : J4171-05  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 03 23:50:26 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 03 23:39:09 2018  
Response via : Initial Calibration

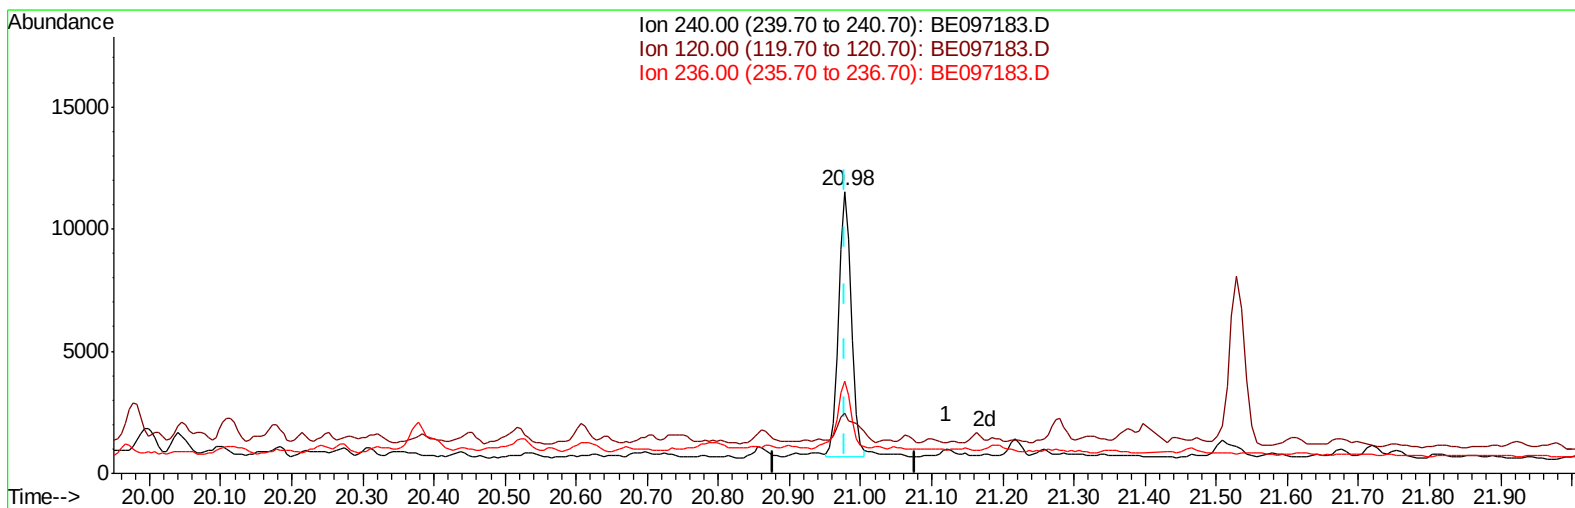

TIC: BE097183.D

(16) Chrysene-d12 (I)

20.978min (-0.000) 0.40ng/ul m

response 13081

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 240.00 | 100   | 100   |
| 120.00 | 20.60 | 21.55 |
| 236.00 | 34.90 | 32.57 |
| 0.00   | 0.00  | 0.00  |