
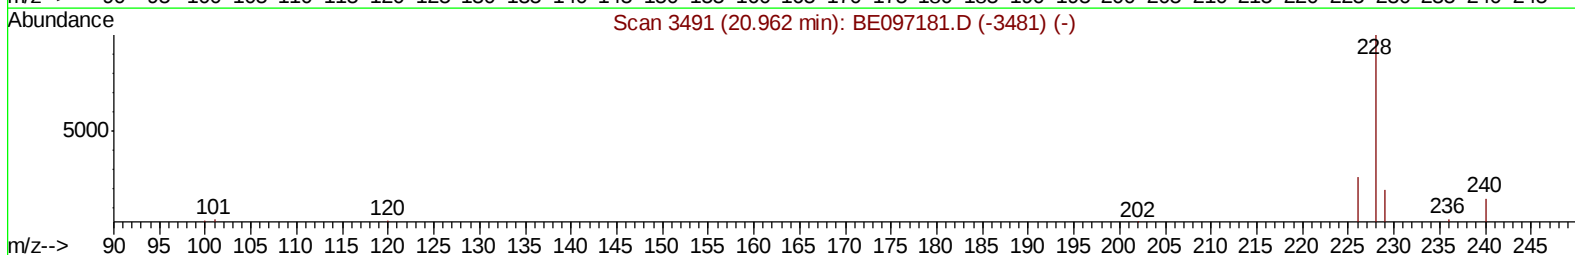
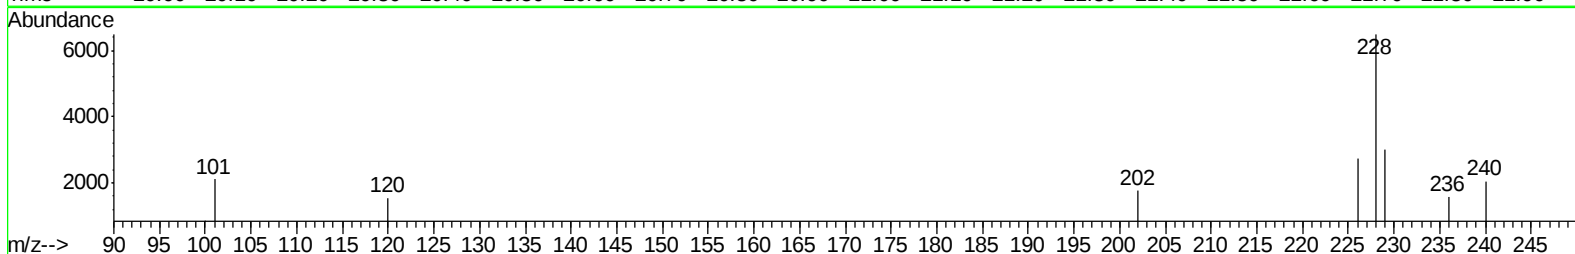


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097183.D
Acq On : 3 Aug 2018 17:18
Operator : SJ/JU
Sample : J4171-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 03 23:50:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

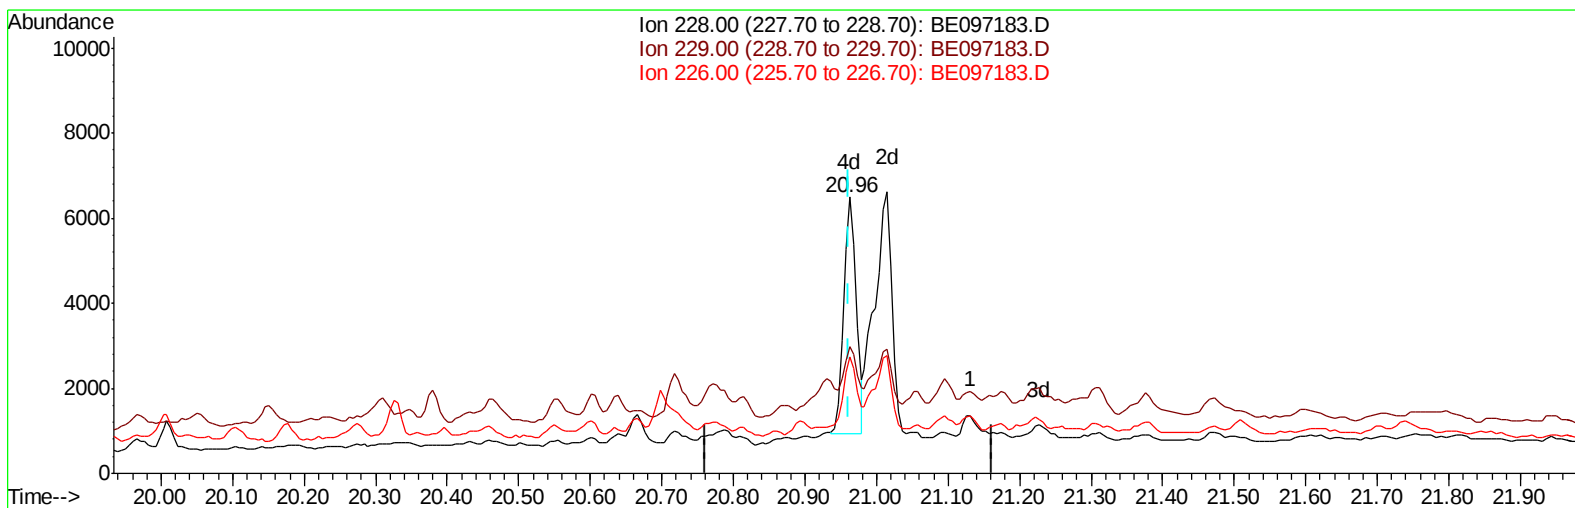

TIC: BE097183.D

(18) Benzo(a)anthracene

20.962min (-0.000) 0.18ng/ul m

response 6715

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	46.02#
226.00	21.30	42.32#
0.00	0.00	0.00