
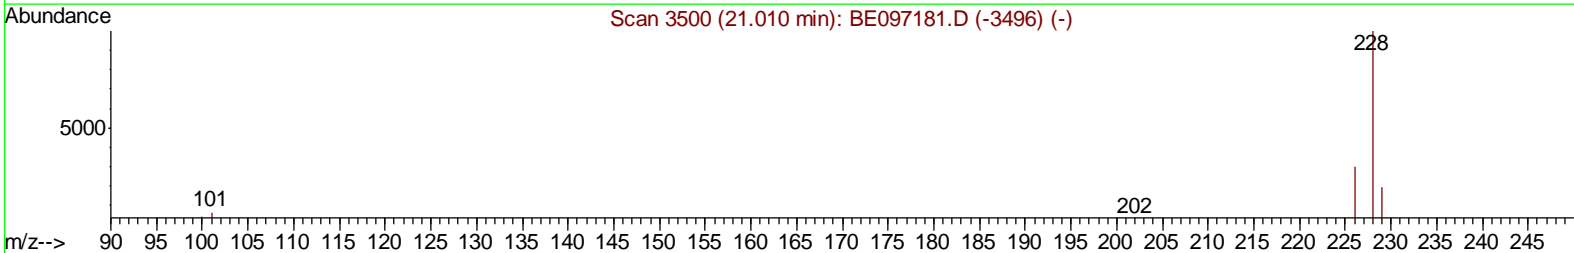
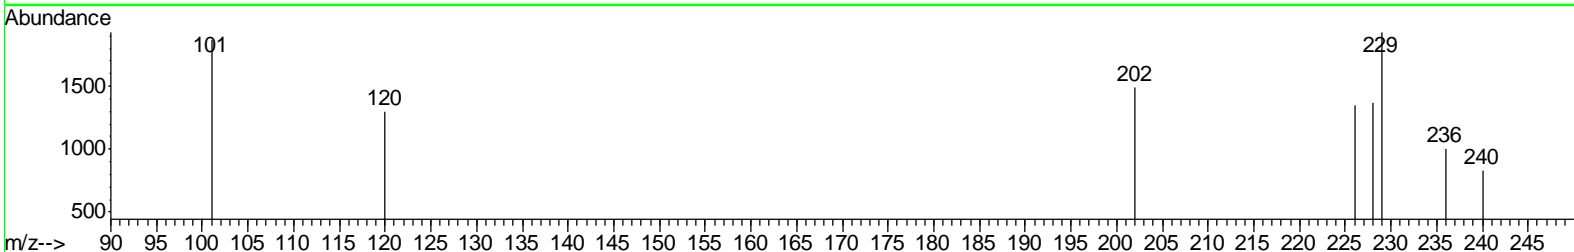


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
 Data File : BE097183.D  
 Acq On : 3 Aug 2018 17:18  
 Operator : SJ/JU  
 Sample : J4171-05  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 03 23:50:26 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Aug 03 23:39:09 2018  
 Response via : Initial Calibration

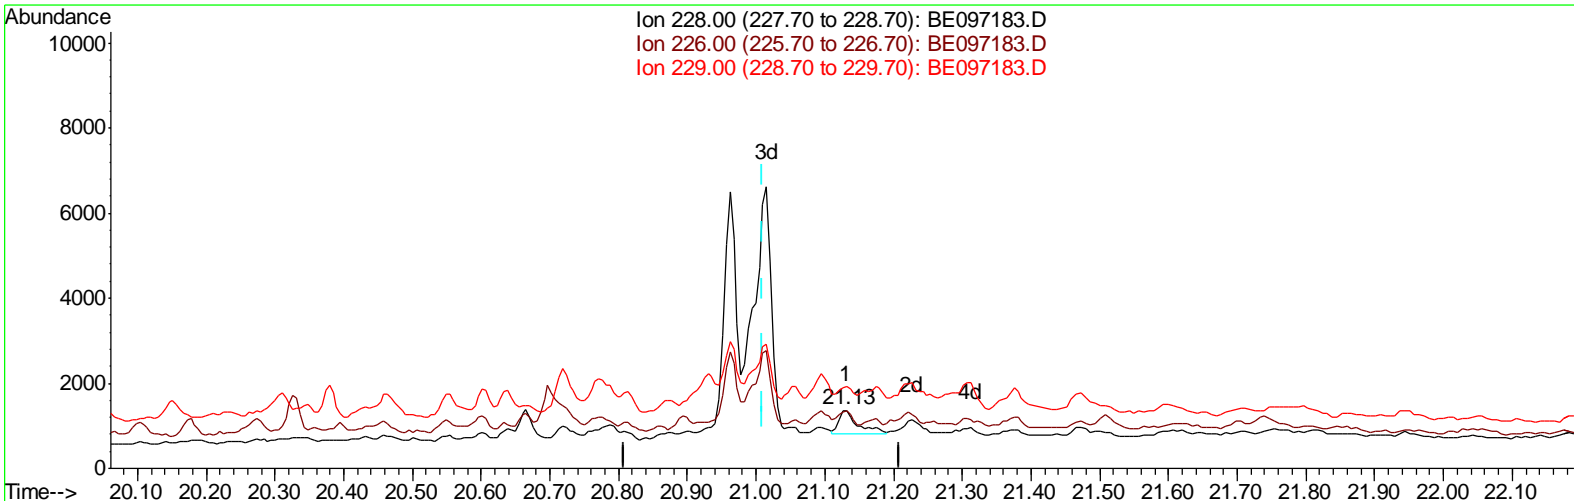

TIC: BE097183.D

(19) Chrysene

21.132min (+0.122) 0.03ng/ul

response 1099

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	98.68#
229.00	22.10	140.94#
0.00	0.00	0.00