
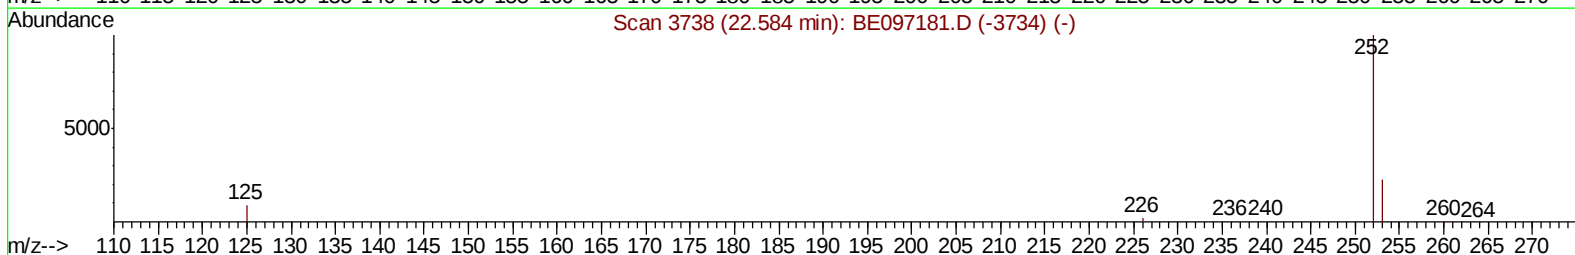
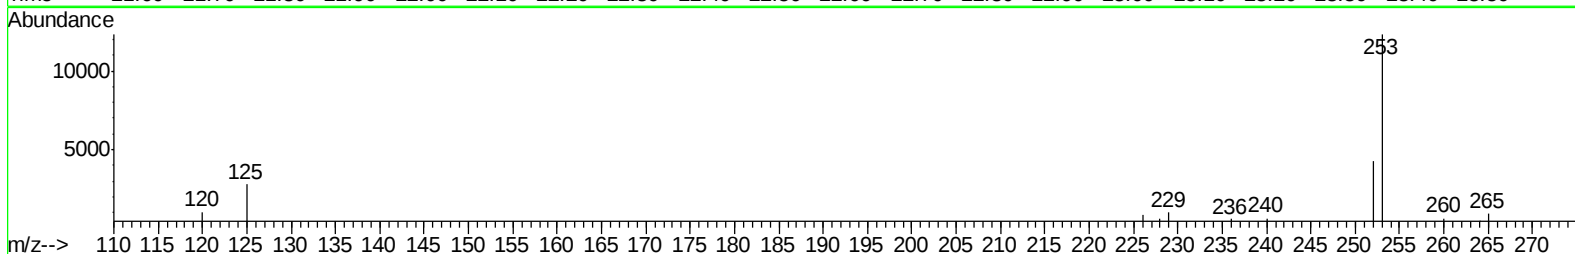


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097183.D
Acq On : 3 Aug 2018 17:18
Operator : SJ/JU
Sample : J4171-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 03 23:53:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

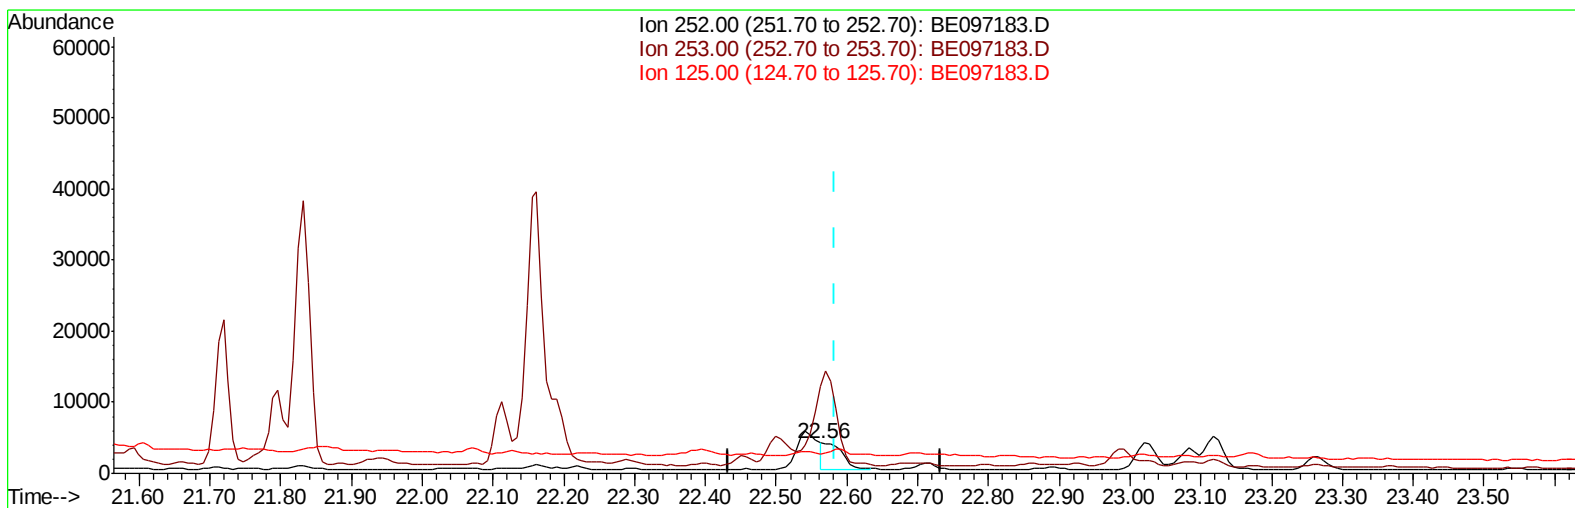

TIC: BE097183.D

(22) Benzo(k)fluoranthene

22.563min (-0.021) 0.20ng/ul m

response 6872

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	288.31#
125.00	17.10	65.11#
0.00	0.00	0.00