
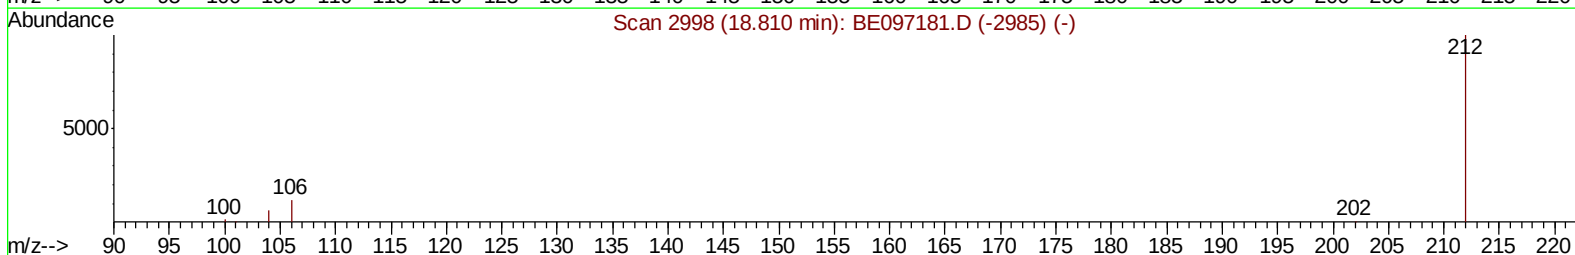
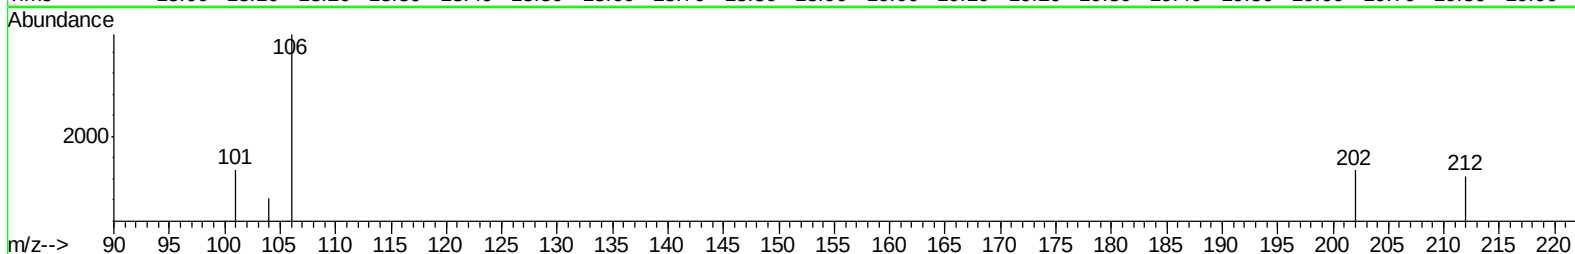


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097184.D
 Acq On : 3 Aug 2018 18:00
 Operator : SJ/JU
 Sample : J4171-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 03 23:54:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration

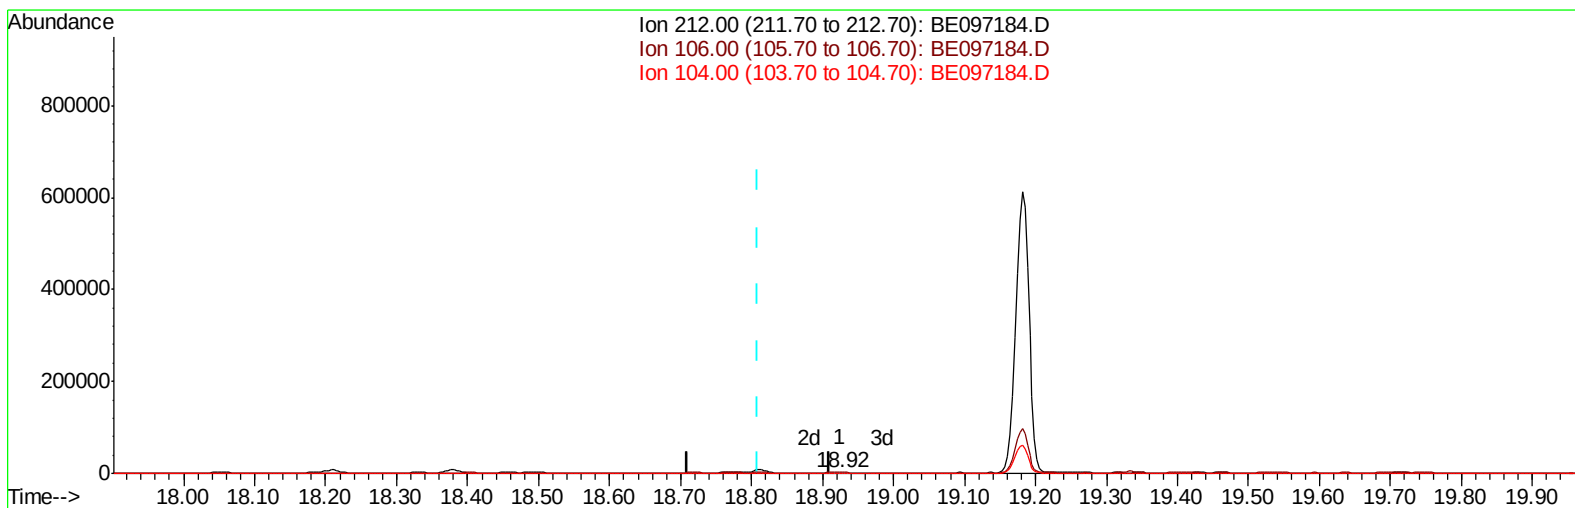

TIC: BE097184.D

(14) Fluoranthene-d10 (SURR)

18.924min (+0.114) 0.03ng/ul

response 1183

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	374.81#
104.00	15.60	49.54#
0.00	0.00	0.00