
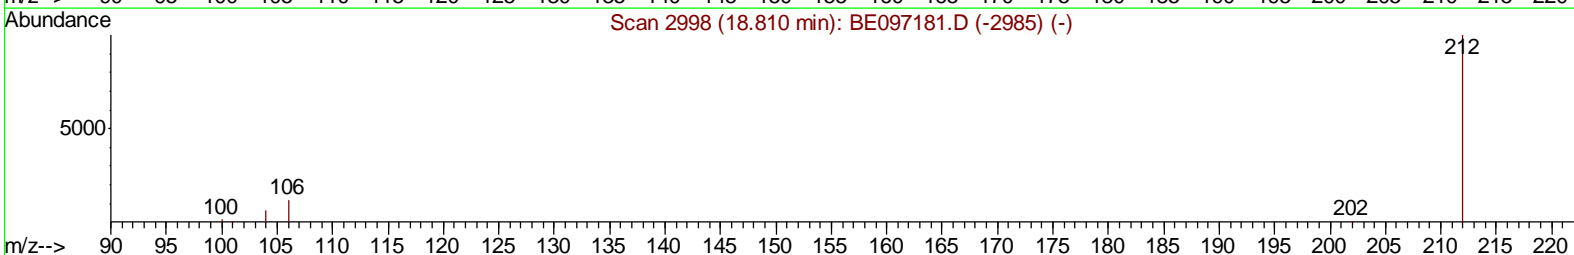
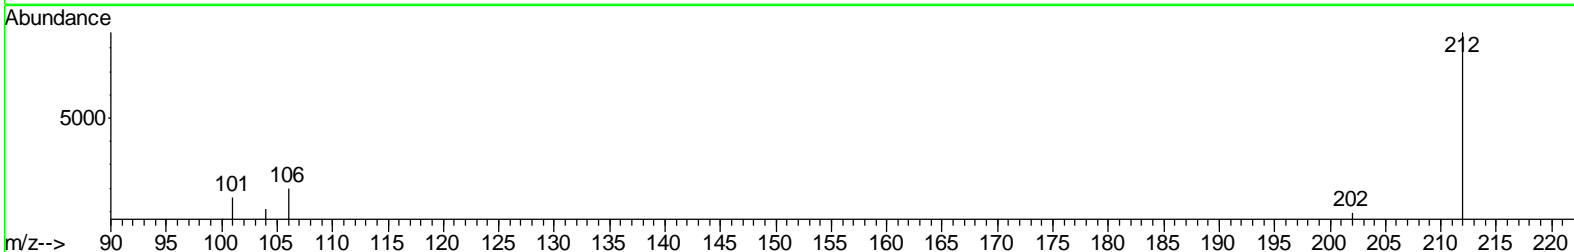


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
 Data File : BE097184.D  
 Acq On : 3 Aug 2018 18:00  
 Operator : SJ/JU  
 Sample : J4171-09  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 03 23:54:51 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Aug 03 23:39:09 2018  
 Response via : Initial Calibration

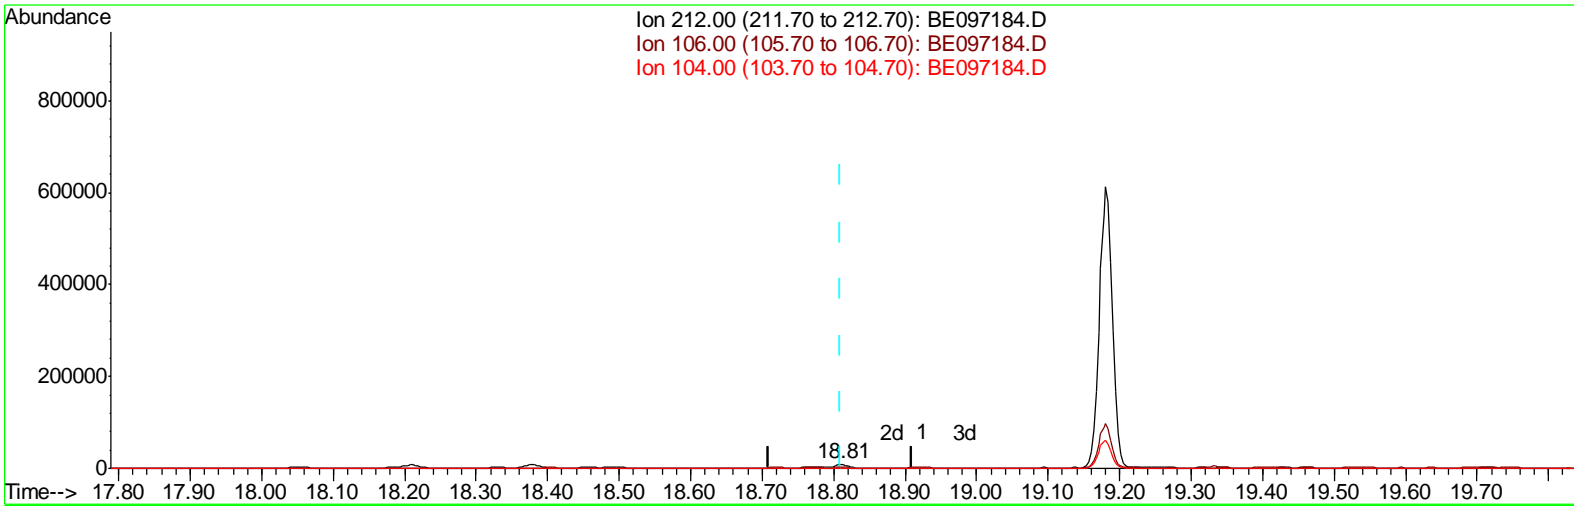

TIC: BE097184.D

(14) Fluoranthene-d10 (SURR)

18.810min (-0.000) 0.29ng/ul m

response 12568

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	35.28#
104.00	15.60	4.66#
0.00	0.00	0.00