
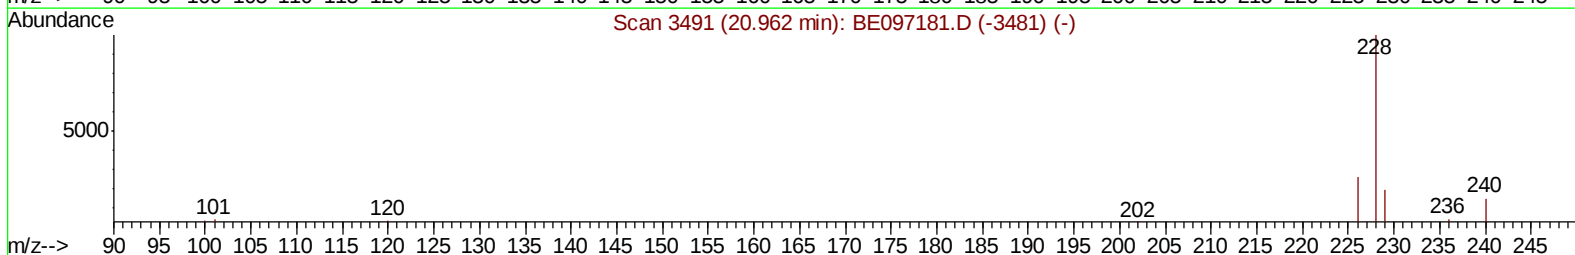
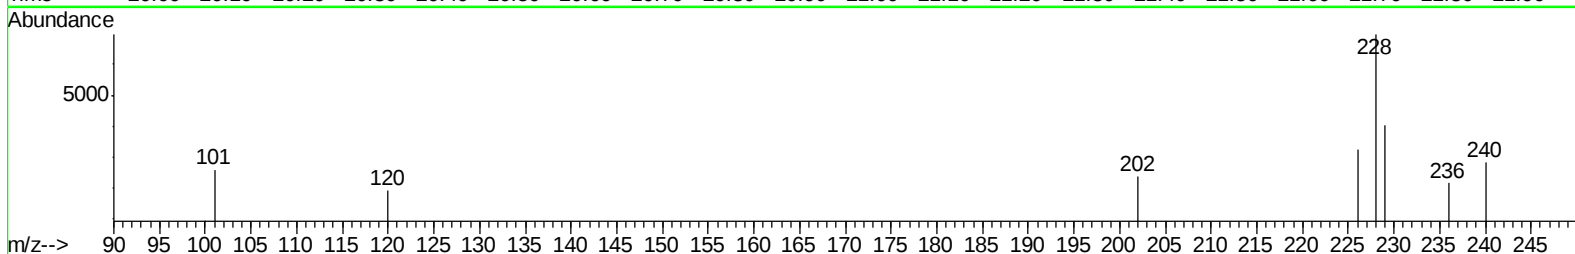


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097184.D
Acq On : 3 Aug 2018 18:00
Operator : SJ/JU
Sample : J4171-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 03 23:54:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

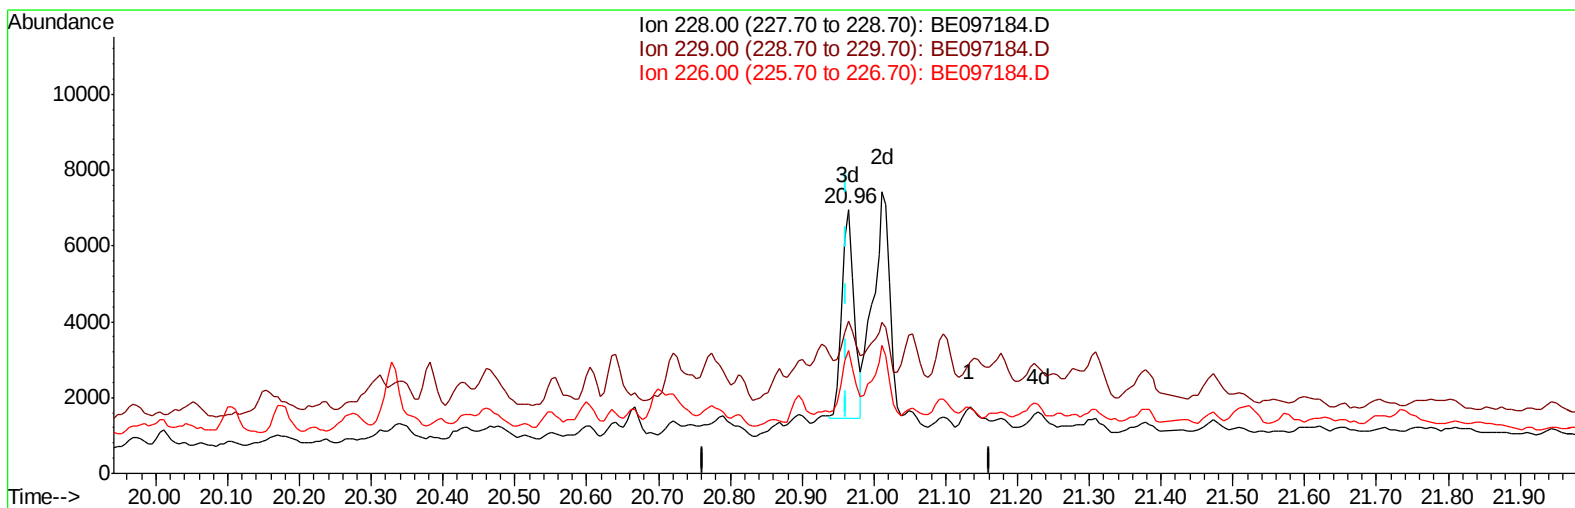

TIC: BE097184.D

(18) Benzo(a)anthracene

20.964min (+0.002) 0.17ng/ul m

response 6508

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	57.61#
226.00	21.30	46.52#
0.00	0.00	0.00