
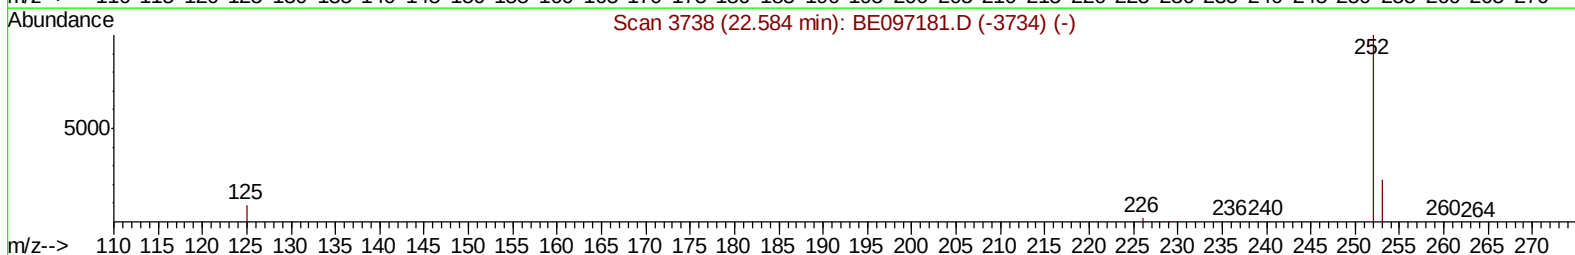
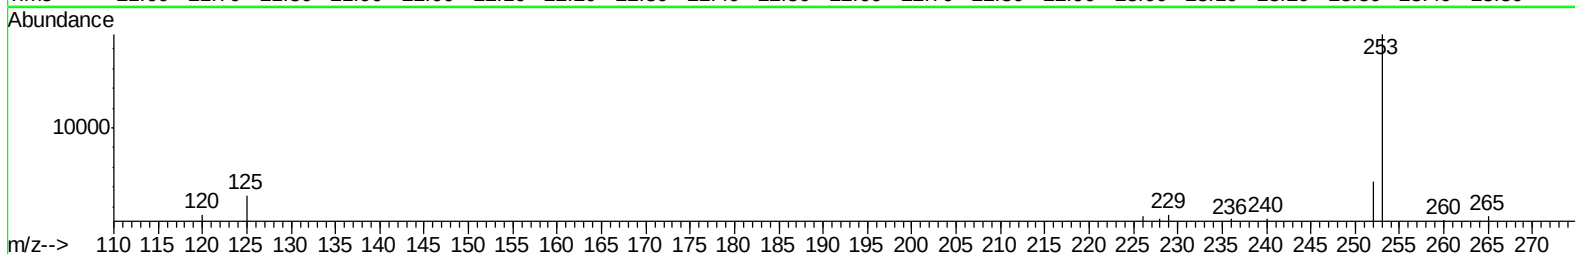


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097184.D
Acq On : 3 Aug 2018 18:00
Operator : SJ/JU
Sample : J4171-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 03 23:57:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

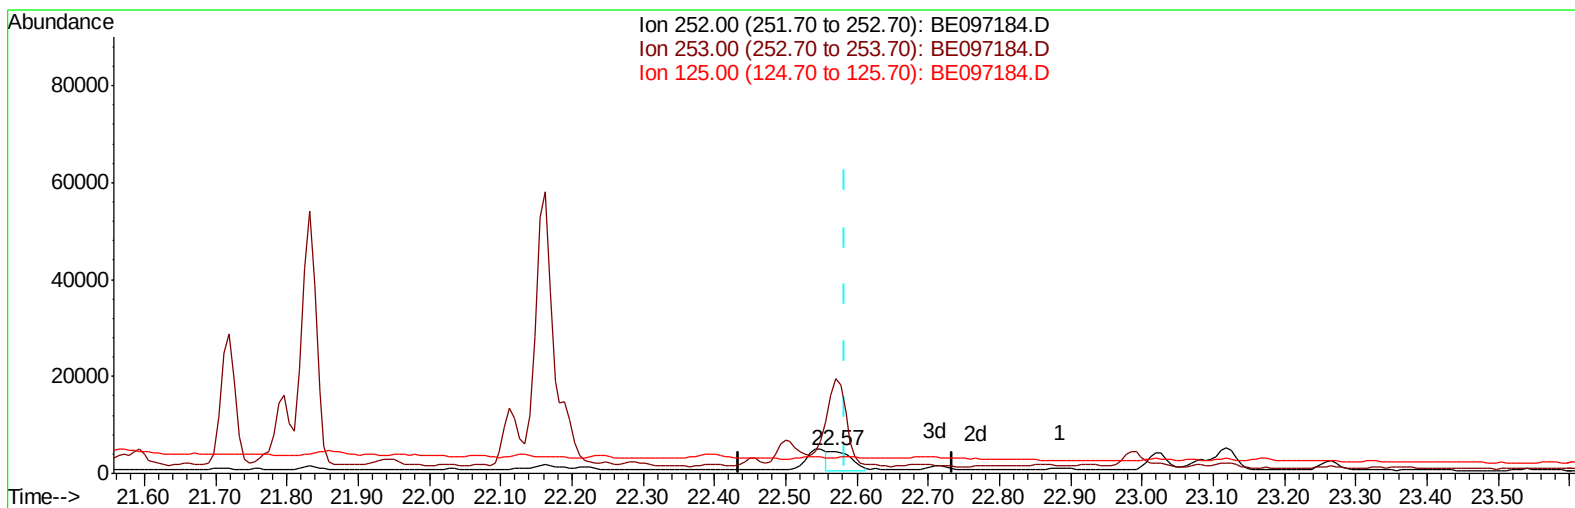

TIC: BE097184.D

(22) Benzo(k)fluoranthene

22.570min (-0.014) 0.25ng/ul m

response 8894

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	424.36#
125.00	17.10	69.79#
0.00	0.00	0.00