
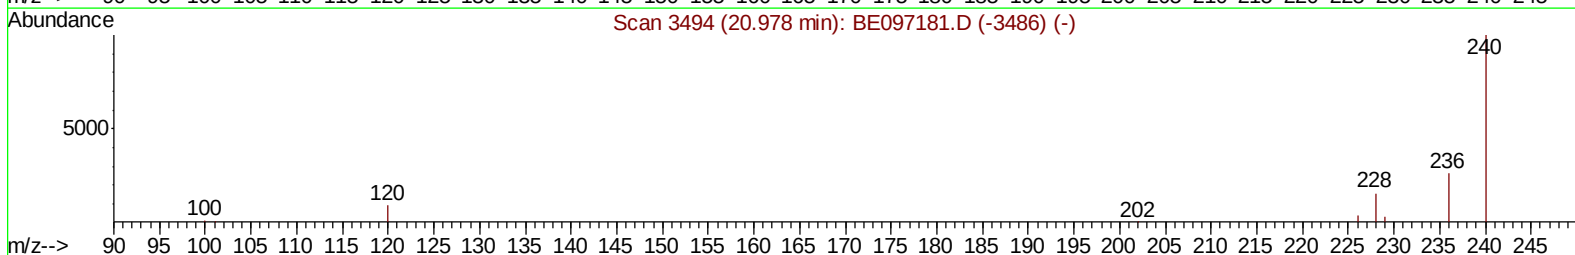
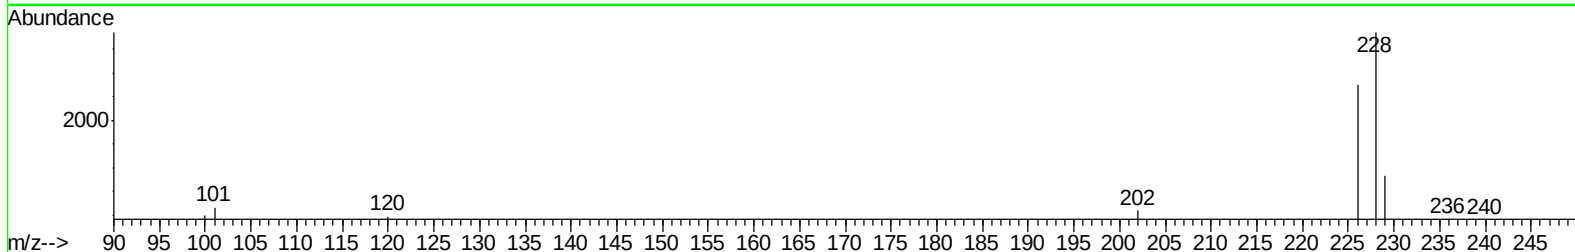


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
Data File : BE097185.D  
Acq On : 3 Aug 2018 18:38  
Operator : SJ/JU  
Sample : J4171-16  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 04 00:00:36 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 03 23:39:09 2018  
Response via : Initial Calibration

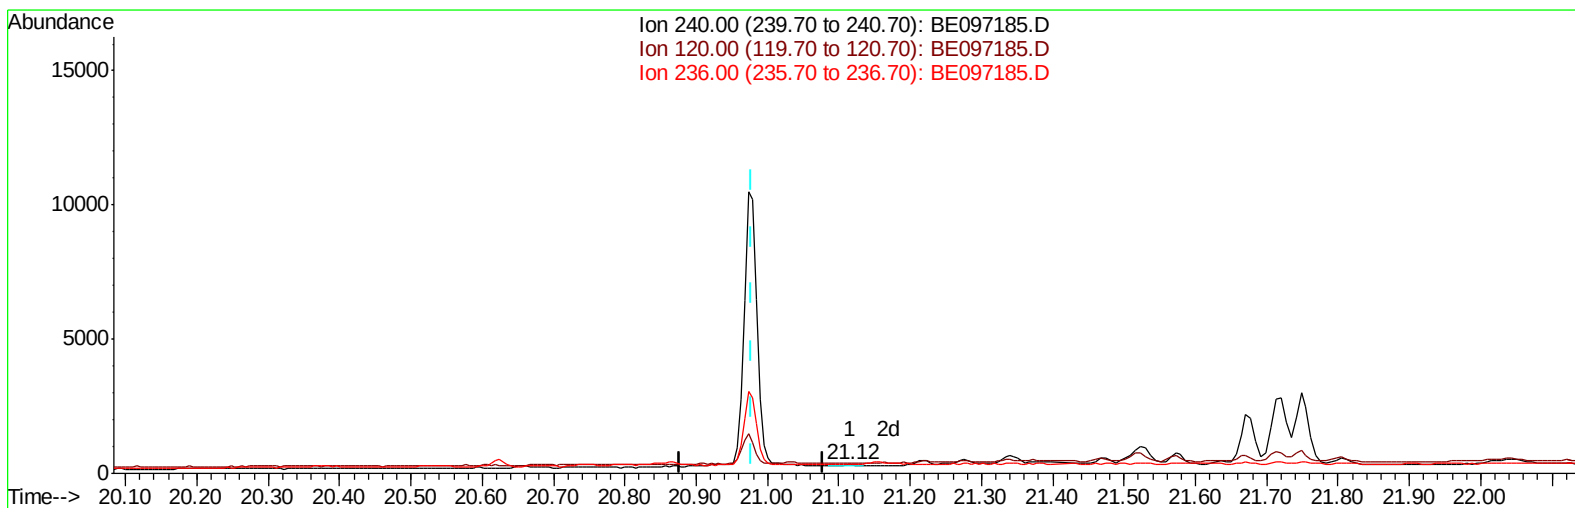

TIC: BE097185.D

(16) Chrysene-d12 (I)

21.117min (+0.139) 0.40ng/ul

response 81

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 240.00 | 100   | 100     |
| 120.00 | 20.60 | 114.98# |
| 236.00 | 34.90 | 101.22# |
| 0.00   | 0.00  | 0.00    |