
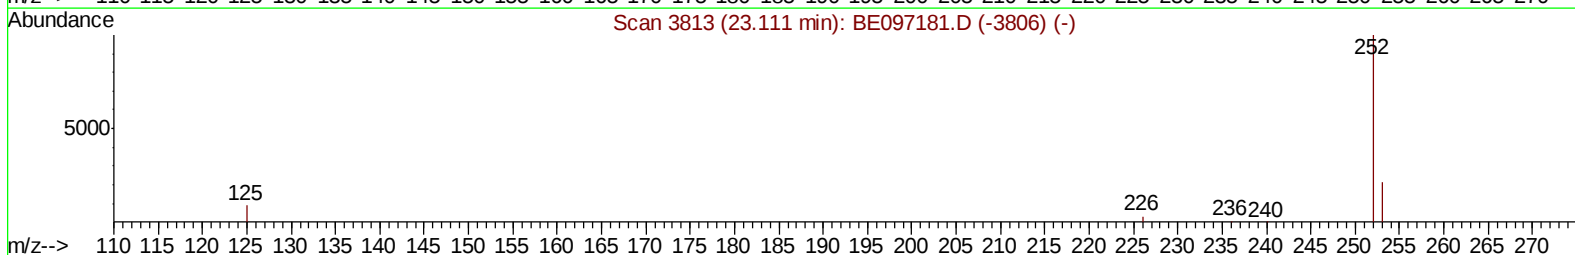
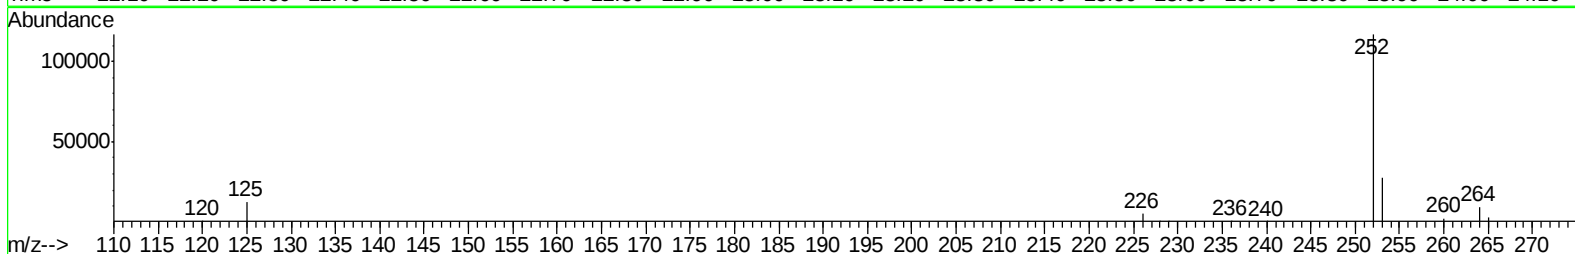


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097186.D
Acq On : 3 Aug 2018 19:17
Operator : SJ/JU
Sample : J4171-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 04 00:07:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

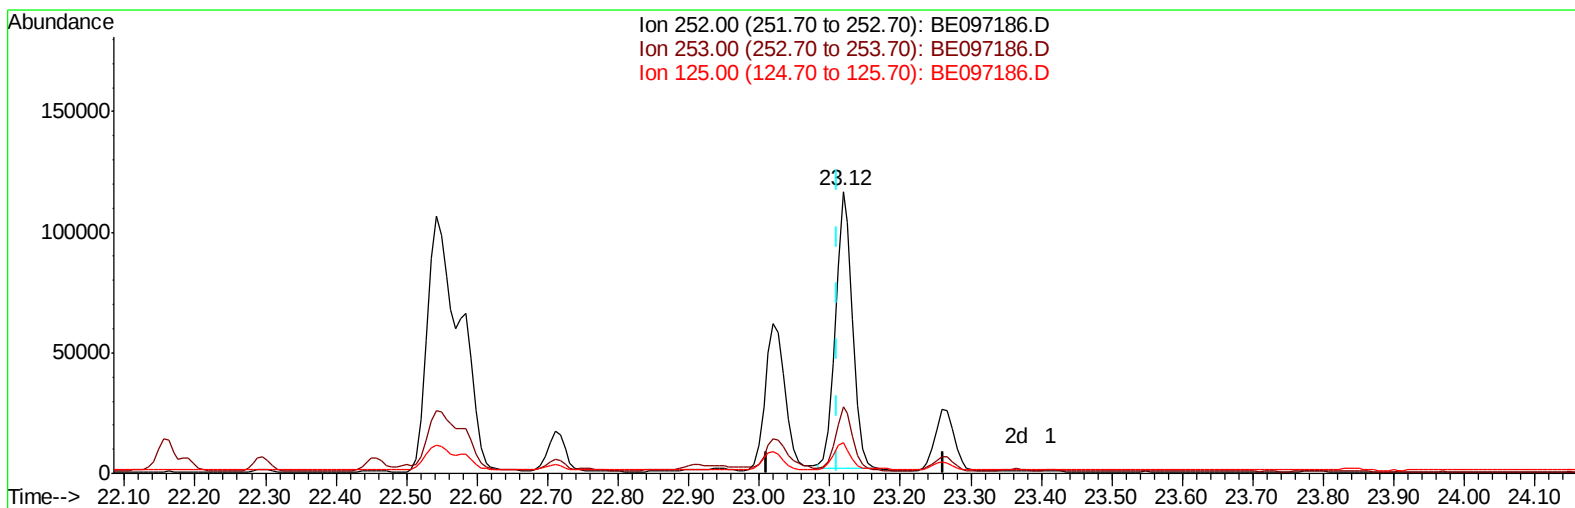

TIC: BE097186.D

(23) Benzo(a)pyrene (C)

23.119min (+0.007) 5.78ng/ul m

response 194472

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.43#
125.00	22.60	10.82#
0.00	0.00	0.00