
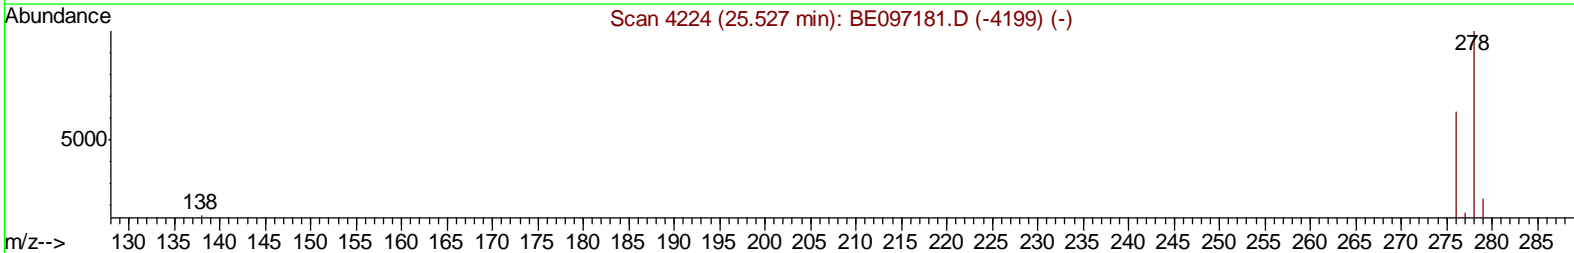
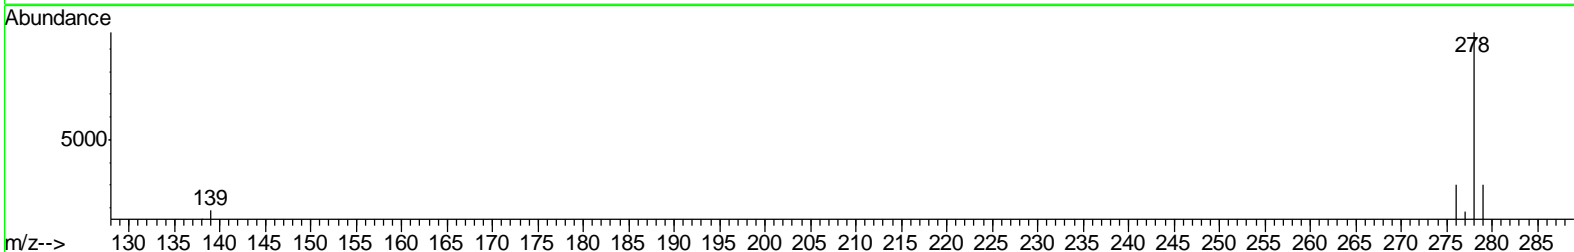


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097186.D
 Acq On : 3 Aug 2018 19:17
 Operator : SJ/JU
 Sample : J4171-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 04 00:07:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration

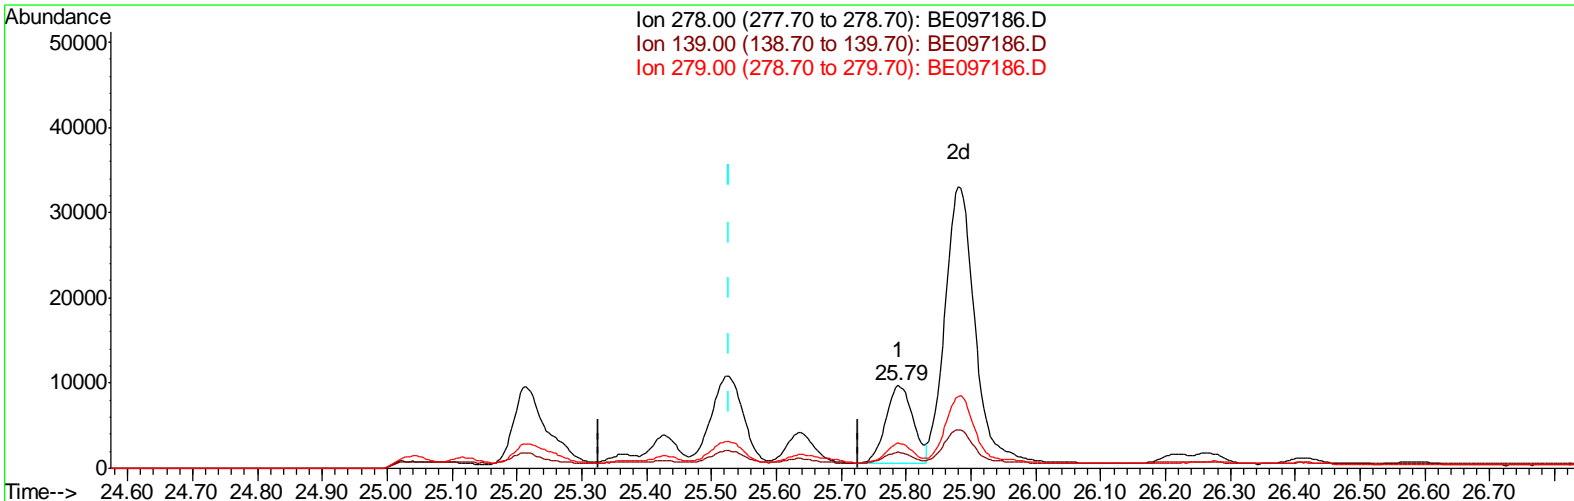

TIC: BE097186.D

(25) Dibenzo(a,h)anthracene

25.788min (+0.260) 0.78ng/ul

response 27038

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	19.35
279.00	32.40	30.77
0.00	0.00	0.00