
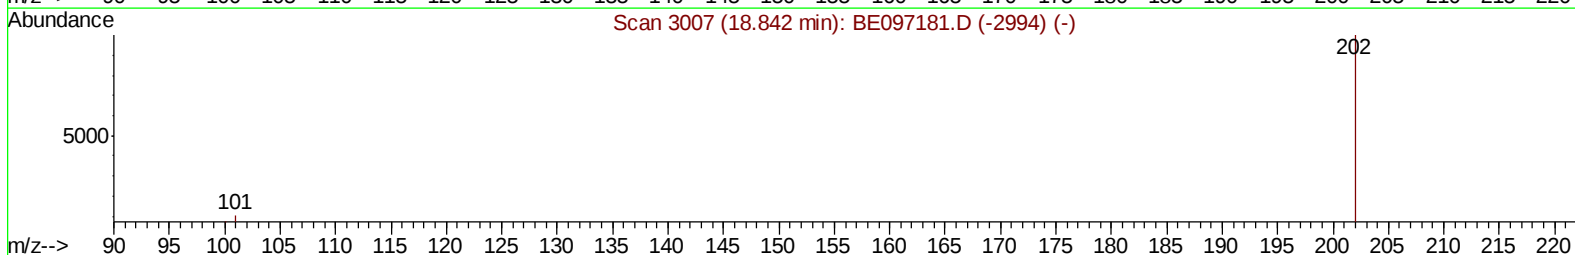
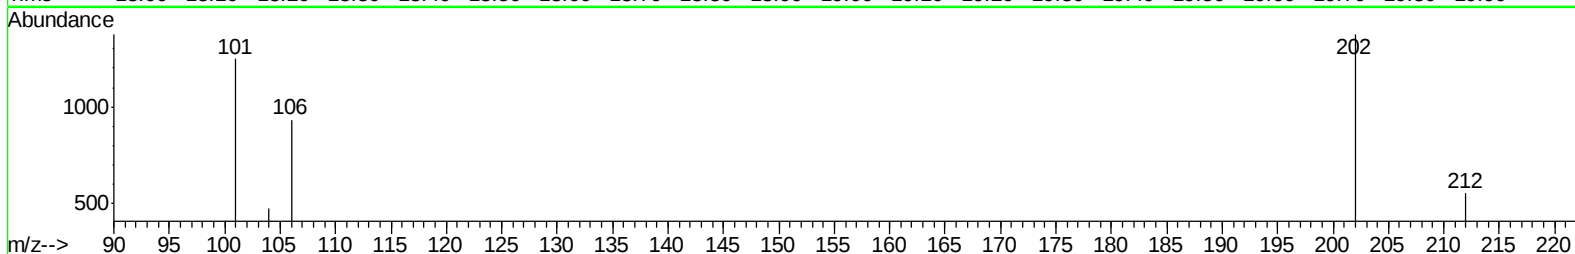


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097187.D
Acq On : 3 Aug 2018 19:53
Operator : SJ/JU
Sample : J4171-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 04 00:10:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

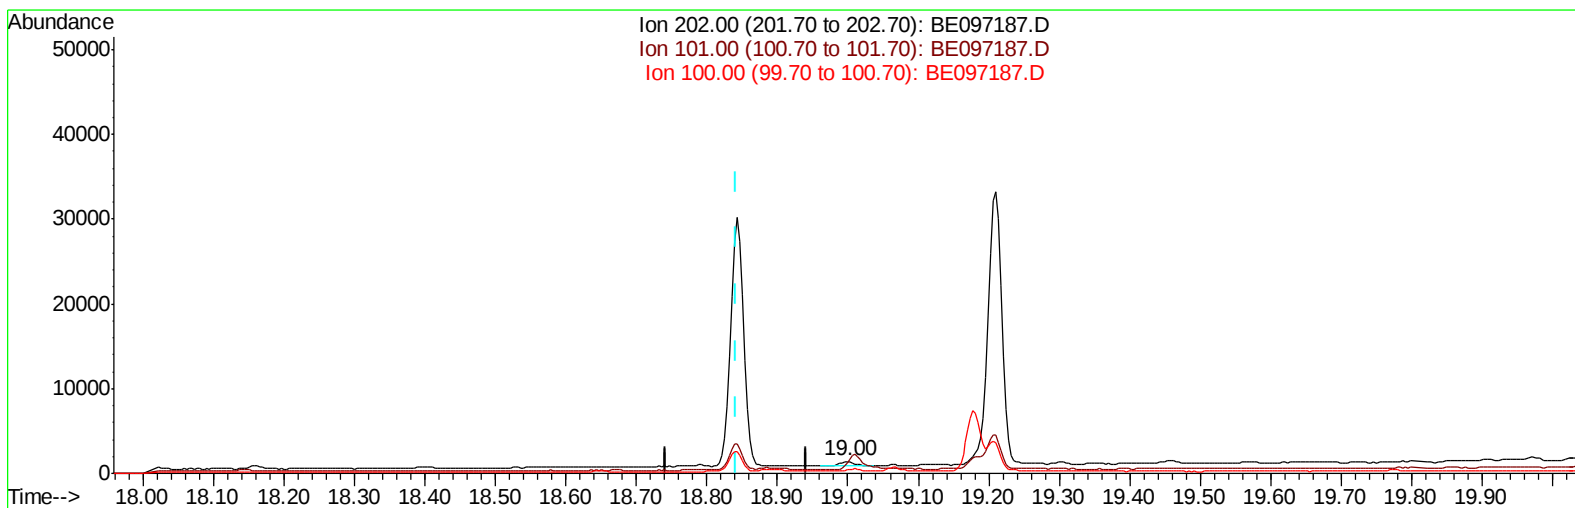

TIC: BE097187.D

(15) Fluoranthene (C)

19.000min (+0.157) 0.02ng/ul

response 879

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	90.68#
100.00	19.50	29.84
0.00	0.00	0.00