
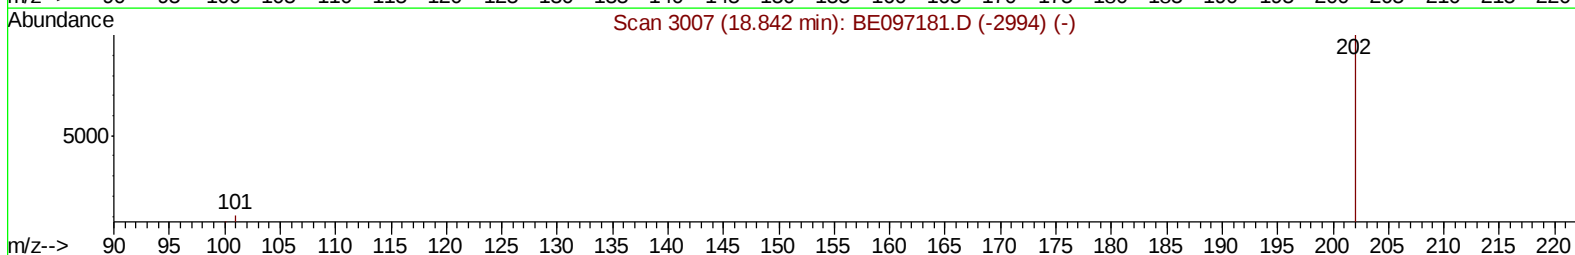
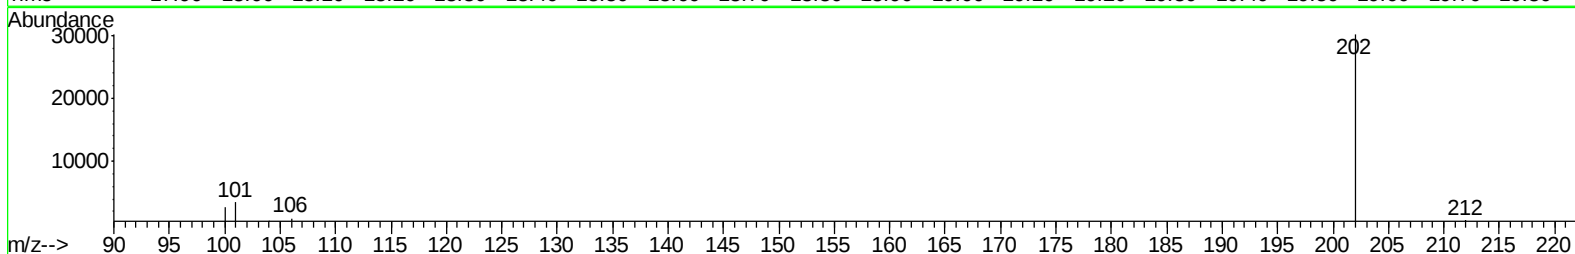


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
Data File : BE097187.D  
Acq On : 3 Aug 2018 19:53  
Operator : SJ/JU  
Sample : J4171-18  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 04 00:10:02 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 03 23:39:09 2018  
Response via : Initial Calibration

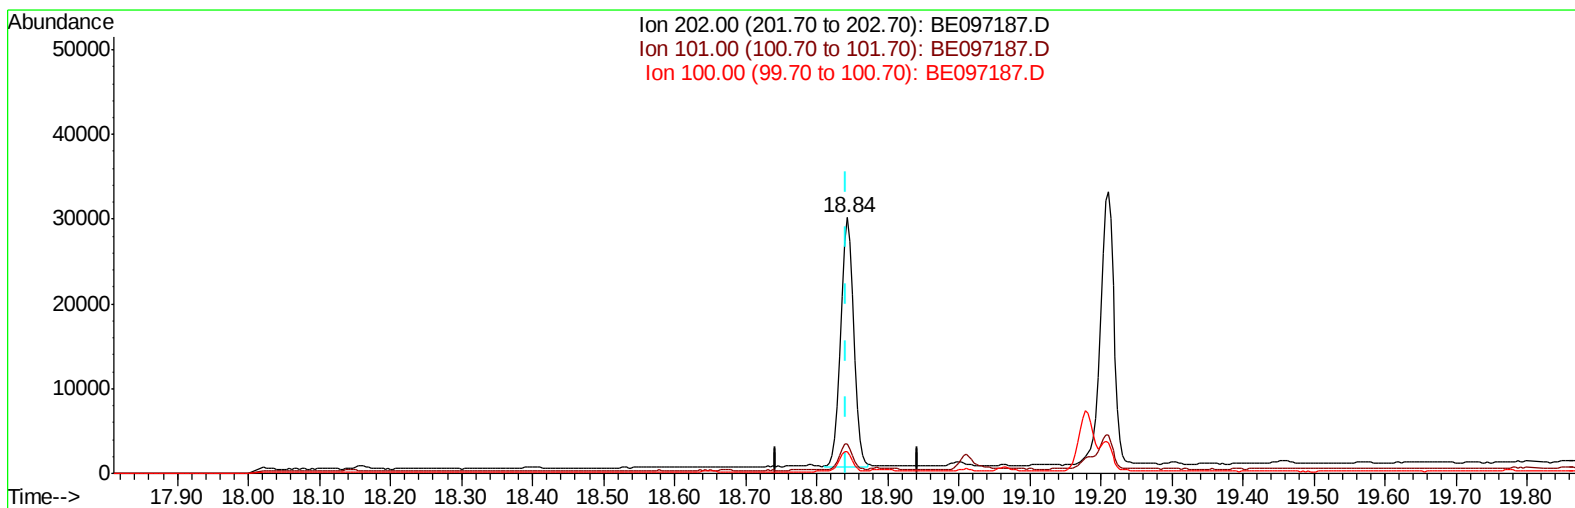

TIC: BE097187.D

(15) Fluoranthene (C)

18.843min (+0.000) 0.97ng/ul m

response 37231

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 202.00 | 100   | 100   |
| 101.00 | 10.30 | 11.50 |
| 100.00 | 19.50 | 8.64  |
| 0.00   | 0.00  | 0.00  |