
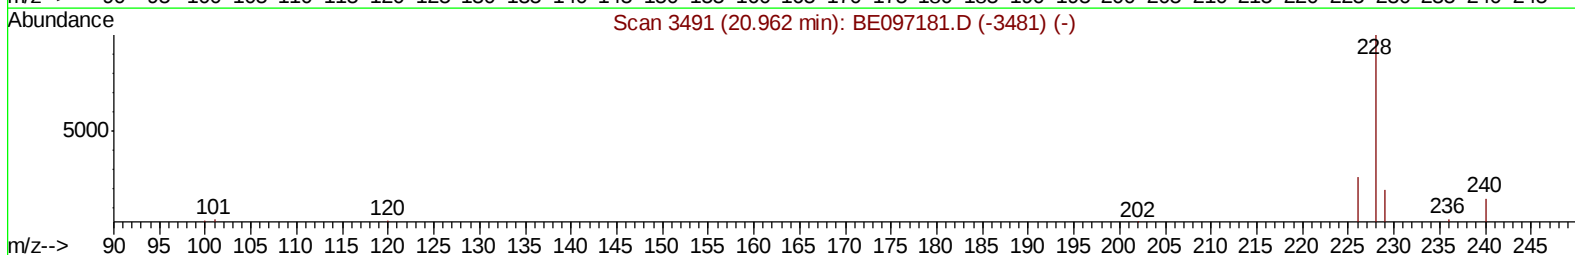
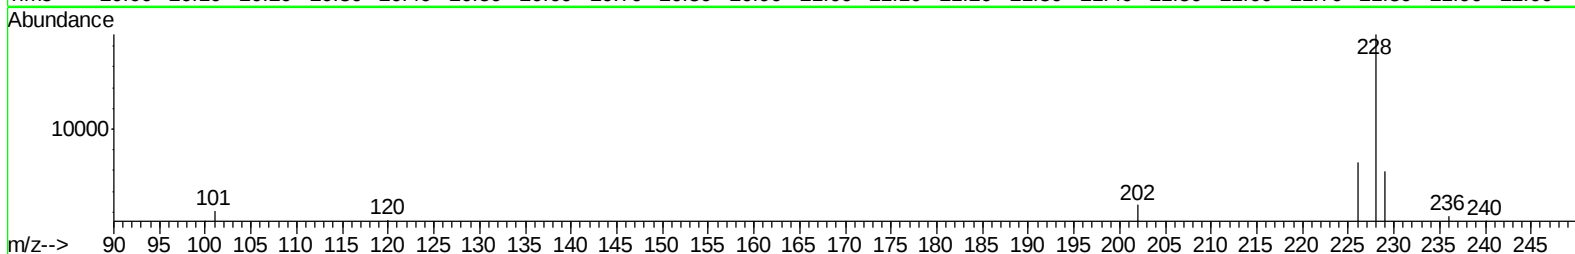


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097187.D
Acq On : 3 Aug 2018 19:53
Operator : SJ/JU
Sample : J4171-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 04 00:11:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

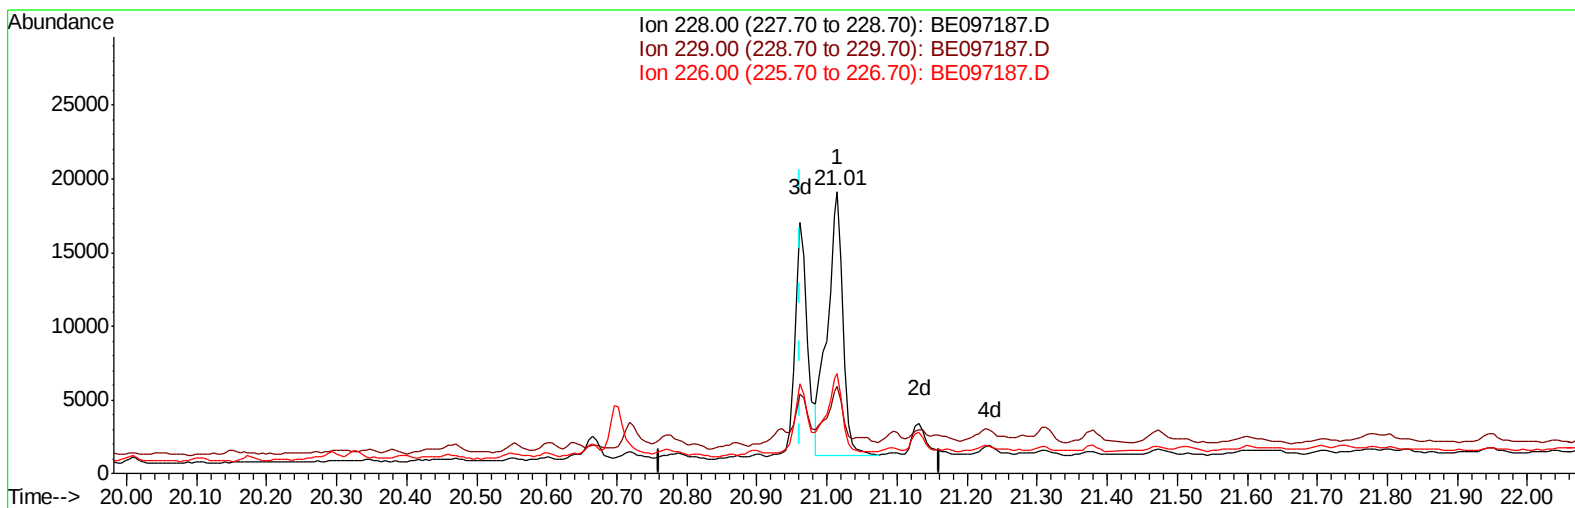

TIC: BE097187.D

(18) Benzo(a)anthracene
21.015min (+0.053) 0.85ng/ul
response 28314

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	30.78
226.00	21.30	35.31#
0.00	0.00	0.00