
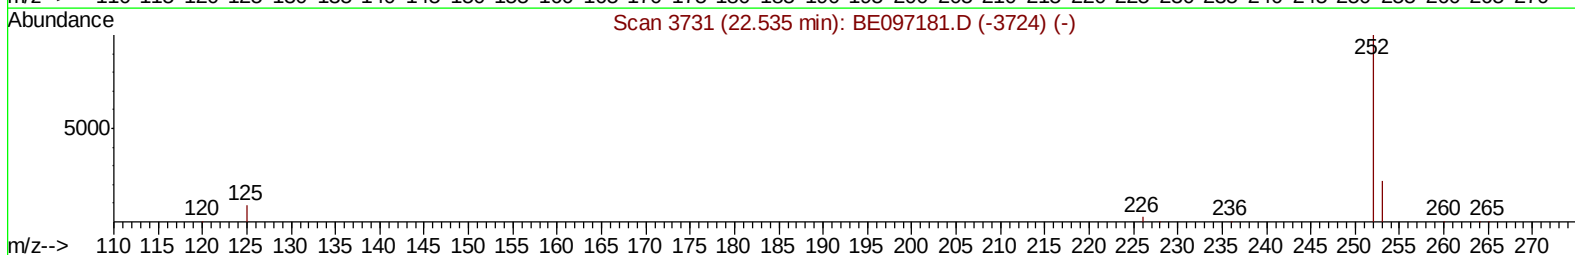
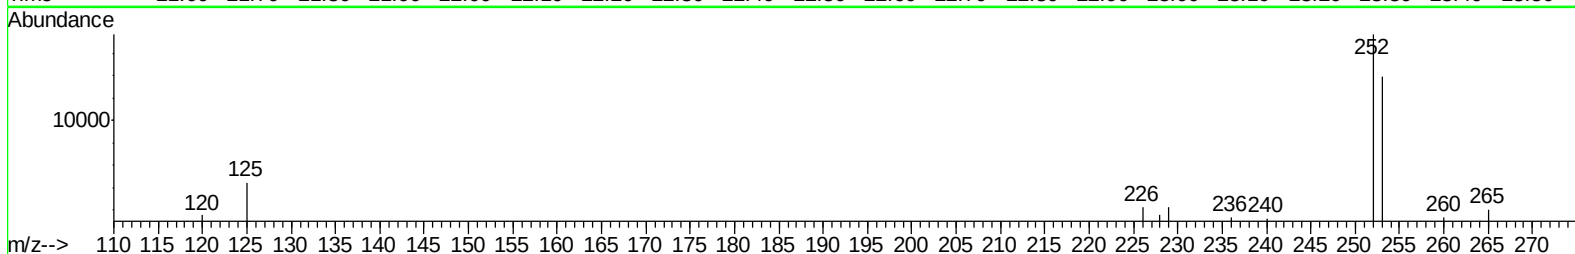


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
Data File : BE097187.D  
Acq On : 3 Aug 2018 19:53  
Operator : SJ/JU  
Sample : J4171-18  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 04 00:12:31 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 03 23:39:09 2018  
Response via : Initial Calibration

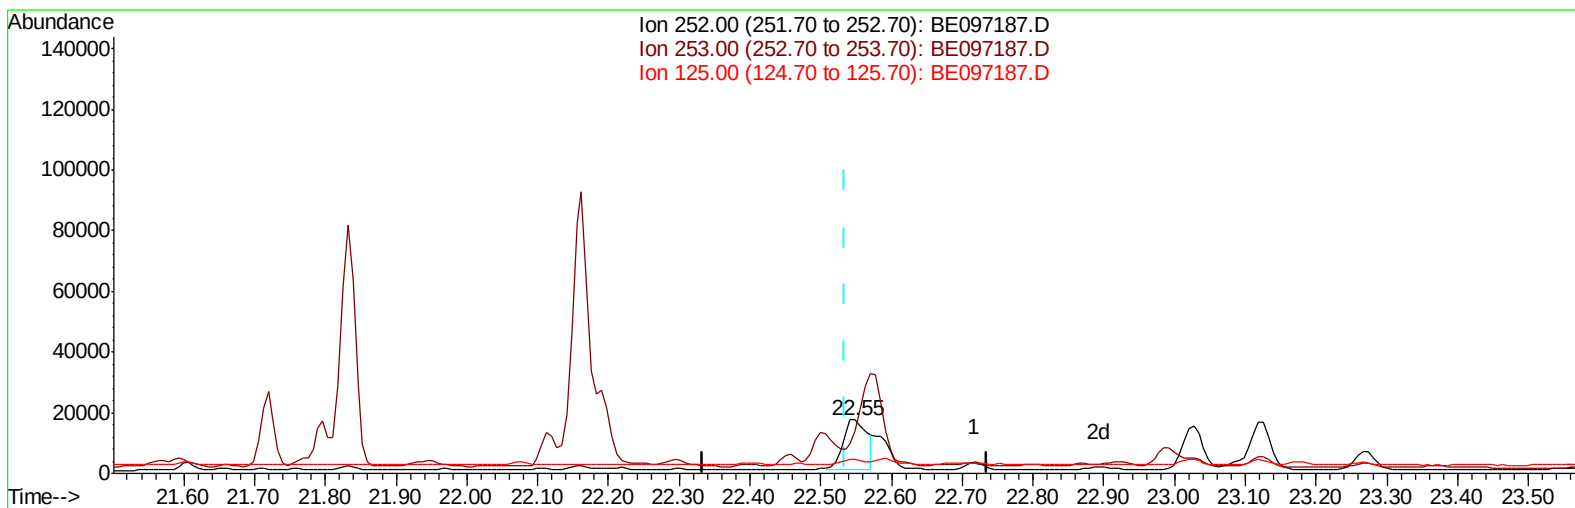

TIC: BE097187.D

(21) Benzo(b)fluoranthene

22.549min (+0.014) 1.26ng/ul m

response 39056

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 32.10 | 78.56# |
| 125.00 | 17.50 | 25.22  |
| 0.00   | 0.00  | 0.00   |