
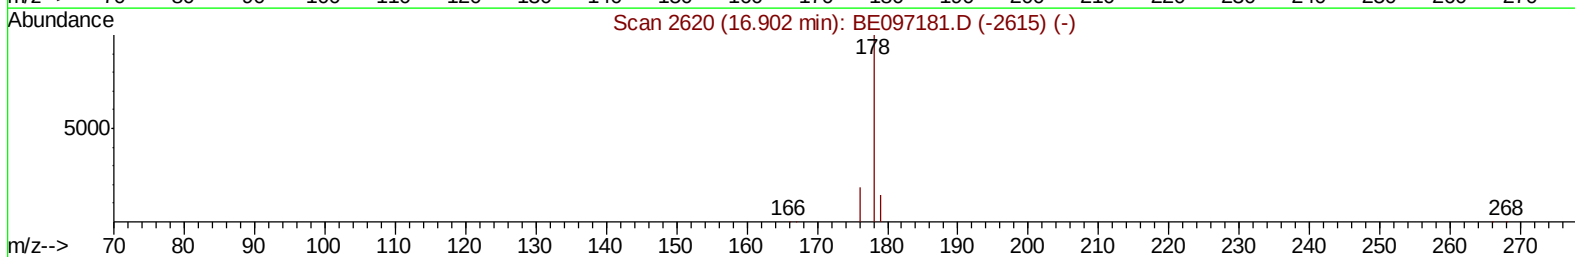
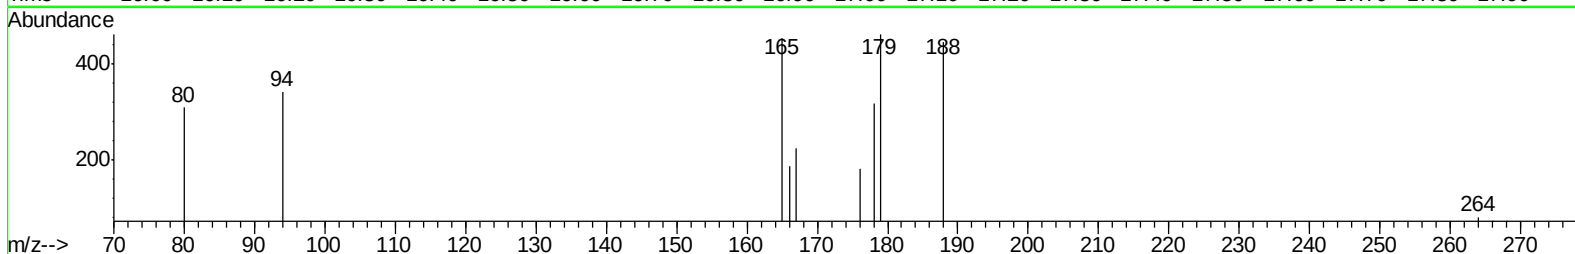


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\  
Data File : BE097188.D  
Acq On : 3 Aug 2018 20:32  
Operator : SJ/JU  
Sample : J4171-07  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 00:15:51 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 03 23:39:09 2018  
Response via : Initial Calibration

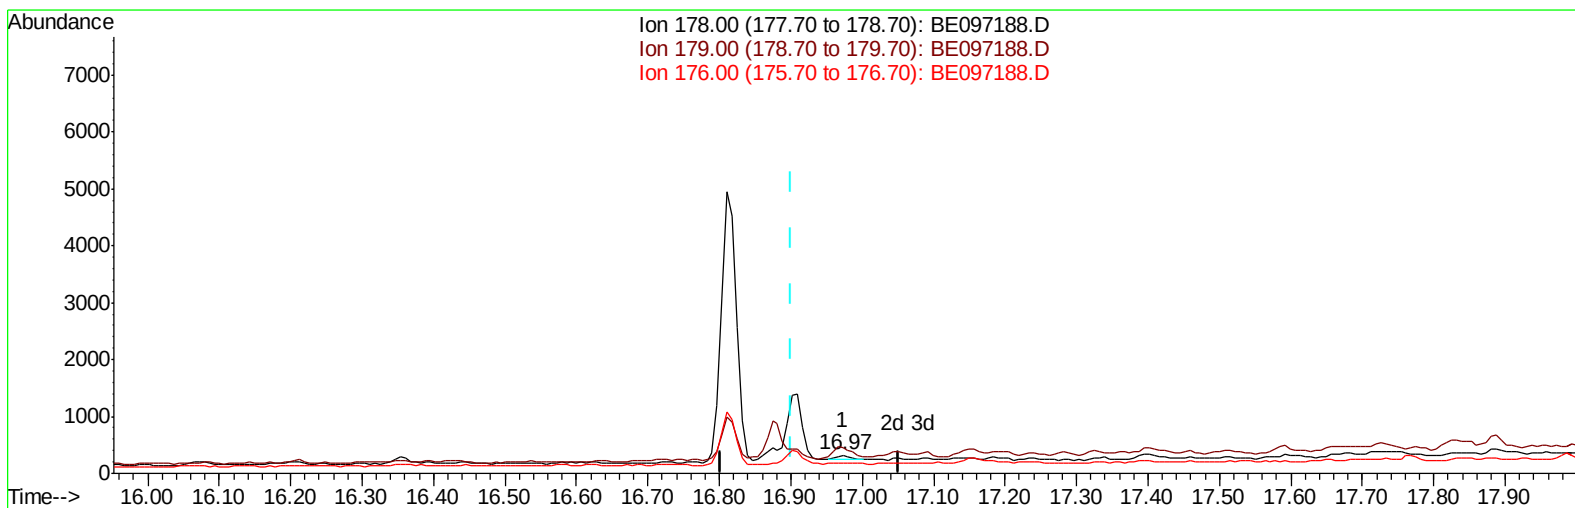

TIC: BE097188.D

(13) Anthracene

16.973min (+0.071) 0.00ng/ul

response 110

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 178.00 | 100   | 100     |
| 179.00 | 22.60 | 145.43# |
| 176.00 | 18.40 | 56.78#  |
| 0.00   | 0.00  | 0.00    |