
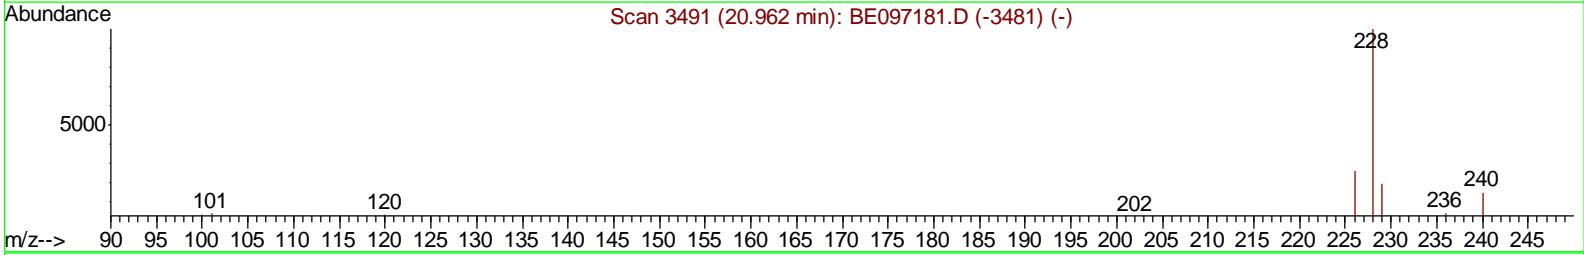
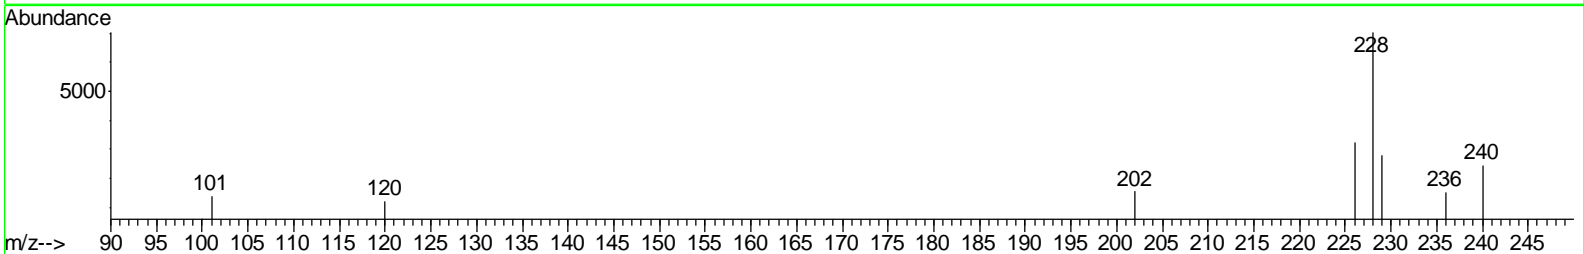


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097188.D
 Acq On : 3 Aug 2018 20:32
 Operator : SJ/JU
 Sample : J4171-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 00:17:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration

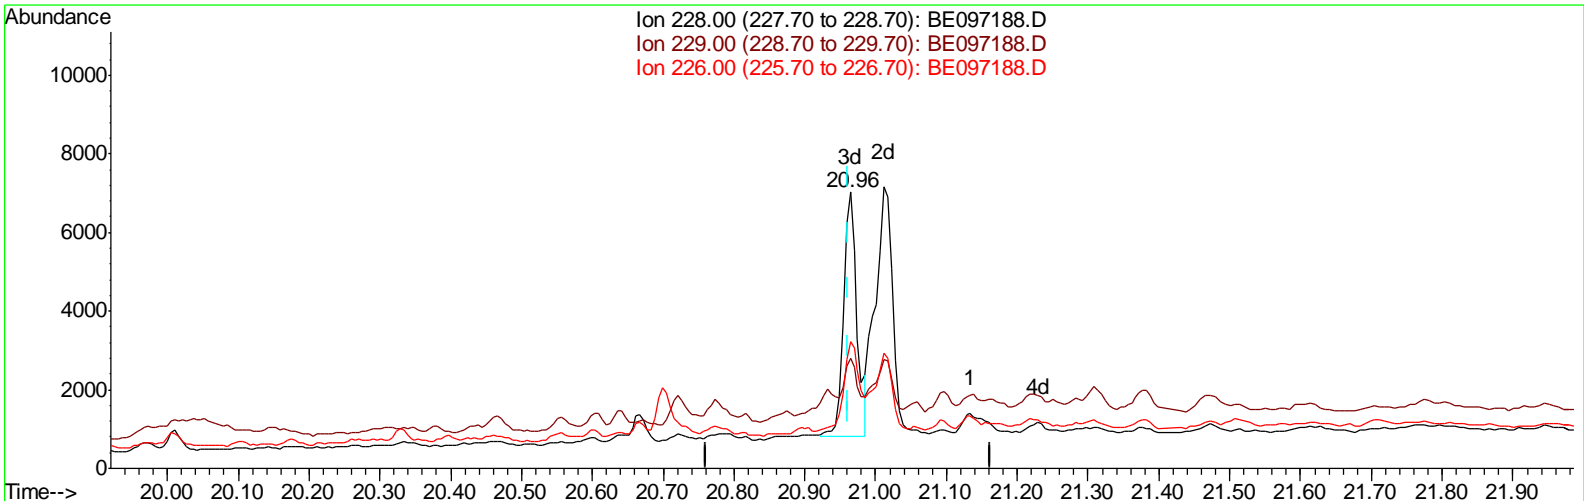

TIC: BE097188.D

(18) Benzo(a)anthracene
 20.964min (+0.002) 0.22ng/ul m
 response 8362

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	39.92#
226.00	21.30	45.80#
0.00	0.00	0.00