
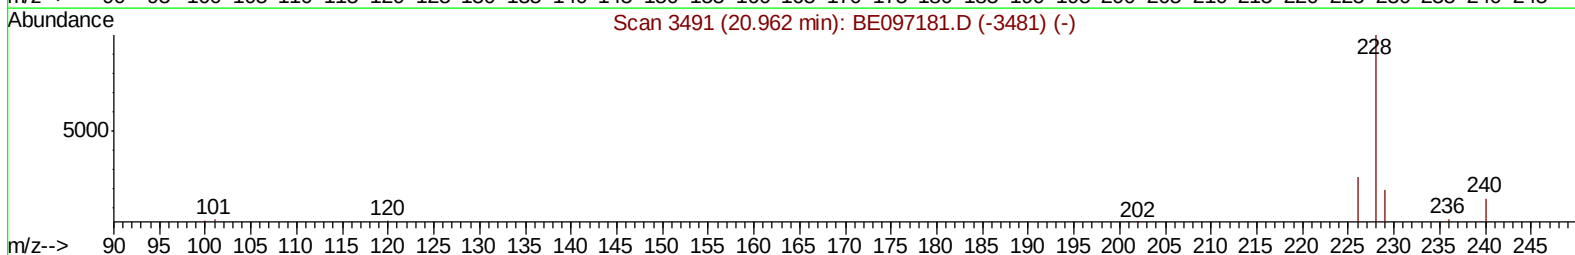
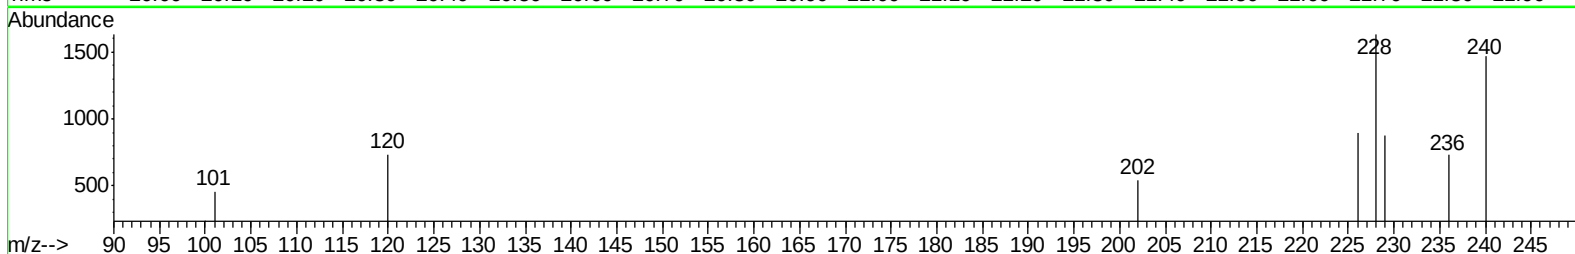


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097189.D
 Acq On : 3 Aug 2018 21:08
 Operator : SJ/JU
 Sample : J4171-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 04 00:22:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration

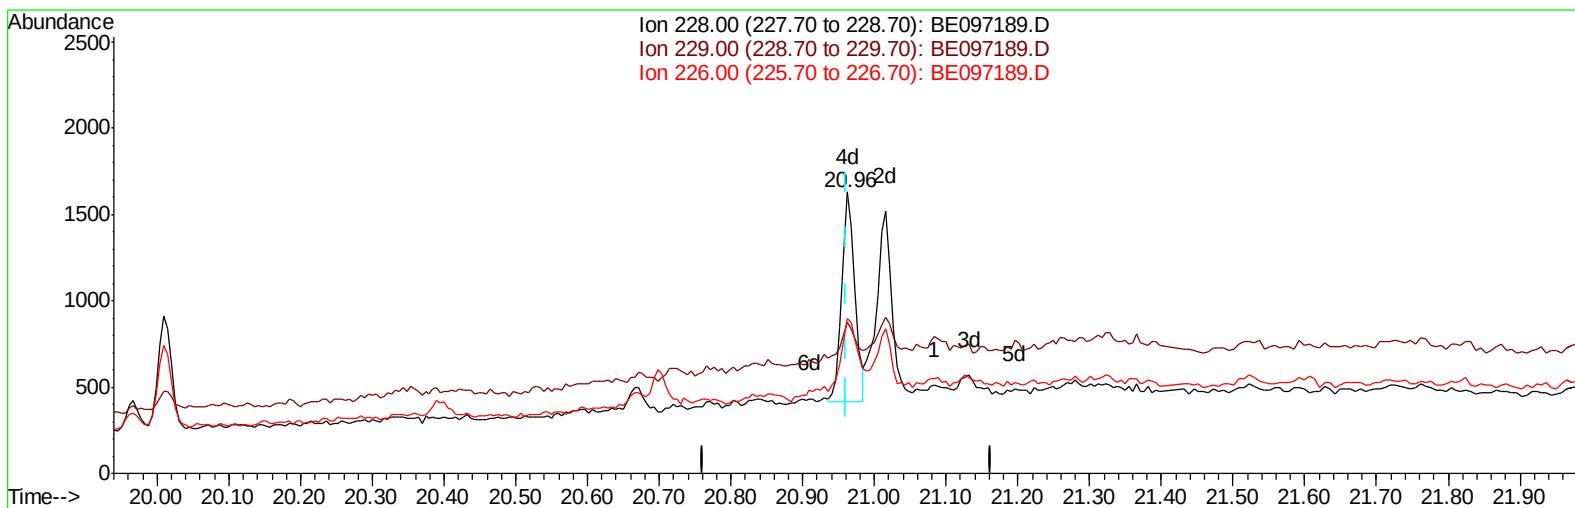

TIC: BE097189.D

(18) Benzo(a)anthracene

20.962min (+0.000) 0.04ng/ul m

response 1522

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	53.62#
226.00	21.30	54.84#
0.00	0.00	0.00