
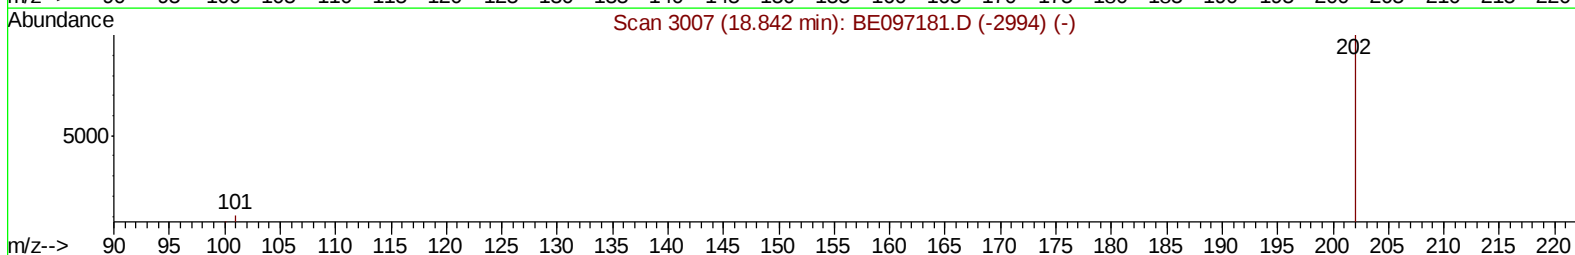
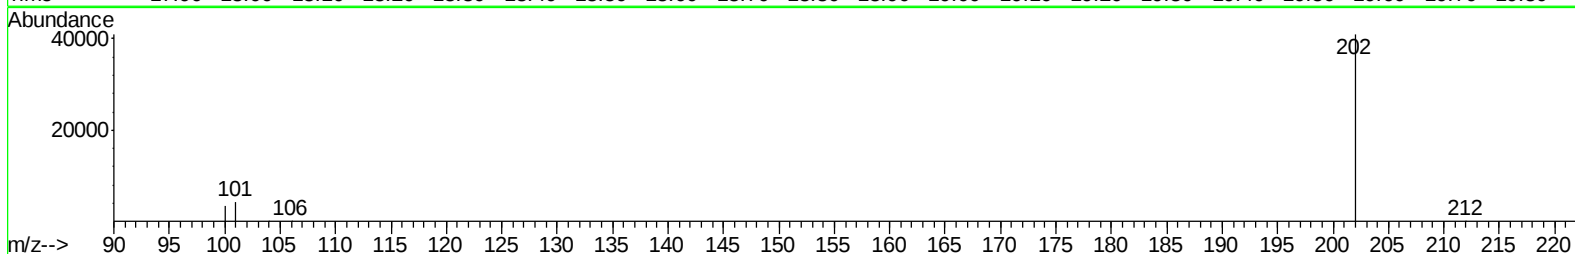


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097190.D
Acq On : 3 Aug 2018 21:47
Operator : SJ/JU
Sample : J4171-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Aug 04 00:26:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

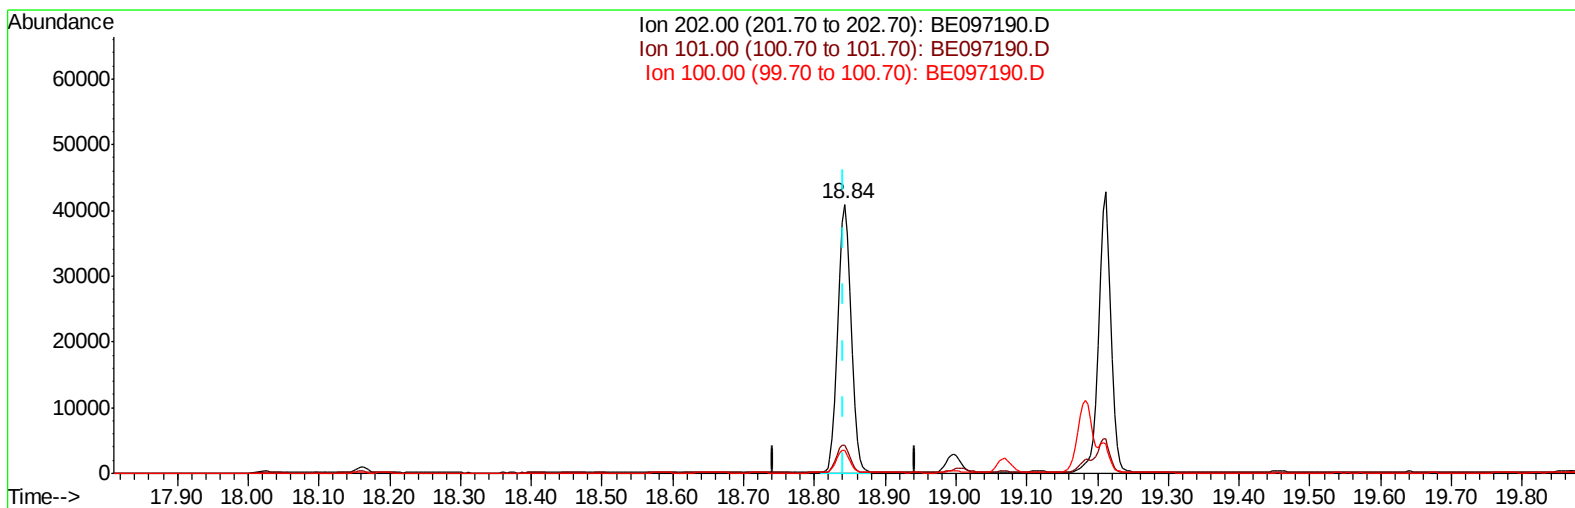

TIC: BE097190.D

(15) Fluoranthene (C)

18.843min (+0.001) 1.42ng/ul m

response 53108

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.66
100.00	19.50	8.42
0.00	0.00	0.00