
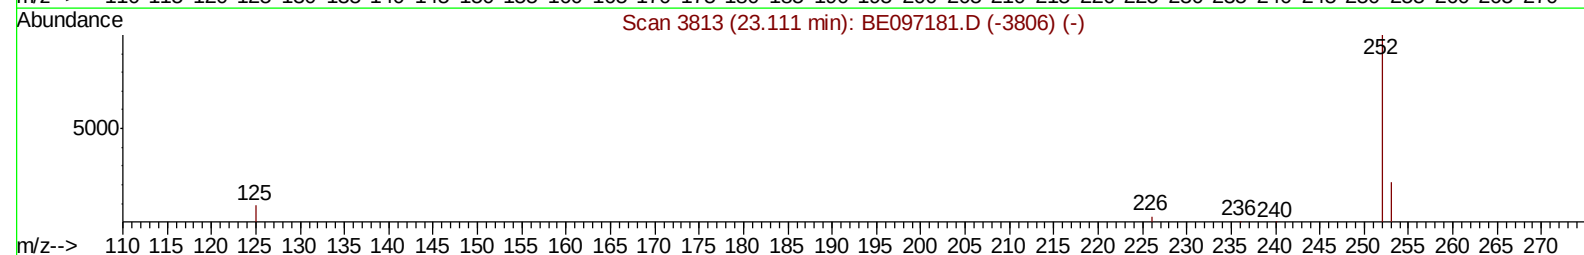
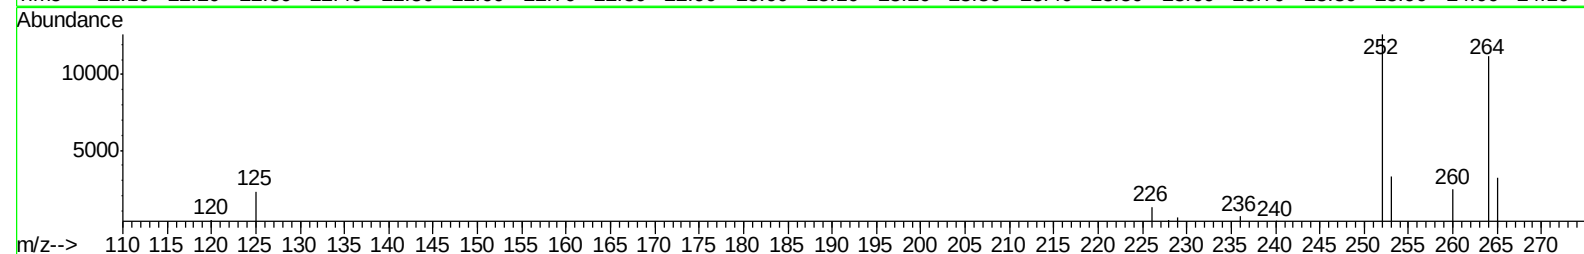


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097190.D
Acq On : 3 Aug 2018 21:47
Operator : SJ/JU
Sample : J4171-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Aug 04 00:28:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

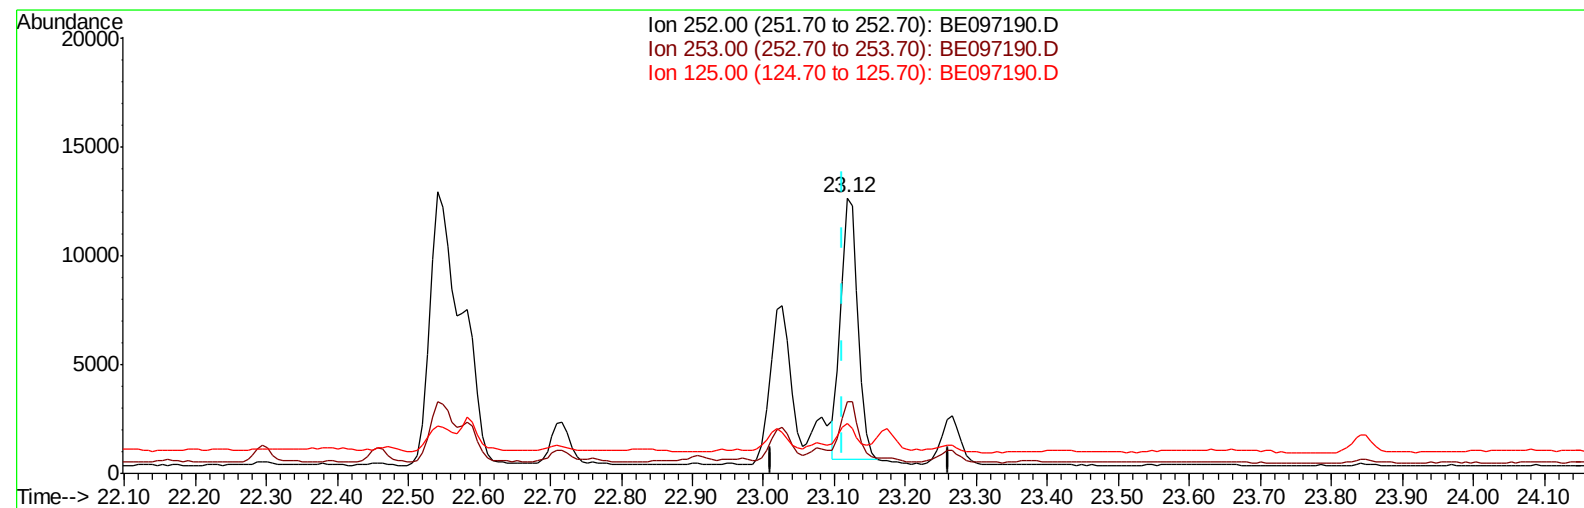

TIC: BE097190.D

(23) Benzo(a)pyrene (C)

23.117min (+0.006) 0.67ng/ul m

response 20548

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	26.07#
125.00	22.60	17.93#
0.00	0.00	0.00